

Data File : VW011422.D
Acq On : 22 Jul 2019 16:14
Operator : SY/VA
Sample : VW0722SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK10

Quant Time: Jul 23 04:58:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 23 04:55:51 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	448763	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	403452	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	187787	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	146847	24.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.04%
7) Chloroethane-d5	2.89	69	106263	24.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.40%
10) 1,1-Dichloroethene-d2	4.02	63	248895	18.34	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.36%
20) 2-Butanone-d5	7.07	46	134072	52.55	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.10%
24) Chloroform-d	7.65	84	283728	24.69	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.76%
26) 1,2-Dichloroethane-d4	8.31	65	176745	25.87	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.48%
29) Benzene-d6	8.27	84	604460	25.05	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.20%
33) 1,2-Dichloropropane-d6	9.27	67	197027	25.20	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.80%
37) Toluene-d8	10.32	98	534606	24.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.88%
38) trans-1,3-Dichloropropene-	10.58	79	83780	24.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.24%
39) 2-Hexanone-d5	10.93	63	90887	53.62	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.24%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	160502	25.69	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.76%
61) 1,2-Dichlorobenzene-d4	13.85	152	177524	25.18	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.72%


Target Compounds					Qvalue
13) Acetone	4.12	43	4112	1.524 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011422.D
Acq On : 22 Jul 2019 16:14
Operator : SY/VA
Sample : VW0722SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK10

Quant Time: Jul 23 04:58:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 23 04:55:51 2019
Response via : Initial Calibration

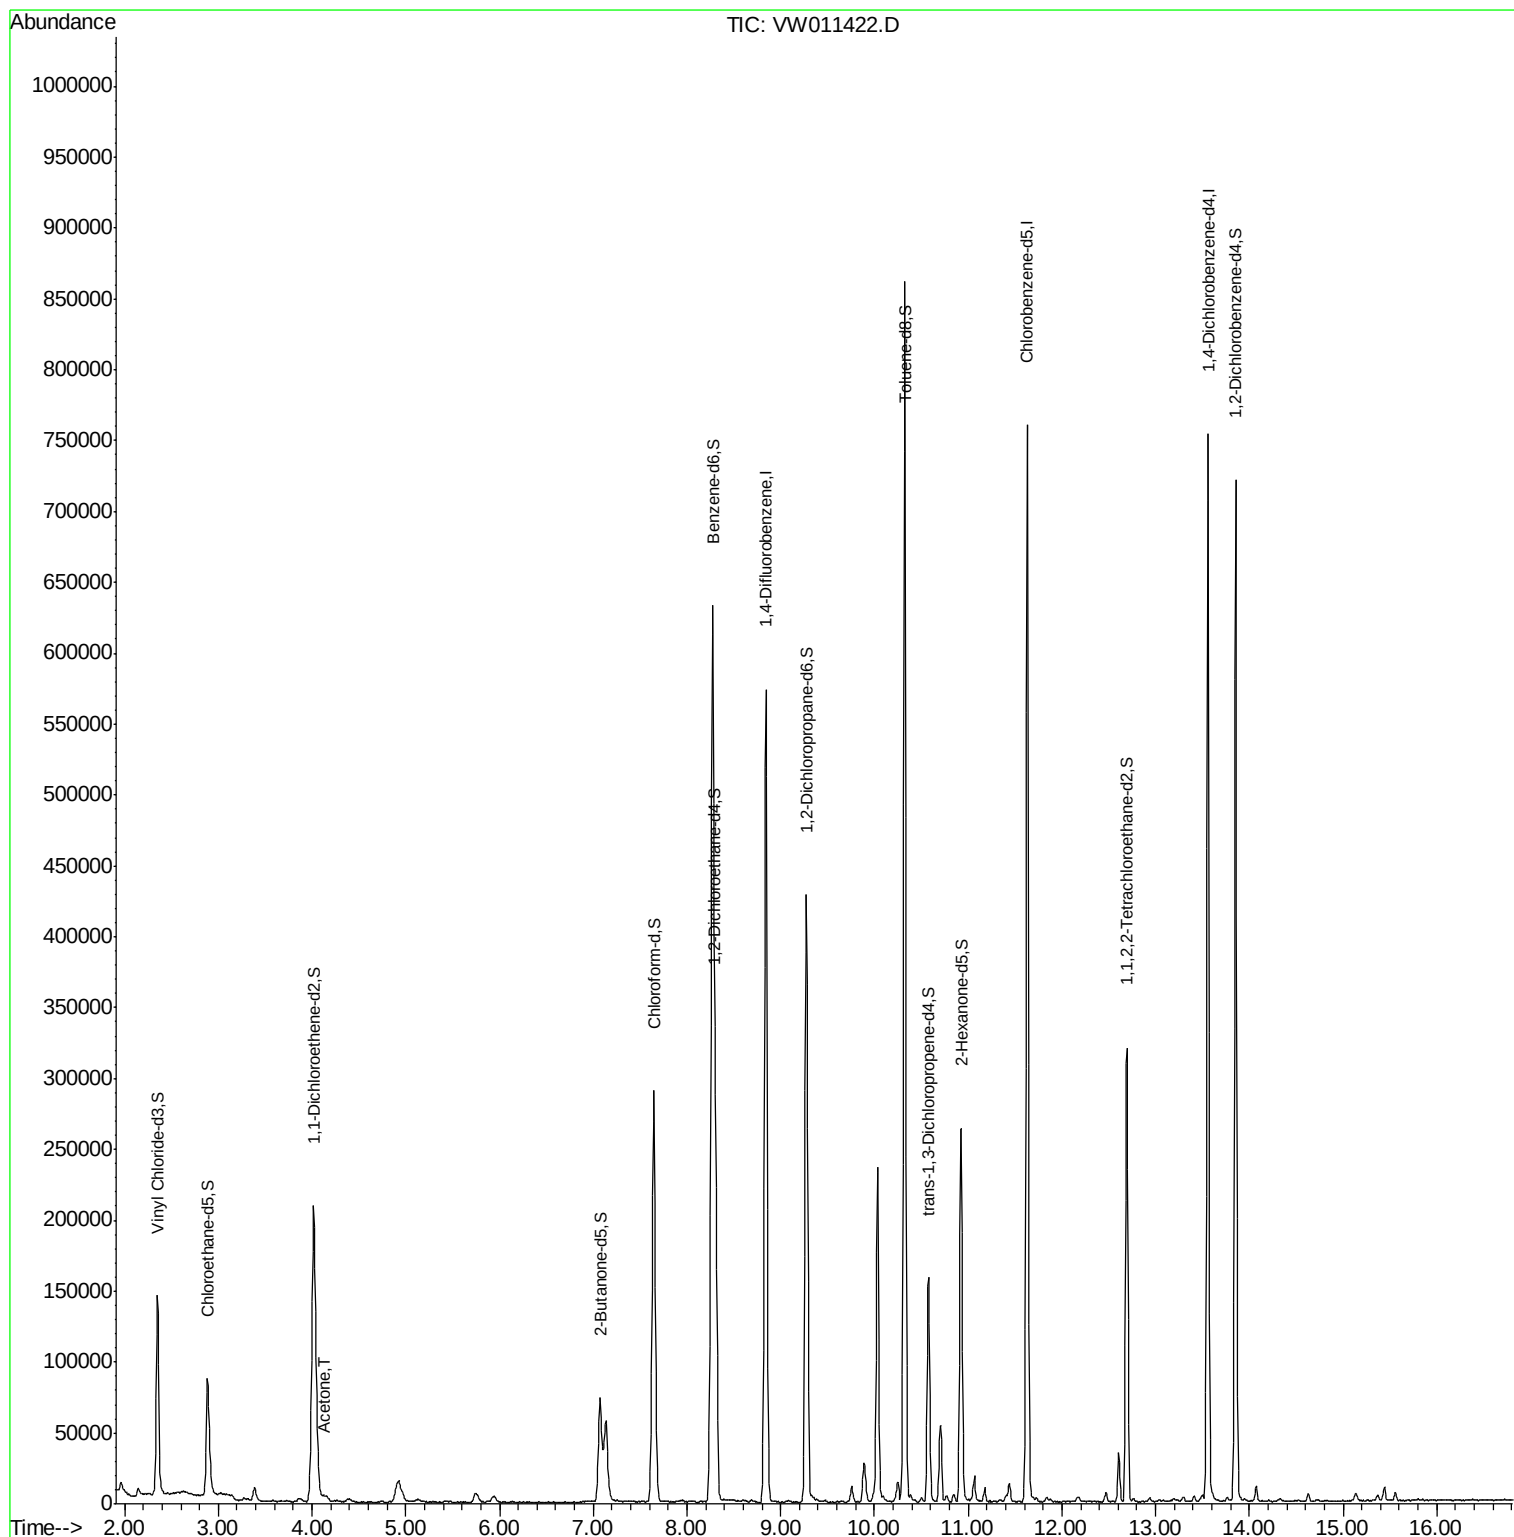

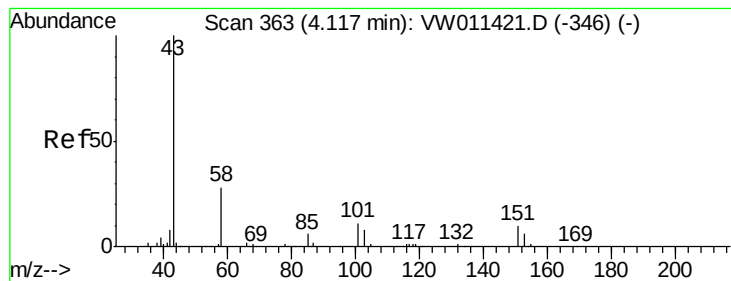

#13

Acetone

Concen: 1.524 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW011422.D

Acq: 22 Jul 2019 16:14

Instrument :

MSVOA_W

ClientSampleId :

VBLK10

Tgt Ion: 43 Resp: 4112

Ion Ratio Lower Upper

43 100

58 16.1 0.0 57.2

