


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW072219\
Data File : VW011413.D
Acq On : 22 Jul 2019 09:42
Operator : SY/VA
Sample : BFB30
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB30

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
Title : VOC Analysis
Last Update : Wed Jul 24 01:19:38 2019

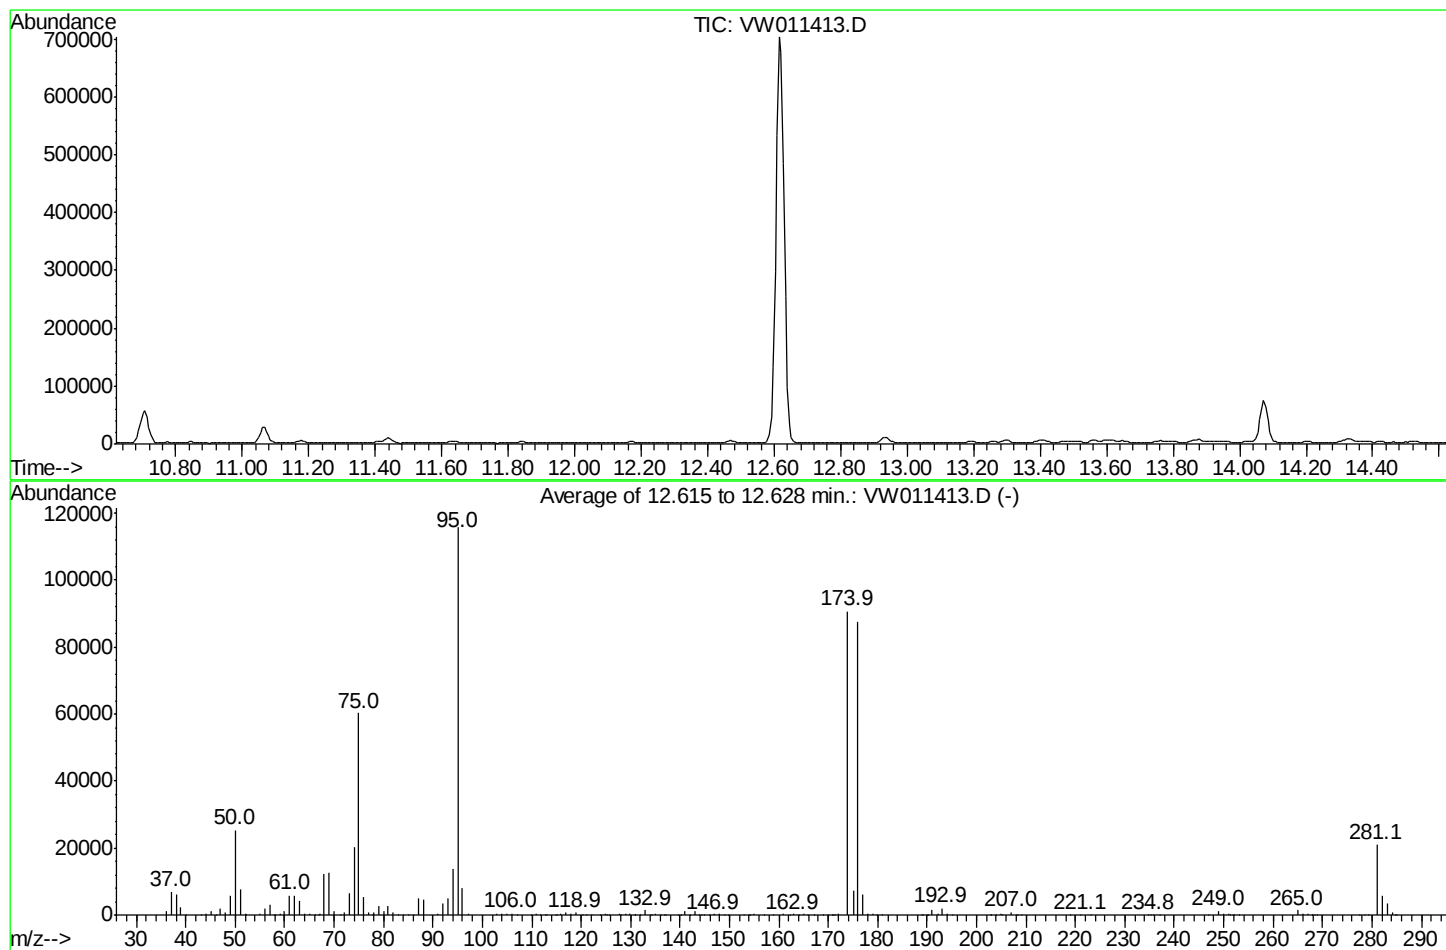

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	25381	PASS
75	95	30	80	52.1	60293	PASS
95	95	100	100	100.0	115773	PASS
96	95	5	9	6.9	7944	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.3	90637	PASS
175	174	5	9	8.0	7222	PASS
176	174	95	101	96.4	87370	PASS
177	176	5	9	7.0	6133	PASS

Scan 1749 (12.567 min): VW011413.D
BFB30

m/z	Abundance
35.90	65.0
39.00	153.0
40.00	475.0
41.10	168.0
41.90	125.0
43.10	140.0
44.00	453.0
47.80	83.0
55.00	62.0
55.90	92.0
57.10	215.0
69.00	57.0
133.20	62.0
207.20	117.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

m/z	Abundance
36.00	1573.0
37.10	8200.0
38.00	6806.0
39.00	3220.0
39.90	521.0
41.10	128.0
42.10	97.0
43.00	235.0
44.00	1159.0
45.00	1633.0
46.00	184.0
47.10	2009.0
48.10	897.0
49.00	5998.0
50.00	29784.0
51.00	9554.0
52.00	410.0
55.10	381.0
56.00	2006.0
57.00	3737.0
58.00	209.0
59.00	436.0
60.00	1307.0
61.00	6583.0
62.00	6847.0
63.00	5024.0
64.00	572.0
65.00	400.0
66.90	434.0
68.00	14061.0
69.00	14566.0
70.00	1089.0
72.00	762.0
73.00	8007.0
74.00	22632.0
75.00	68064.0
76.10	6148.0
76.90	946.0
77.70	542.0
78.00	557.0
78.90	3285.0
80.00	1138.0
80.90	3389.0
81.90	809.0
83.00	104.0
83.90	144.0
85.00	77.0
86.00	153.0
87.00	5479.0
88.00	5365.0
91.00	512.0
92.00	3871.0
93.00	5728.0
94.00	15178.0
95.00	127744.0
96.00	8771.0
97.10	329.0
102.80	425.0
103.90	645.0
104.90	342.0
105.90	497.0
107.00	107.0
109.90	196.0
110.90	364.0
111.80	205.0
112.80	174.0
114.80	290.0
115.80	429.0
116.90	854.0
118.00	707.0
118.90	910.0
120.10	113.0
120.90	121.0
121.90	64.0
123.80	109.0
124.90	754.0
125.70	226.0
127.80	416.0
128.90	209.0
129.90	651.0
130.80	218.0
131.80	79.0
132.90	2464.0
135.00	333.0
135.90	104.0
136.80	207.0
139.60	80.0
140.10	143.0
140.90	1163.0
142.00	207.0
142.80	1214.0
143.90	157.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

144.80	233.0
145.90	146.0
146.90	496.0
147.90	321.0
148.90	198.0
149.80	216.0
153.00	59.0
154.00	94.0
154.90	366.0
157.00	190.0
158.90	222.0
160.90	287.0
162.20	103.0
163.00	385.0
164.00	81.0
164.90	358.0
165.70	66.0
167.00	62.0
170.10	72.0
170.70	92.0
171.30	211.0
172.10	592.0
173.90	92536.0
175.00	7456.0
175.90	88408.0
177.00	6676.0
177.90	463.0
178.90	794.0
179.90	126.0
180.80	91.0
188.90	171.0
189.80	106.0
191.00	2485.0
192.20	579.0
193.00	3241.0
194.00	618.0
195.10	359.0
202.80	249.0
203.90	105.0
205.00	440.0
205.20	445.0
207.00	1450.0
208.00	364.0
209.00	255.0
218.90	59.0
221.10	189.0
223.00	72.0
234.70	203.0
235.10	207.0
237.10	93.0
246.90	100.0
249.00	1884.0
250.00	561.0
250.90	947.0
251.90	164.0
253.00	126.0
265.00	2239.0
266.00	739.0
267.10	707.0
267.80	168.0
269.00	69.0
277.50	66.0
279.20	251.0
281.10	31688.0
282.10	9024.0
283.00	5292.0
284.00	1068.0
285.10	341.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

m/z	Abundance
36.00	1310.0
37.00	7648.0
38.10	6640.0
39.10	2758.0
40.00	470.0
40.90	147.0
42.90	189.0
44.10	966.0
45.10	1529.0
46.10	143.0
47.00	1910.0
48.00	1064.0
49.00	6472.0
50.00	26584.0
51.00	8356.0
52.00	370.0
55.00	403.0
56.00	2068.0
57.00	3615.0
58.10	184.0
59.10	188.0
60.00	1337.0
61.00	6664.0
62.00	6310.0
63.00	4390.0
64.00	565.0
65.10	357.0
66.00	85.0
67.10	564.0
68.00	13386.0
69.00	14144.0
70.00	1137.0
71.10	106.0
72.00	742.0
73.00	6807.0
74.00	22576.0
75.00	65880.0
76.00	5690.0
77.00	660.0
77.90	758.0
78.90	2906.0
80.00	1044.0
80.90	2813.0
81.90	702.0
82.90	149.0
83.90	107.0
85.90	194.0
87.00	5642.0
88.00	4810.0
91.00	500.0
92.00	3484.0
93.00	5392.0
94.00	14733.0
95.00	128040.0
96.00	8725.0
97.00	309.0
102.90	367.0
103.80	584.0
105.00	266.0
105.90	492.0
107.00	208.0
110.00	136.0
110.90	183.0
111.80	100.0
113.00	170.0
114.70	139.0
115.20	109.0
115.90	403.0
116.90	810.0
118.00	494.0
118.90	776.0
120.90	70.0
122.00	61.0
123.80	83.0
124.90	435.0
127.80	584.0
128.90	302.0
129.90	532.0
131.00	203.0
133.00	1253.0
133.90	234.0
134.80	259.0
136.80	235.0
139.60	54.0
140.10	100.0
140.90	1141.0
142.10	194.0
142.90	1303.0
143.90	116.0
144.70	99.0
145.80	210.0
146.90	309.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

148.00	282.0
148.90	163.0
149.90	141.0
152.90	116.0
153.80	87.0
155.00	328.0
157.00	168.0
158.80	170.0
160.90	227.0
162.30	88.0
162.90	263.0
165.00	238.0
168.90	83.0
170.00	57.0
170.90	98.0
172.10	622.0
173.90	100312.0
175.00	8033.0
175.90	97568.0
176.90	6830.0
178.00	321.0
178.90	284.0
189.10	141.0
190.10	117.0
191.00	1265.0
192.00	262.0
192.90	2022.0
194.10	288.0
194.90	186.0
203.00	202.0
204.90	482.0
207.00	1090.0
208.00	149.0
208.90	131.0
221.00	82.0
223.00	82.0
234.80	286.0
235.80	75.0
249.00	1225.0
249.90	300.0
250.90	418.0
251.20	372.0
251.90	149.0
253.00	68.0
265.00	1613.0
266.00	376.0
267.10	527.0
268.00	157.0
278.60	138.0
279.10	162.0
281.00	20840.0
282.10	5477.0
283.00	3119.0
284.10	731.0
284.80	228.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

m/z	Abundance
36.00	1026.0
37.10	5064.0
38.10	4855.0
39.00	1734.0
39.90	520.0
41.10	138.0
42.00	66.0
42.90	121.0
44.00	948.0
45.00	769.0
47.00	1453.0
47.90	738.0
49.00	4218.0
50.00	19776.0
51.10	5333.0
52.00	230.0
52.20	247.0
55.10	273.0
56.00	1507.0
57.10	2401.0
57.80	160.0
59.00	140.0
59.90	989.0
61.00	4288.0
62.00	4084.0
63.00	3063.0
64.10	374.0
65.00	184.0
67.10	264.0
68.00	8851.0
69.00	9279.0
70.00	707.0
71.20	104.0
72.00	531.0
73.00	5038.0
74.00	15374.0
75.00	46936.0
76.00	3853.0
77.00	551.0
78.00	523.0
79.00	2224.0
79.90	811.0
80.90	2301.0
81.90	561.0
83.00	180.0
87.00	4179.0
88.00	3624.0
90.90	271.0
92.00	2603.0
93.00	3930.0
94.00	11154.0
95.00	91536.0
96.00	6337.0
97.00	239.0
102.90	137.0
104.00	249.0
104.80	165.0
106.00	377.0
107.00	128.0
109.90	109.0
111.00	156.0
111.80	57.0
112.90	62.0
115.10	77.0
115.80	376.0
116.90	555.0
117.90	363.0
118.90	603.0
125.10	165.0
128.00	425.0
128.90	164.0
129.80	263.0
130.90	111.0
133.00	542.0
134.10	150.0
134.90	207.0
137.00	179.0
139.70	74.0
141.00	968.0
143.00	853.0
144.20	65.0
144.60	104.0
145.70	143.0
147.00	137.0
148.00	263.0
148.70	62.0
149.90	88.0
154.20	51.0
154.90	191.0
157.00	129.0
158.70	100.0
160.70	152.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

162.90	186.0
165.00	151.0
168.90	58.0
170.90	149.0
173.90	79064.0
175.00	6179.0
175.90	76136.0
176.90	4893.0
178.00	162.0
178.90	199.0
188.70	73.0
189.20	94.0
190.10	89.0
190.90	695.0
192.00	220.0
193.00	830.0
193.90	196.0
202.90	101.0
204.90	166.0
207.00	557.0
208.20	118.0
209.00	71.0
234.80	66.0
249.00	624.0
249.90	184.0
251.00	395.0
252.10	68.0
264.90	552.0
266.10	188.0
266.90	151.0
267.90	65.0
268.40	87.0
278.50	81.0
279.00	79.0
281.10	10395.0
282.00	2813.0
283.00	1850.0
284.00	330.0
285.00	114.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30