


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072221\
Data File : VW019564.D
Acq On : 22 Jul 2021 19:57
Operator : SY/VA
Sample : M3122-14
Misc : 3.53g/10.0mL/MSVOA_W/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDC9

Manual Integrations
APPROVED

MMDadoda
7/23/2021 9:23:53 AM

Quant Time: Jul 23 01:52:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 23 01:46:10 2021
Response via : Initial Calibration

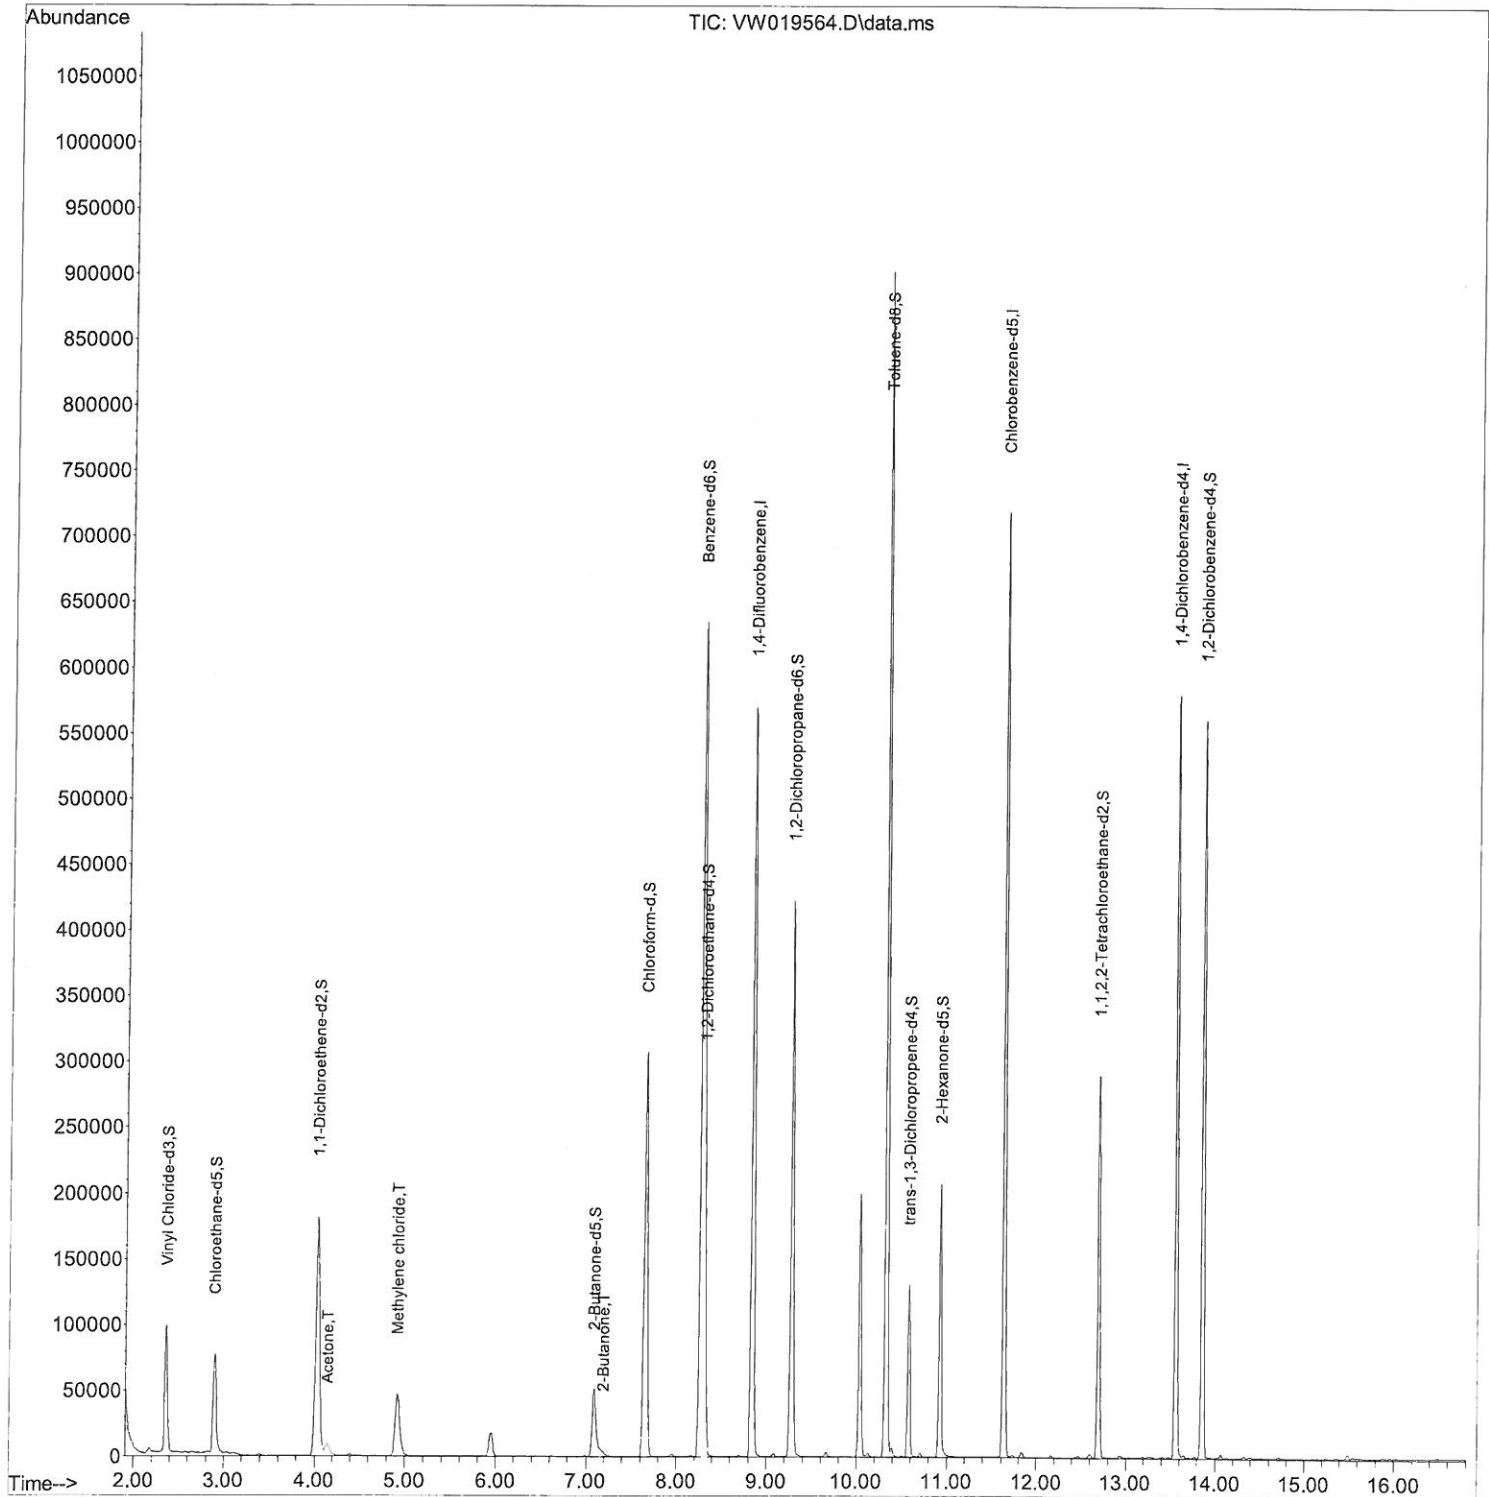

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072221\
 Data File : VW019564.D
 Acq On : 22 Jul 2021 19:57
 Operator : SY/VA
 Sample : M3122-14
 Misc : 3.53g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC9

Manual Integrations
 APPROVED

MMDadoda
 7/23/2021 9:23:53 AM

Quant Time: Jul 23 01:52:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 23 01:46:10 2021
 Response via : Initial Calibration

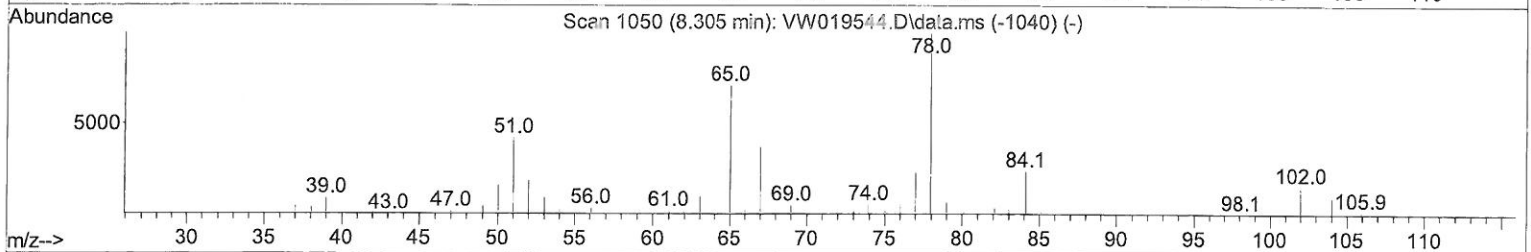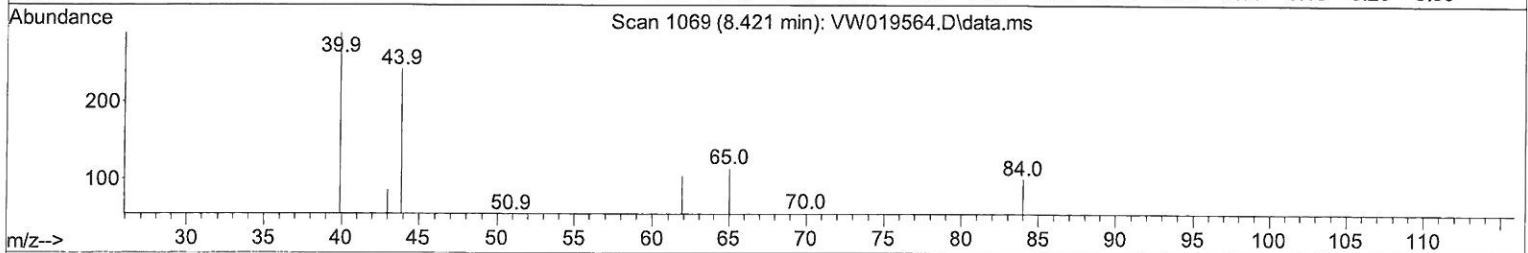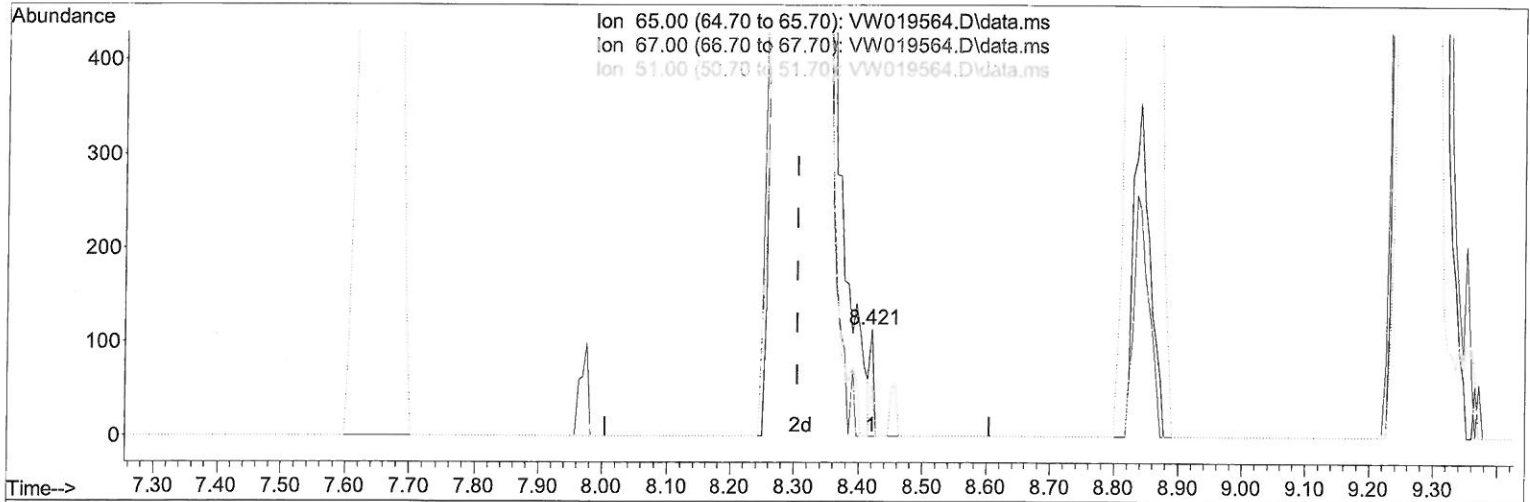

TIC: VW019564.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.421min (+ 0.116) 0.01 ug/L

response 42

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.70	61.90
51.00	98.00	92.86
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072221\
 Data File : VW019564.D
 Acq On : 22 Jul 2021 19:57
 Operator : SY/VA
 Sample : M3122-14
 Misc : 3.53g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC9

Manual Integrations
 APPROVED

MMDadoda
 7/23/2021 9:23:53 AM

Quant Time: Jul 23 01:52:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 23 01:46:10 2021
 Response via : Initial Calibration

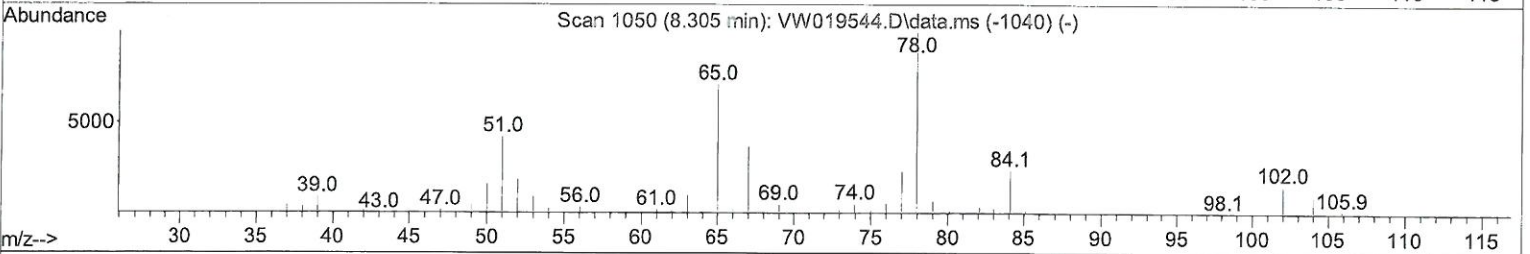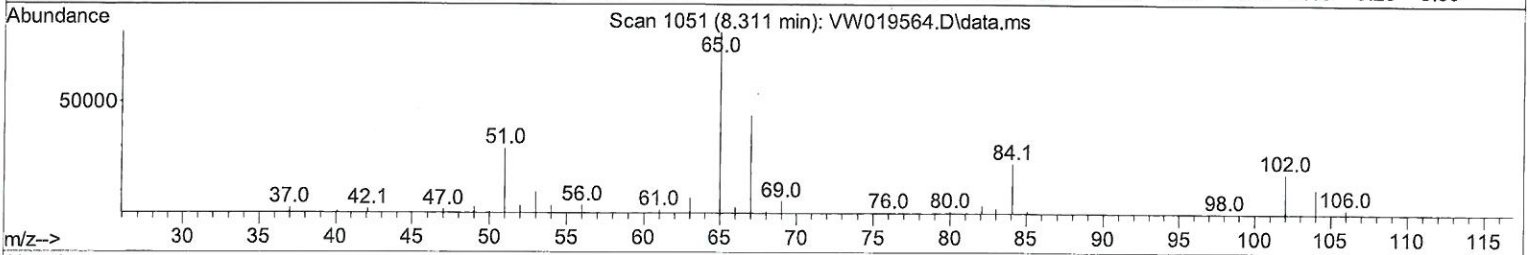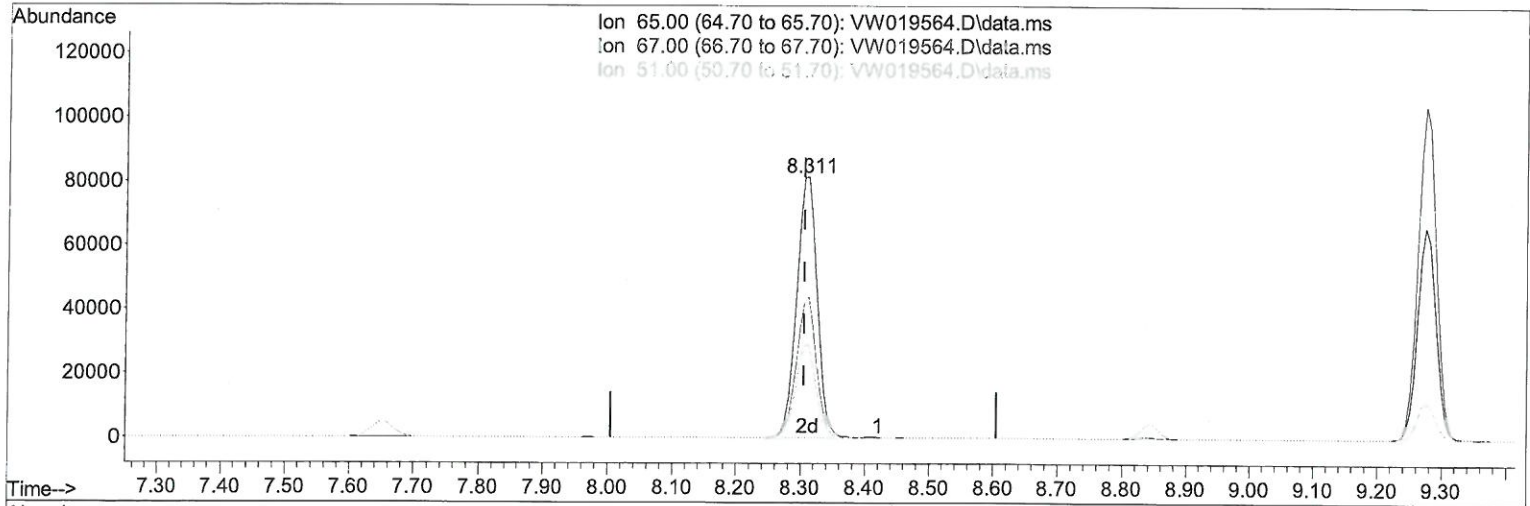

TIC: VW019564.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.311min (+ 0.006) 25.27 ug/L m

response 182269

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.70	0.01#
51.00	98.00	0.02#
0.00	0.00	0.00

Handwritten: 7ME
 7/30/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072221\
 Data File : VW019564.D
 Acq On : 22 Jul 2021 19:57
 Operator : SY/VA
 Sample : M3122-14
 Misc : 3.53g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC9

Manual Integrations
 APPROVED

MMDadoda
 7/23/2021 9:23:53 AM

Quant Time: Jul 23 01:52:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 23 01:46:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	475726	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	414146	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	156568	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	108641	16.118	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	64.480%	
7) Chloroethane-d5	2.898	69	104135	21.665	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	86.640%	
11) 1,1-Dichloroethene-d2	4.025	63	205765	15.821	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	63.280%	
21) 2-Butanone-d5	7.086	46	88915	45.449	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	90.900%	
24) Chloroform-d	7.653	84	331273	25.202	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	100.800%	
26) 1,2-Dichloroethane-d4	8.311	65	182269m	25.268	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	101.080%	
32) Benzene-d6	8.281	84	657697	26.679	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	106.720%	
36) 1,2-Dichloropropane-d6	9.274	67	206147	26.829	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	107.320%	
41) Toluene-d8	10.323	98	578075	26.008	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	104.040%	
43) trans-1,3-Dichloroprop...	10.579	79	74981	22.787	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	91.160%	
47) 2-Hexanone-d5	10.927	63	71224	49.963	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	99.920%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	151579	24.414	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	97.640%	
66) 1,2-Dichlorobenzene-d4	13.853	152	146996	26.610	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	106.440%	
Target Compounds						
13) Acetone	4.141	43	18594	12.899	ug/L	81
16) Methylene chloride	4.922	84	41963	4.425	ug/L	95
22) 2-Butanone	7.189	43	6232	2.794	ug/L #	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

> MD
 7/30/21