

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW072320\
 Data File : VW015924.D
 Acq On : 23 Jul 2020 16:16
 Operator : SY/VA
 Sample : L3395-03MSD
 Misc : 5.82G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAY13MSD

Quant Time: Jul 24 09:36:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 24 06:59:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	388863	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	342735	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	117733	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	118297	21.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.24%
7) Chloroethane-d5	2.90	69	91415	20.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.04%
10) 1,1-Dichloroethene-d2	4.02	63	227438	20.50	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	82.00%
20) 2-Butanone-d5	7.09	46	83040	57.61	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.22%
24) Chloroform-d	7.65	84	222622	20.38	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.52%
26) 1,2-Dichloroethane-d4	8.31	65	137917	23.00	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.00%
29) Benzene-d6	8.27	84	440084	21.10	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.40%
33) 1,2-Dichloropropane-d6	9.27	67	140355	22.44	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.76%
37) Toluene-d8	10.33	98	375631	19.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.52%
38) trans-1,3-Dichloropropene-	10.58	79	59498	22.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.28%
39) 2-Hexanone-d5	10.93	63	63198	60.69	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.38%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	126803	26.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.52%
61) 1,2-Dichlorobenzene-d4	13.85	152	100867	21.97	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.88%

Target Compounds


					Qvalue
12) 1,1-Dichloroethene	4.04	96	100914	20.188 ug/L	89
13) Acetone	4.14	43	50420	41.654 ug/L	97
14) Carbon disulfide	4.38	76	5796	0.367 ug/L #	94
21) 2-Butanone	7.20	43	3833	2.561 ug/L	86
34) Benzene	8.33	78	473127	22.729 ug/L	100
35) Trichloroethene	9.09	95	116783	21.208 ug/L	98
44) Toluene	10.39	91	490557	22.469 ug/L	99
52) Chlorobenzene	11.66	112	290374	20.756 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW072320\
Data File : VW015924.D
Acq On : 23 Jul 2020 16:16
Operator : SY/VA
Sample : L3395-03MSD
Misc : 5.82G/10ML/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAY13MSD

Quant Time: Jul 24 09:36:10 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 24 06:59:55 2020
Response via : Initial Calibration




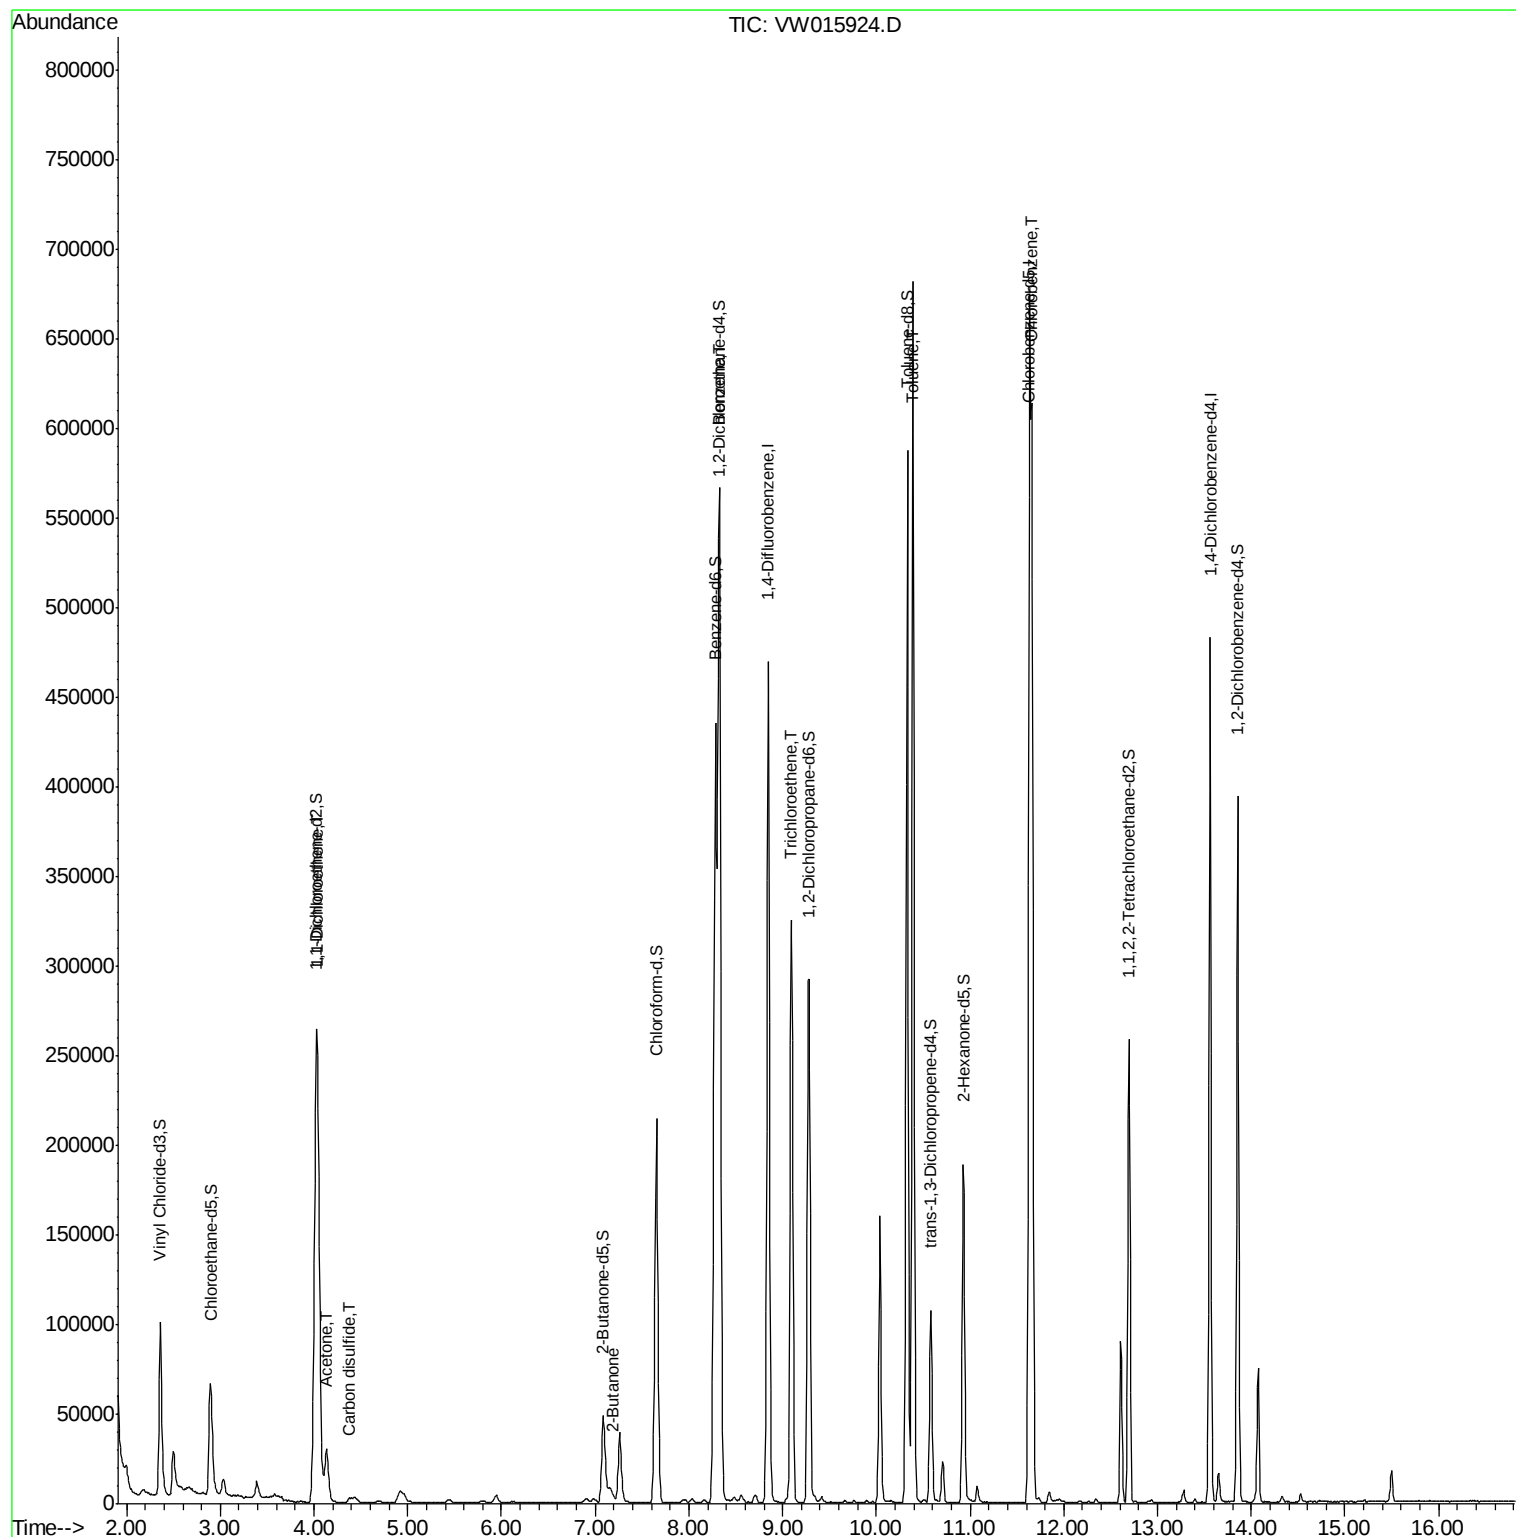


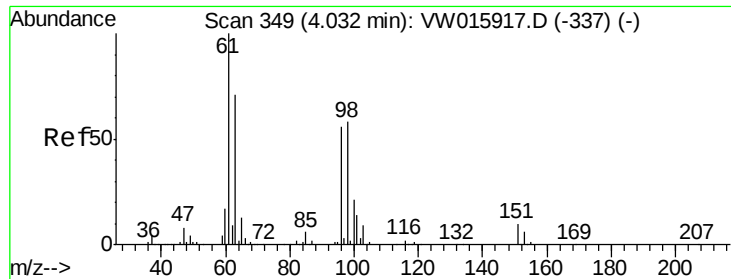

#12
 1,1-Dichloroethene
 Concen: 20.188 ug/L
 RT: 4.04 min Scan# 350
 Delta R.T. 0.01 min
 Lab File: VW015924.D
 Acq: 23 Jul 2020 16:16




Instrument :
 MSVOA_W
 ClientSampled :
 GAY13MSD


Tgt Ion: 96 Resp: 100914
 Ion Ratio Lower Upper
 96 100
 61 180.4 125.0 232.2
 63 144.8 82.3 152.8

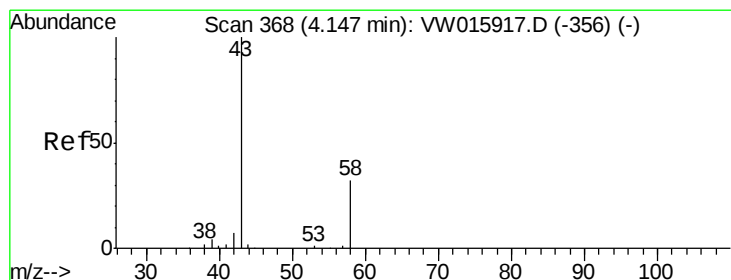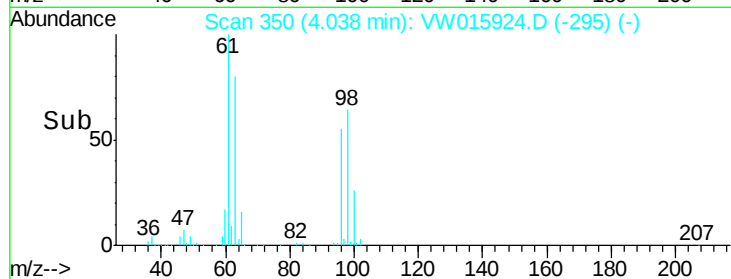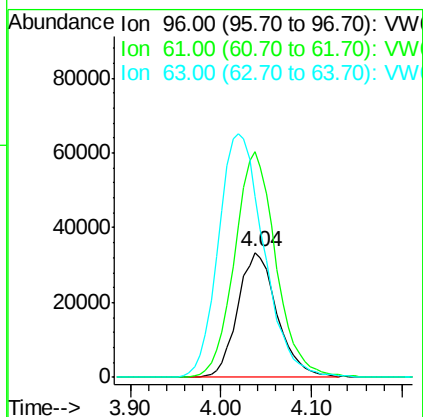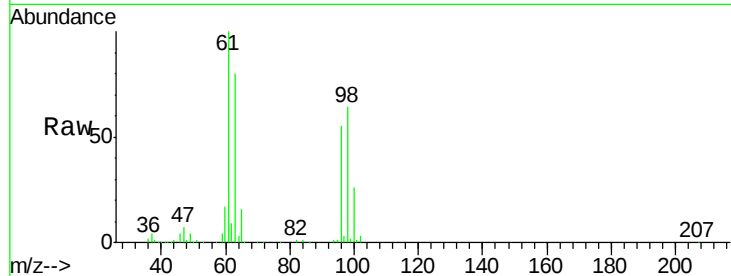

#13
 Acetone
 Concen: 41.654 ug/L
 RT: 4.14 min Scan# 366
 Delta R.T. -0.01 min
 Lab File: VW015924.D
 Acq: 23 Jul 2020 16:16

Tgt Ion: 43 Resp: 50420
 Ion Ratio Lower Upper
 43 100
 58 30.6 0.0 58.2

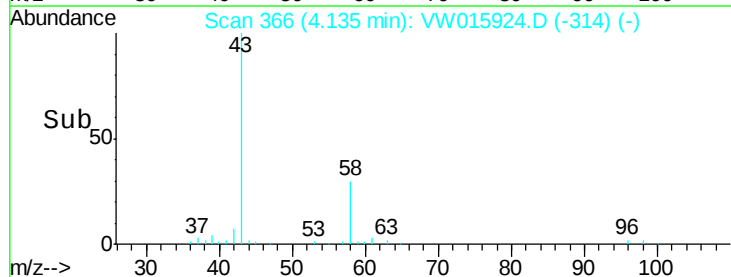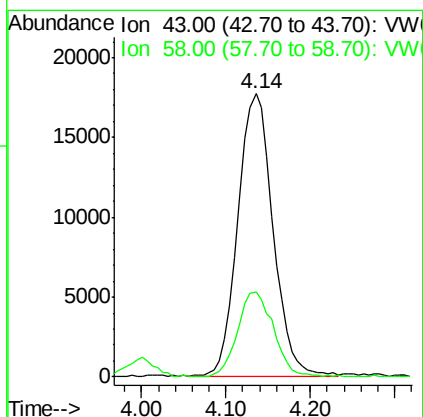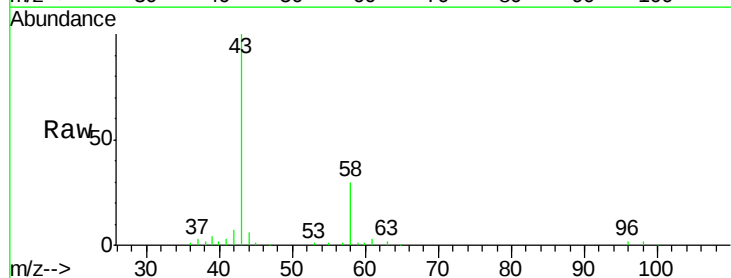

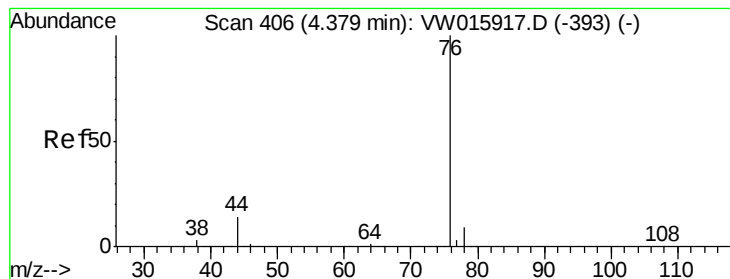

#14

Carbon disulfide

Concen: 0.367 ug/L

RT: 4.38 min Scan# 406

Delta R.T. 0.00 min

Lab File: VW015924.D

Acq: 23 Jul 2020 16:16

Instrument :

MSVOA_W

ClientSampleId :


GAY13MSD

Tgt Ion: 76 Resp: 5796

Ion Ratio Lower Upper




76 100

78 7.0 7.2 10.8#

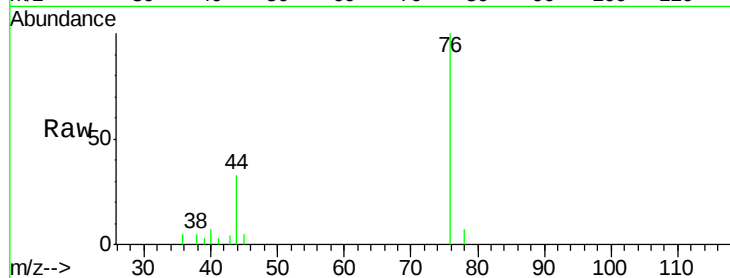

Abundance Ion 76.00 (75.70 to 76.70): VW

Ion 78.00 (77.70 to 78.70): VW

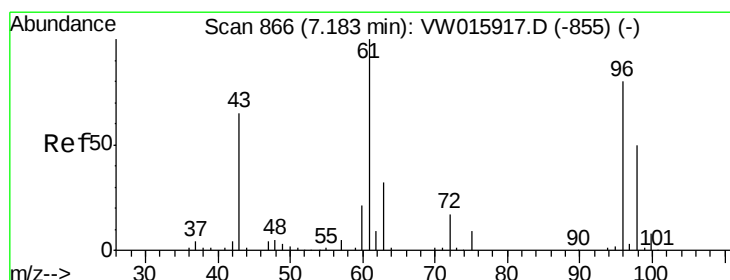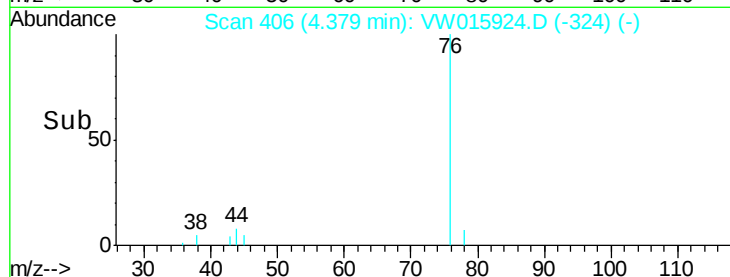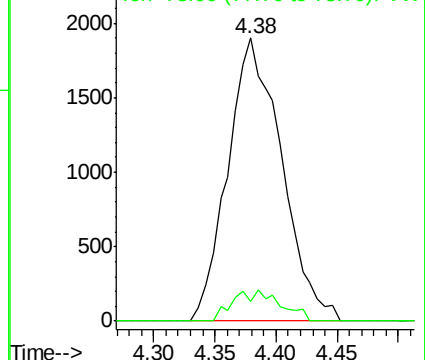

#21

2-Butanone

Concen: 2.561 ug/L

RT: 7.20 min Scan# 868

Delta R.T. 0.01 min

Lab File: VW015924.D


Acq: 23 Jul 2020 16:16

Tgt Ion: 43 Resp: 3833

Ion Ratio Lower Upper



43 100


72 35.3 13.9 41.7

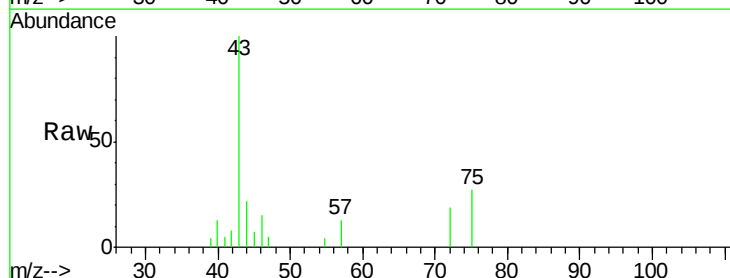

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 72.00 (71.70 to 72.70): VW

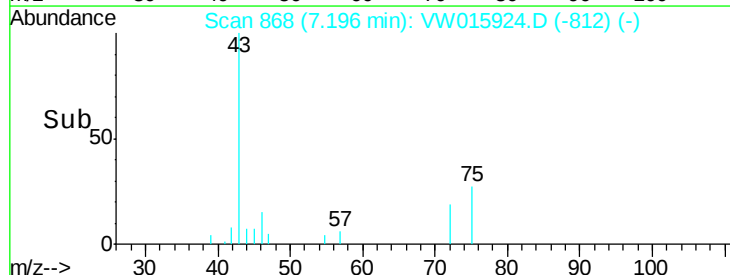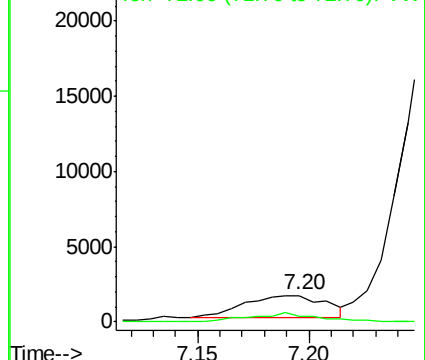

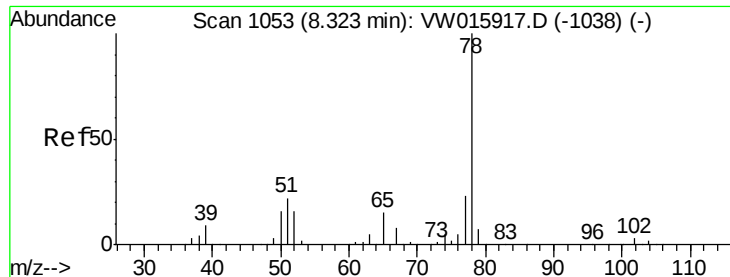

#34

Benzene

Concen: 22.729 ug/L

RT: 8.33 min Scan# 1054

Delta R.T. 0.01 min

Lab File: VW015924.D

Acq: 23 Jul 2020 16:16


Instrument :

MSVOA_W




ClientSampleId :

GAY13MSD

Tgt Ion: 78 Resp: 473127

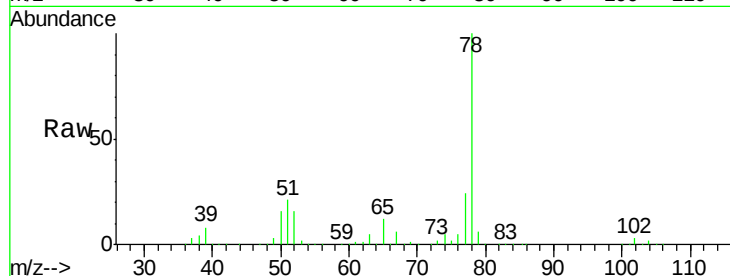

Abundance Ion 78.00 (77.70 to 78.70): VW

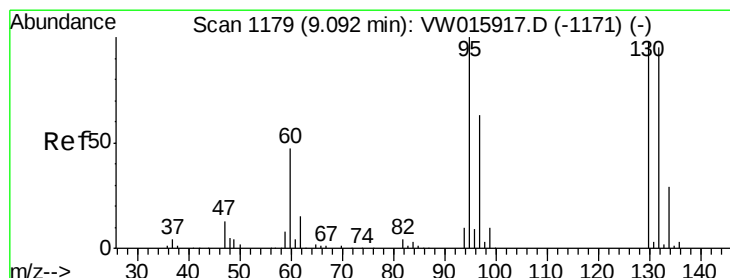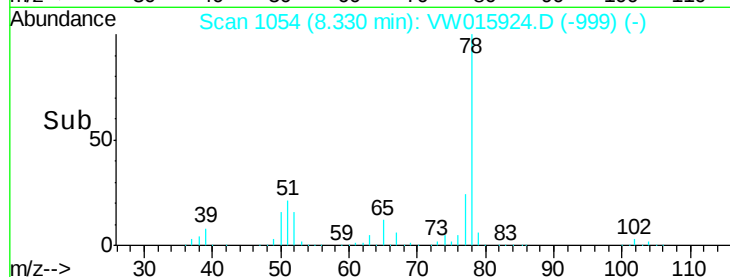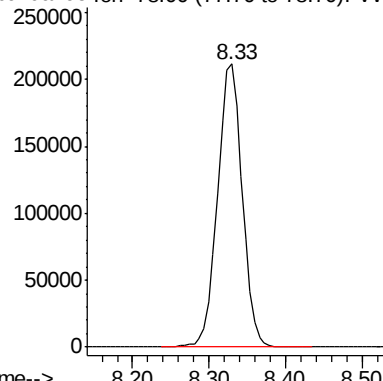

#35

Trichloroethene

Concen: 21.208 ug/L

RT: 9.09 min Scan# 1179

Delta R.T. 0.00 min

Lab File: VW015924.D

Acq: 23 Jul 2020 16:16

Tgt Ion: 95 Resp: 116783

Ion	Ratio	Lower	Upper
95	100		
97	63.4	44.4	82.4
132	96.2	65.1	120.9
130	99.9	68.6	127.4




Ion 95.00 (94.70 to 95.70): VW


Ion 97.00 (96.70 to 97.70): VW

Ion 132.00 (131.70 to 132.70): VW

Ion 130.00 (129.70 to 130.70): VW

Abundance Ion 95.00 (94.70 to 95.70): VW

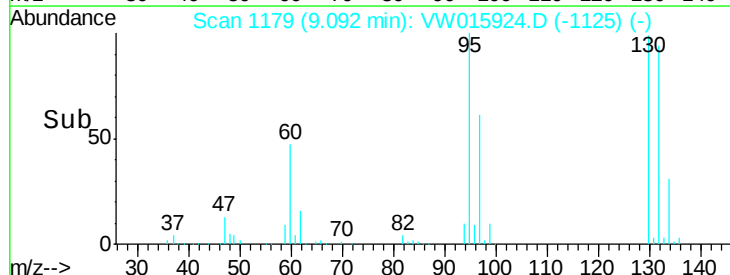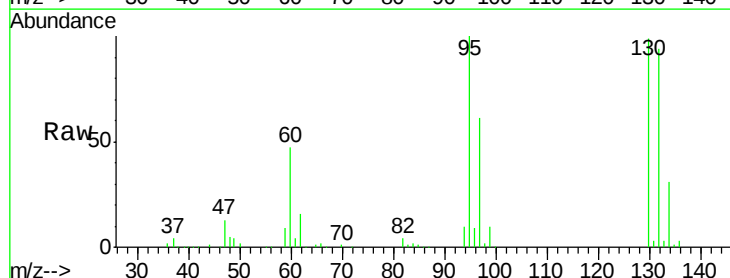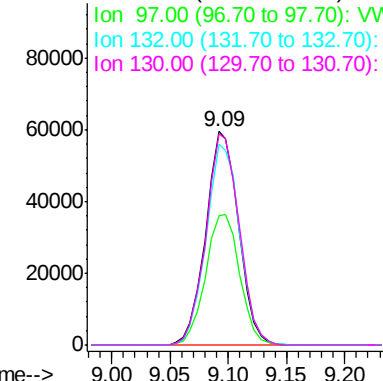

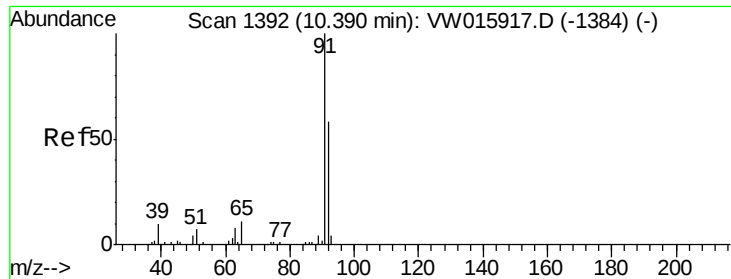

#44

Toluene

Concen: 22.469 ug/L

RT: 10.39 min Scan# 1392

Delta R.T. 0.00 min

Lab File: VW015924.D

Acq: 23 Jul 2020 16:16

Instrument :

MSVOA_W

ClientSampleId :





GAY13MSD

Tgt Ion: 91 Resp: 490557

Ion Ratio Lower Upper

91 100

92 59.8 41.2 76.4

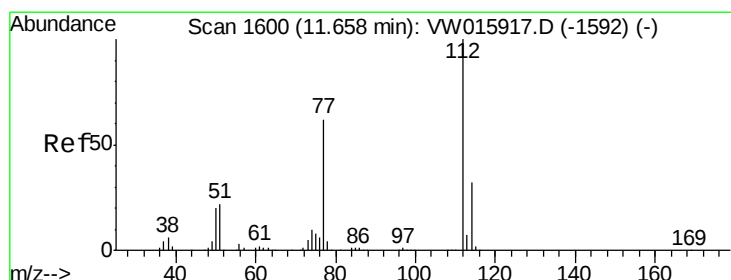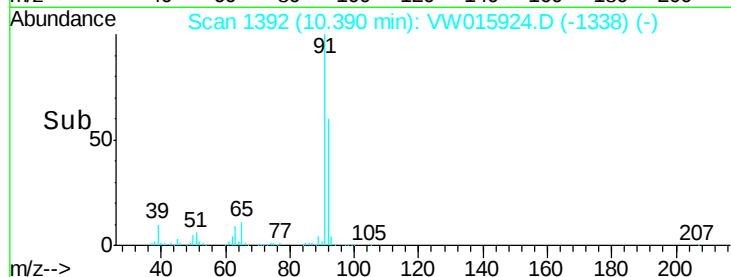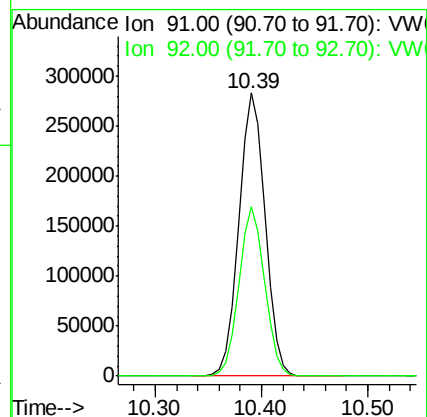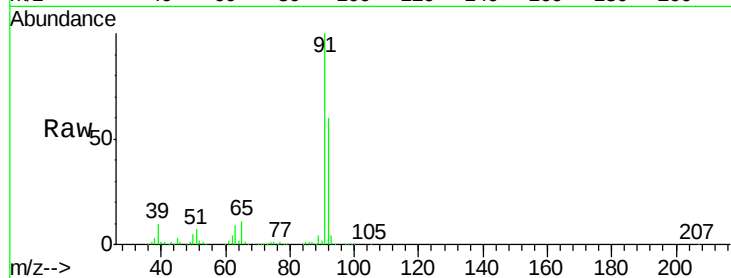

#52

Chlorobenzene

Concen: 20.756 ug/L

RT: 11.66 min Scan# 1600

Delta R.T. 0.00 min

Lab File: VW015924.D

Acq: 23 Jul 2020 16:16

Tgt Ion: 112 Resp: 290374

Ion Ratio Lower Upper

112 100

77 61.9 47.8 71.6

114 32.0 22.1 41.1

