

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW072320\
 Data File : VW015931.D
 Acq On : 23 Jul 2020 19:01
 Operator : SY/VA
 Sample : L3388-10
 Misc : 4.93G/10ML/MSVOA_W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AD6

Quant Time: Jul 24 08:07:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 24 06:59:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	367590	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	299809	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	105782	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	123917	23.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.56%
7) Chloroethane-d5	2.90	69	95655	22.71	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.84%
10) 1,1-Dichloroethene-d2	4.01	63	176423	16.82	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.28%
20) 2-Butanone-d5	7.08	46	52712	38.69	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.38%
24) Chloroform-d	7.65	84	217382	21.06	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.24%
26) 1,2-Dichloroethane-d4	8.31	65	130376	23.00	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.00%
29) Benzene-d6	8.27	84	431458	23.64	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.56%
33) 1,2-Dichloropropane-d6	9.27	67	133648	24.43	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.72%
37) Toluene-d8	10.33	98	357093	21.60	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.40%
38) trans-1,3-Dichloropropene-	10.58	79	42619	18.28	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.12%
39) 2-Hexanone-d5	10.93	63	36453	40.02	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.04%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	105839	25.17	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.68%
61) 1,2-Dichlorobenzene-d4	13.85	152	90016	21.82	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.28%


Target Compounds					Qvalue
16) Methylene chloride	4.92	84	13951	2.316 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW072320\
Data File : VW015931.D
Acq On : 23 Jul 2020 19:01
Operator : SY/VA
Sample : L3388-10
Misc : 4.93G/10ML/MSVOA_W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AD6

Quant Time: Jul 24 08:07:34 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 24 06:59:55 2020
Response via : Initial Calibration

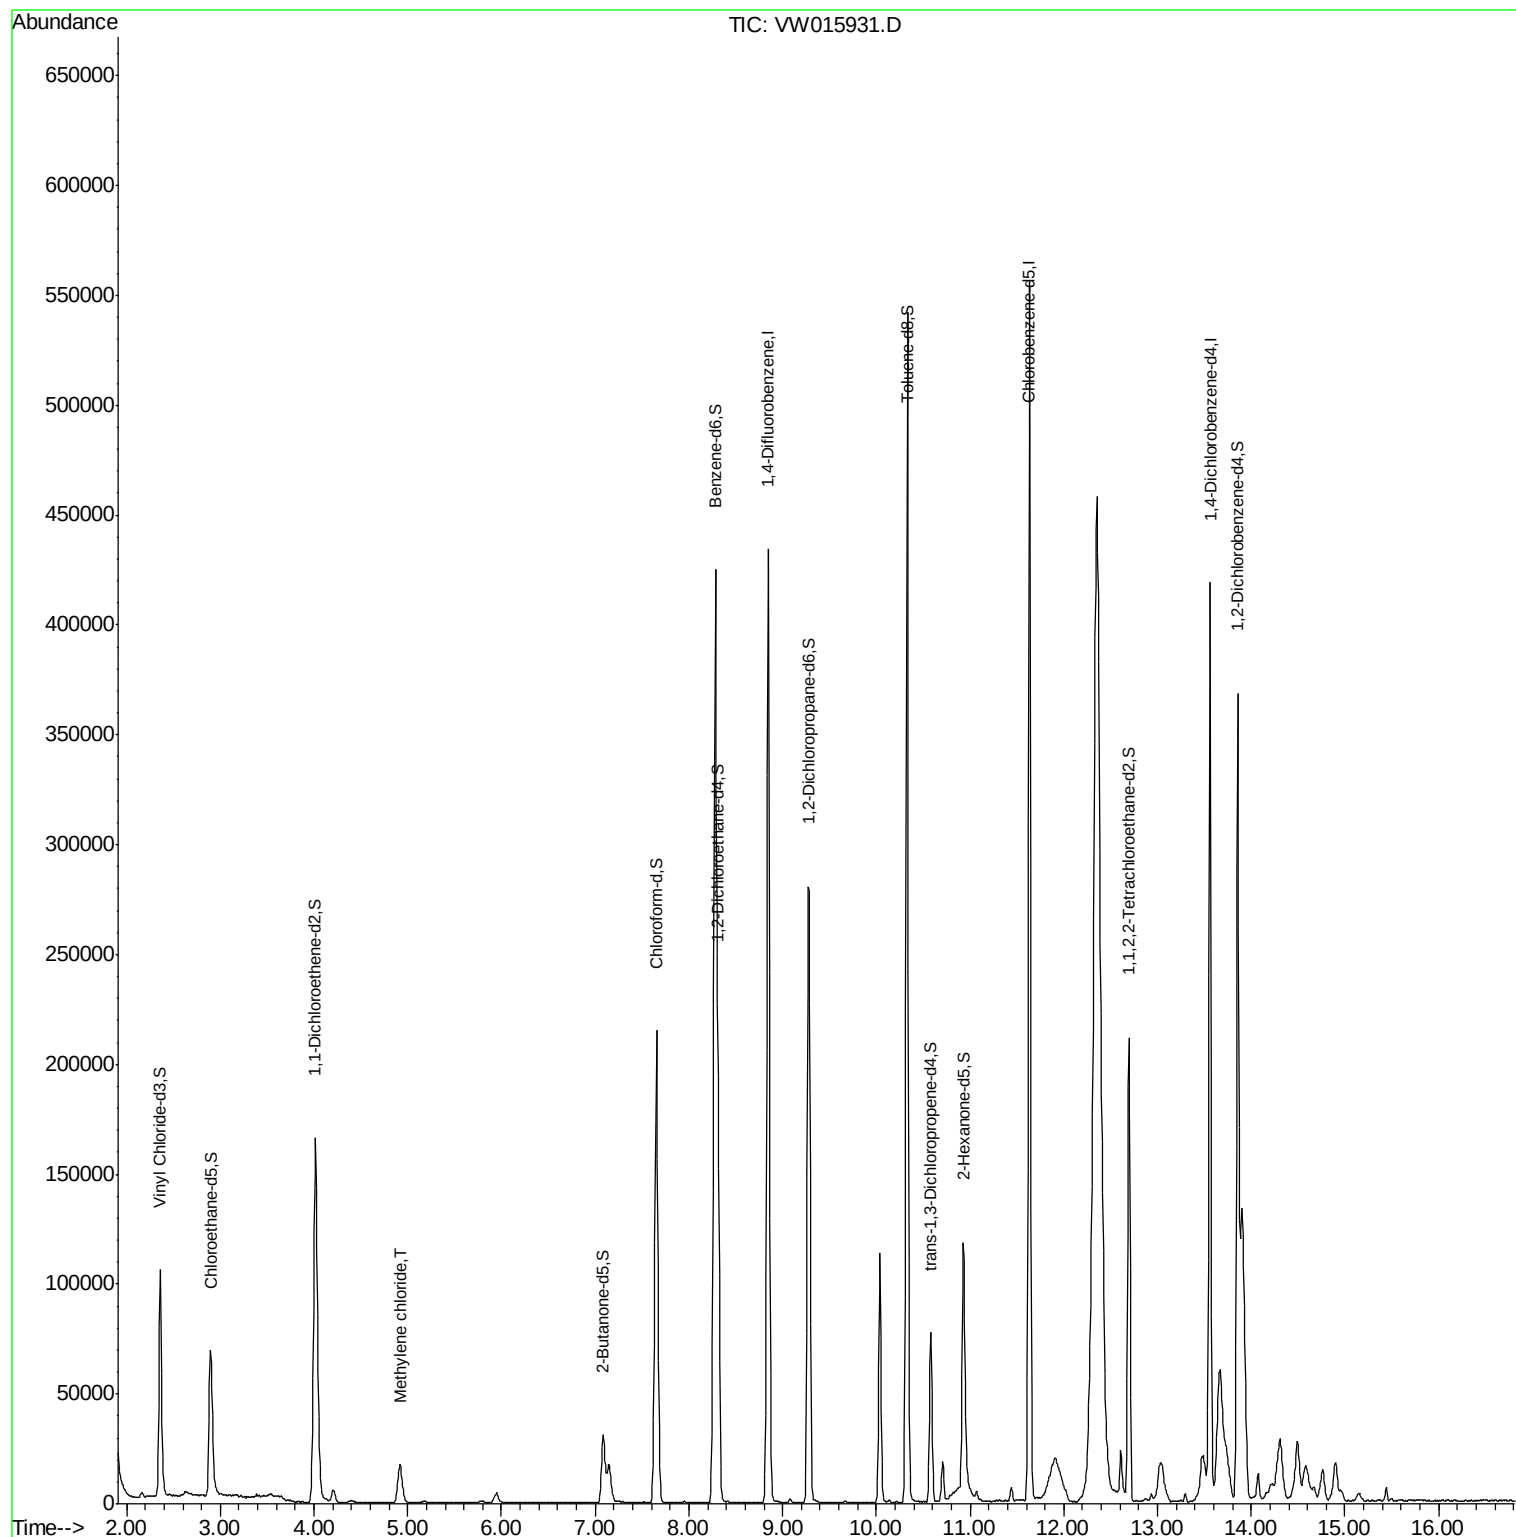

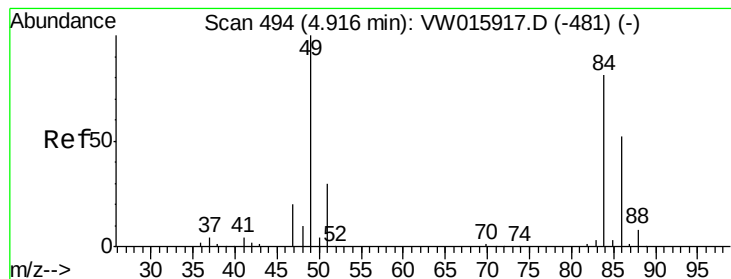

#16
Methylene chloride
Concen: 2.316 ug/L
RT: 4.92 min Scan# 494
Delta R.T. 0.00 min
Lab File: VW015931.D
Acq: 23 Jul 2020 19:01

Instrument :
MSVOA_W
ClientSampleId :
C0AD6

Tgt Ion: 84 Resp: 13951
Ion Ratio Lower Upper
84 100
49 130.4 91.1 169.1
86 61.9 46.0 85.4

