
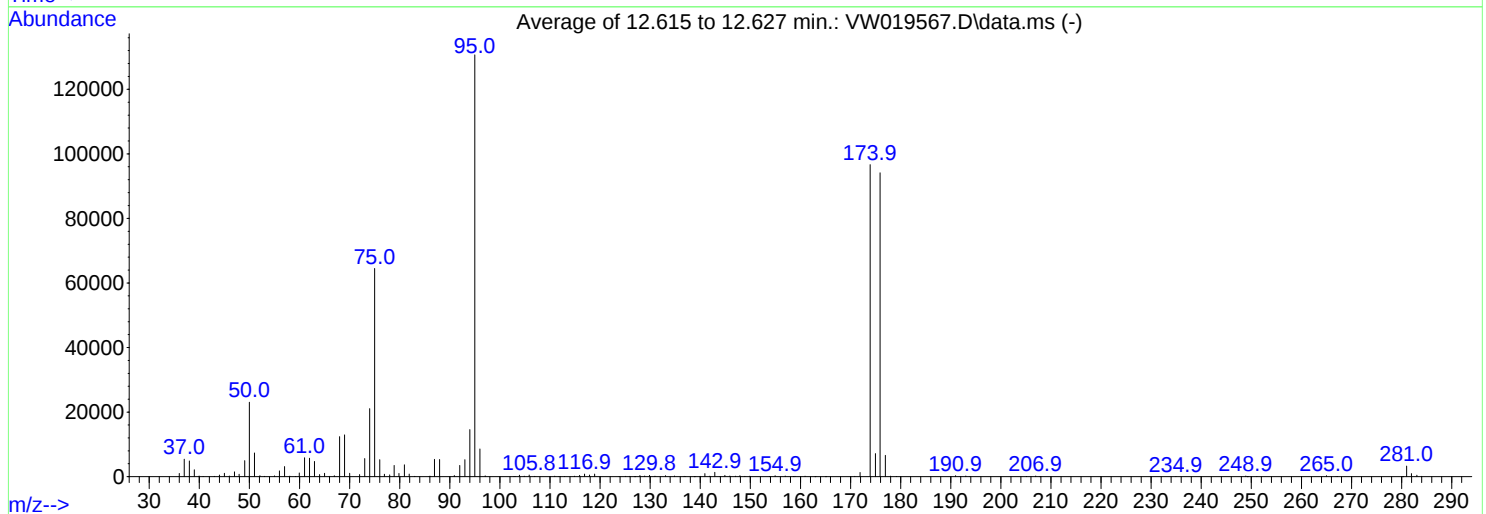


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072321\
 Data File : VW019567.D
 Acq On : 23 Jul 2021 08:56
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W071921S.M
 Title : SW846 8260
 Last Update : Tue Jul 20 04:37:55 2021

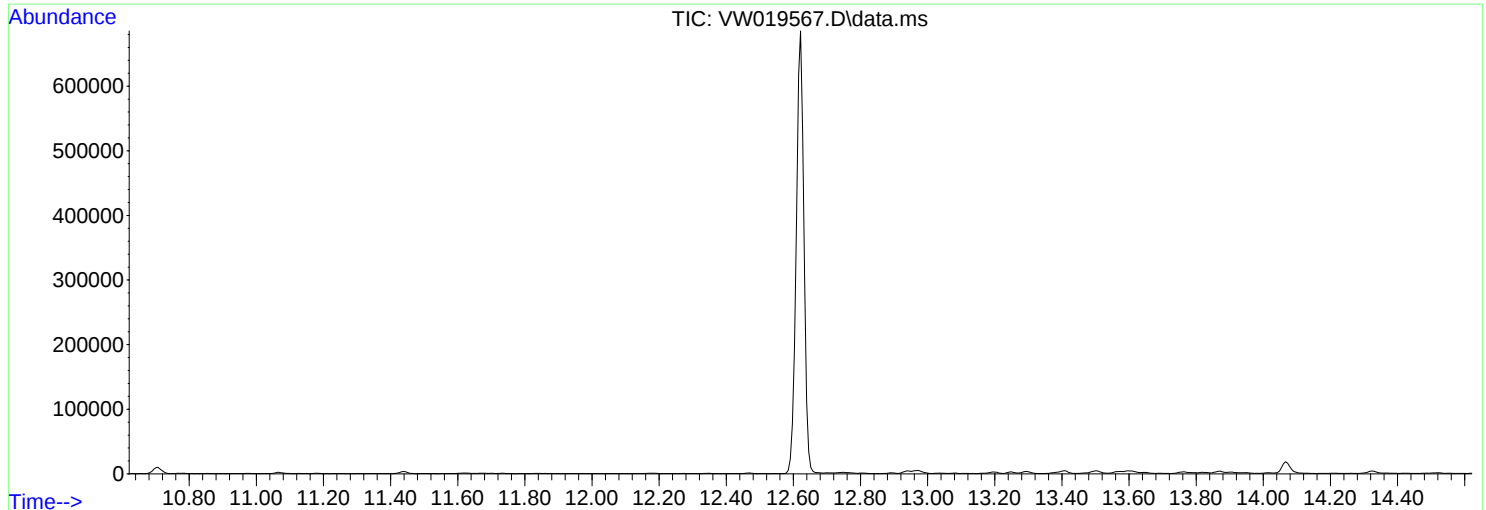

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	23067	PASS
75	95	30	60	49.4	64509	PASS
95	95	100	100	100.0	130685	PASS
96	95	5	9	6.6	8595	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.0	96693	PASS
175	174	5	9	7.4	7164	PASS
176	174	95	101	97.4	94136	PASS
177	176	5	9	7.0	6610	PASS