

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW072518\
 Data File : VW004193.D
 Acq On : 25 Jul 2018 12:09
 Operator : SY/AP
 Sample : J4040-16
 Misc : 5.95G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AE7

Quant Time: Jul 26 00:50:15 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071818S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 26 00:50:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	281813	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	280694	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	127230	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	48790	17.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.00%
7) Chloroethane-d5	2.89	69	39076	19.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.80%
10) 1,1-Dichloroethene-d2	4.01	63	83484	12.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.92%
20) 2-Butanone-d5	7.09	46	81084	49.60	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.20%
24) Chloroform-d	7.65	84	158663	23.72	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.88%
26) 1,2-Dichloroethane-d4	8.31	65	97305	24.15	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.60%
29) Benzene-d6	8.27	84	278035	21.36	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.44%
33) 1,2-Dichloropropane-d6	9.28	67	102812	23.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.68%
37) Toluene-d8	10.33	98	232195	19.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.40%
38) trans-1,3-Dichloropropene-	10.58	79	34678	18.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.68%
39) 2-Hexanone-d5	10.93	63	53879	46.09	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.18%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	119064	25.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.12%
61) 1,2-Dichlorobenzene-d4	13.87	152	104206	25.47	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.88%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.13	43	4198	2.362	ug/L	97
40) 1,2-Dichloropropane	9.27	63	11106	2.381	ug/L #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW072518\
Data File : VW004193.D
Acq On : 25 Jul 2018 12:09
Operator : SY/AP
Sample : J4040-16
Misc : 5.95G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AE7

Quant Time: Jul 26 00:50:15 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071818S.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 26 00:50:03 2018
Response via : Initial Calibration

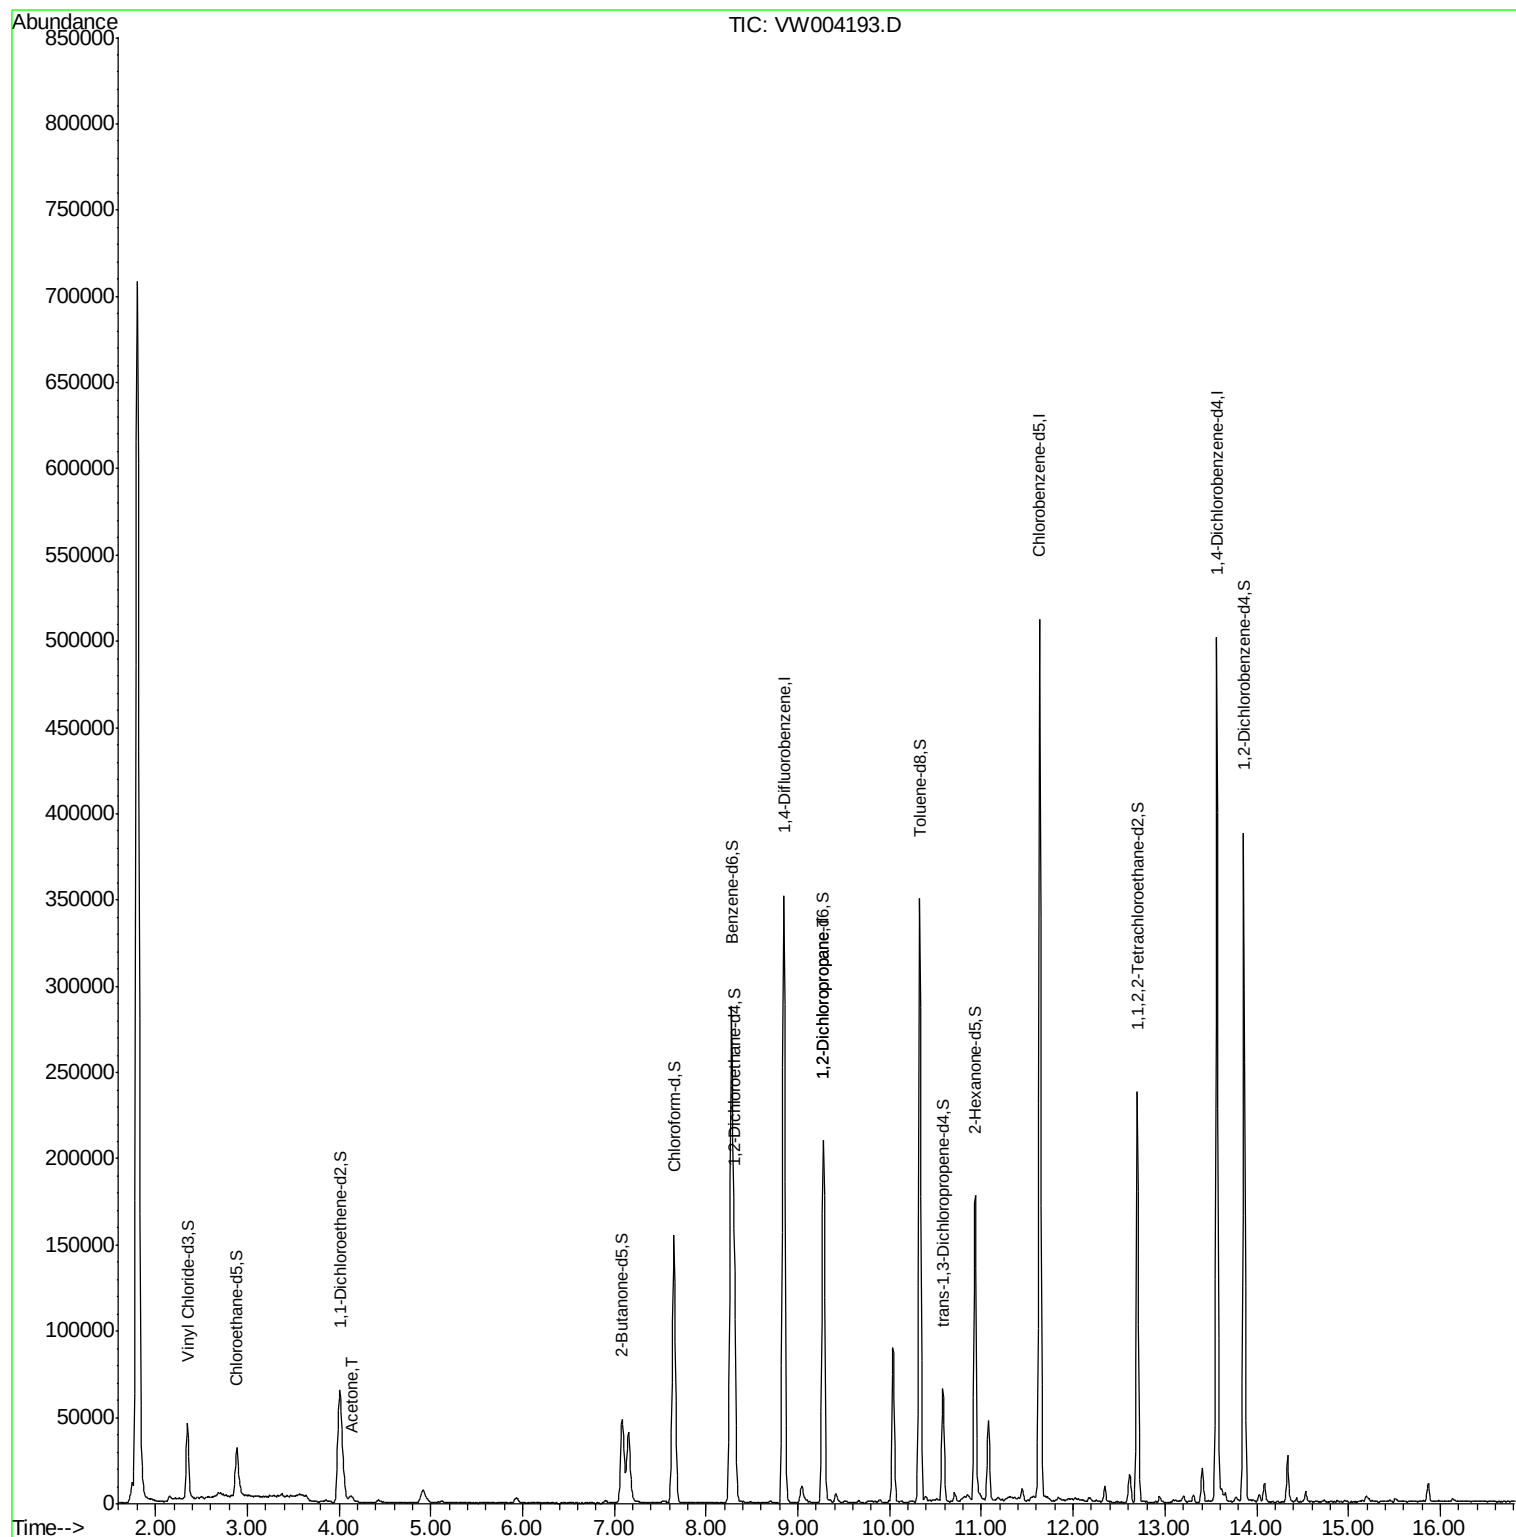

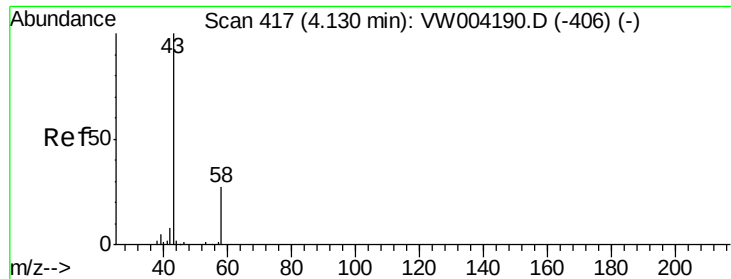

#13

Acetone

Concen: 2.362 ug/L

RT: 4.13 min Scan# 417

Delta R.T. -0.00 min

Lab File: VW004193.D

Acq: 25 Jul 2018 12:09

Instrument :

MSVOA_W

ClientSampleId :


C0AE7

Tgt Ion: 43 Resp: 4198

Ion Ratio Lower Upper




43 100

58 31.1 0.0 59.4

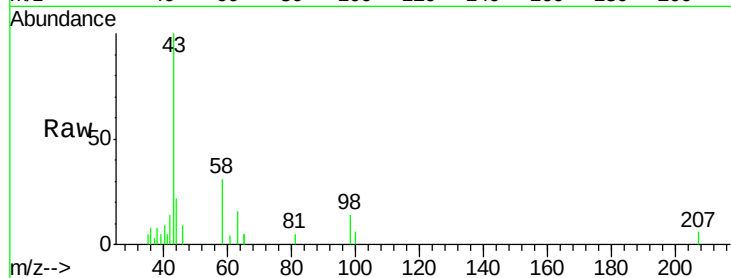

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

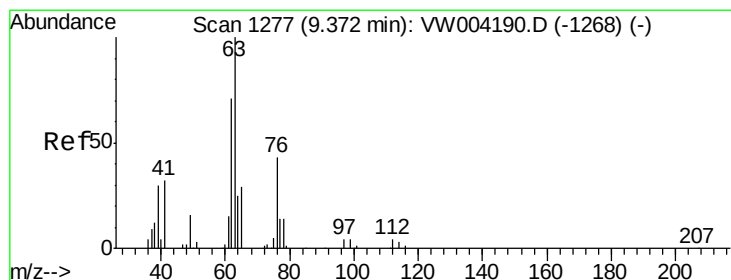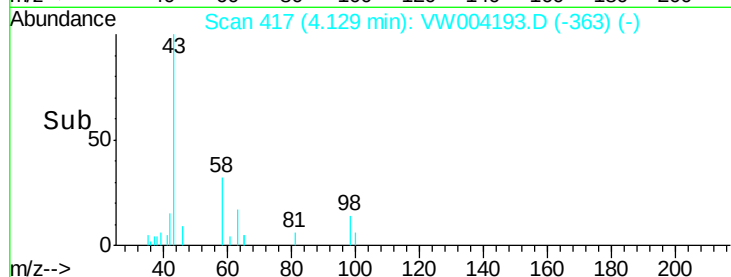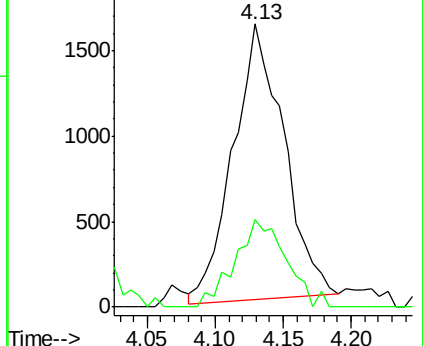

#40

1,2-Dichloropropane

Concen: 2.381 ug/L

RT: 9.27 min Scan# 1261

Delta R.T. -0.10 min

Lab File: VW004193.D


Acq: 25 Jul 2018 12:09

Tgt Ion: 63 Resp: 11106

Ion Ratio Lower Upper

63 100

112 0.6 3.0 4.4#

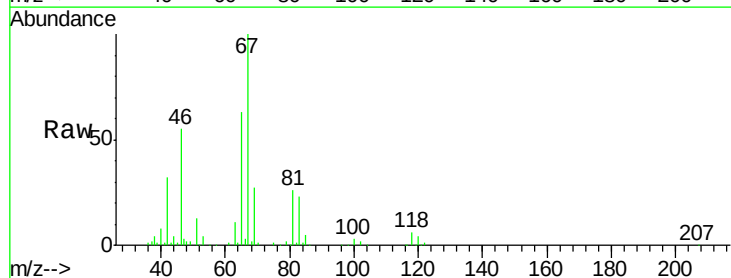

Abundance Ion 63.00 (62.70 to 63.70): VW

Ion 112.00 (111.70 to 112.70): V

