

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW072518\
 Data File : VW004193.D
 Acq On : 25 Jul 2018 12:09
 Operator : SY/AP
 Sample : J4040-16
 Misc : 5.95G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AE7

Quant Time: Jul 26 00:57:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071818S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 26 00:50:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	281813	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	280694	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	127230	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	48790	17.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.00%
7) Chloroethane-d5	2.89	69	39076	19.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.80%
10) 1,1-Dichloroethene-d2	4.01	63	83484	12.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.92%
20) 2-Butanone-d5	7.09	46	81084	49.60	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.20%
24) Chloroform-d	7.65	84	158663	23.72	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.88%
26) 1,2-Dichloroethane-d4	8.31	65	97305	24.15	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.60%
29) Benzene-d6	8.27	84	278035	21.36	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.44%
33) 1,2-Dichloropropane-d6	9.28	67	102812	23.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.68%
37) Toluene-d8	10.33	98	232195	19.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.40%
38) trans-1,3-Dichloropropene-	10.58	79	34678	18.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.68%
39) 2-Hexanone-d5	10.93	63	53879	46.09	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.18%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	119064	25.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.12%
61) 1,2-Dichlorobenzene-d4	13.87	152	104206	25.47	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.88%


Target Compounds					Ovalue
13) Acetone	4.13	43	4198	2.362 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW072518\
Data File : VW004193.D
Acq On : 25 Jul 2018 12:09
Operator : SY/AP
Sample : J4040-16
Misc : 5.95G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AE7

Quant Time: Jul 26 00:57:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071818S.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 26 00:50:03 2018
Response via : Initial Calibration

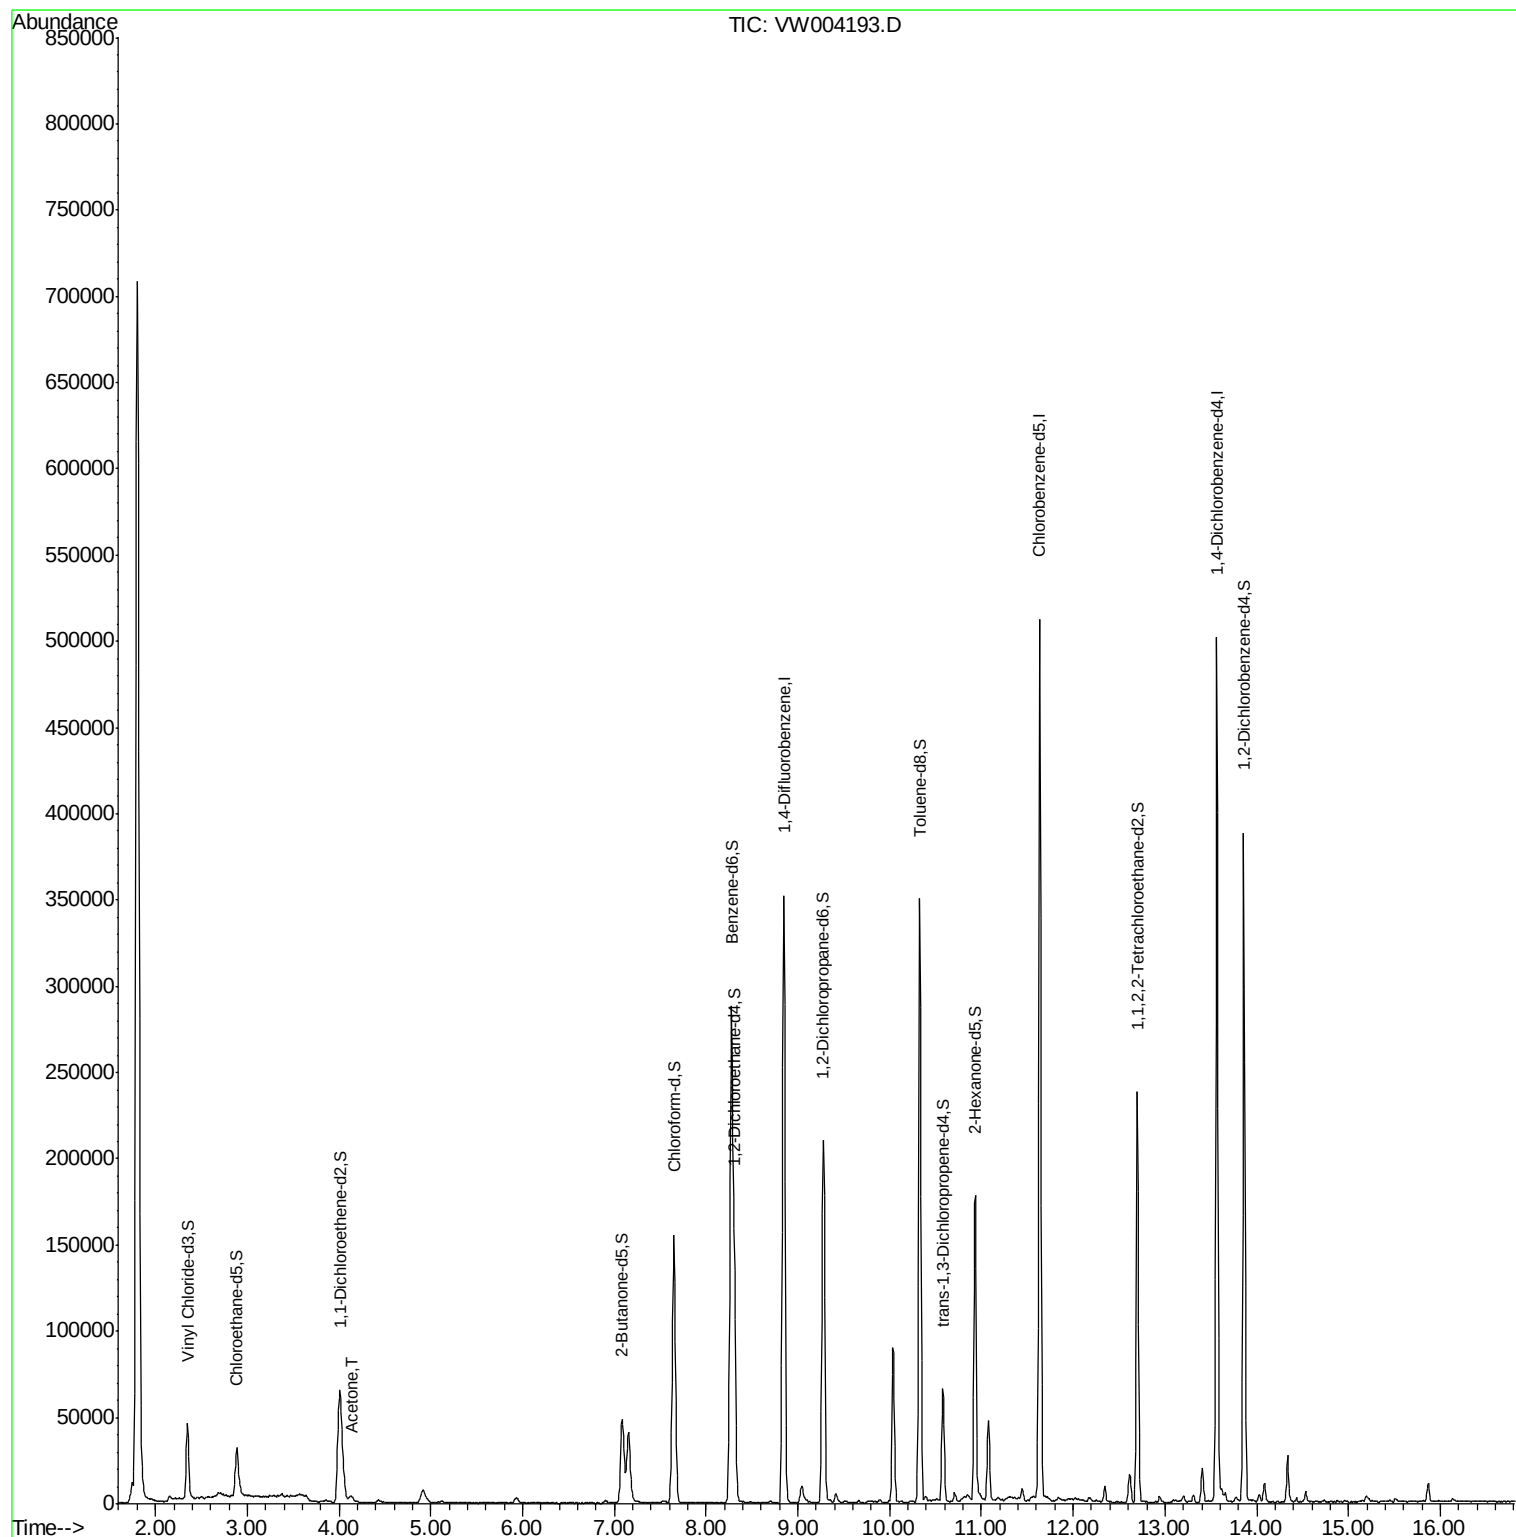

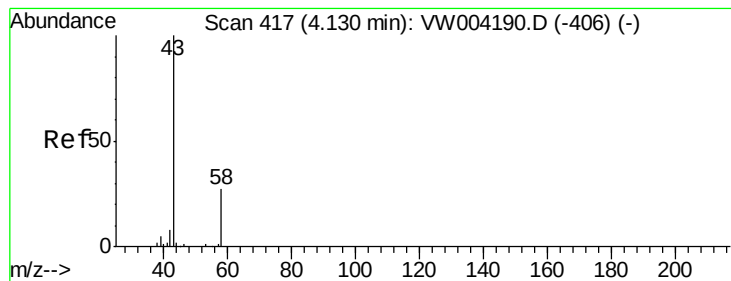

#13
 Acetone
 Concen: 2.362 ug/L
 RT: 4.13 min Scan# 417
 Delta R.T. -0.00 min
 Lab File: VW004193.D
 Acq: 25 Jul 2018 12:09

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AE7

Tot Ion: 43 Resp: 4198
 Ion Ratio Lower Upper
 43 100
 58 31.1 0.0 59.4

