

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW072519\
 Data File : VW011480.D
 Acq On : 24 Jul 2019 17:32
 Operator : SY/VA
 Sample : K3983-04
 Misc : 6.19G/5ML/MSVOA W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SP-4

Quant Time: Jul 25 05:24:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070819S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 11 08:14:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	251014	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	418324	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	333418	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	119970	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	158364	50.21	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.42%	
35) Dibromofluoromethane	7.88	113	126185	50.61	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.22%	
50) Toluene-d8	10.32	98	503268	49.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.86%	
62) 4-Bromofluorobenzene	12.62	95	149344	40.43	ug/l	0.00
Spiked Amount	50.000		Recovery	=	80.86%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW072519\
Data File : VW011480.D
Acq On : 24 Jul 2019 17:32
Operator : SY/VA
Sample : K3983-04
Misc : 6.19G/5ML/MSVOA W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SP-4

Quant Time: Jul 25 05:24:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W070819S.M
Quant Title : SW846 8260
QLast Update : Thu Jul 11 08:14:17 2019
Response via : Initial Calibration

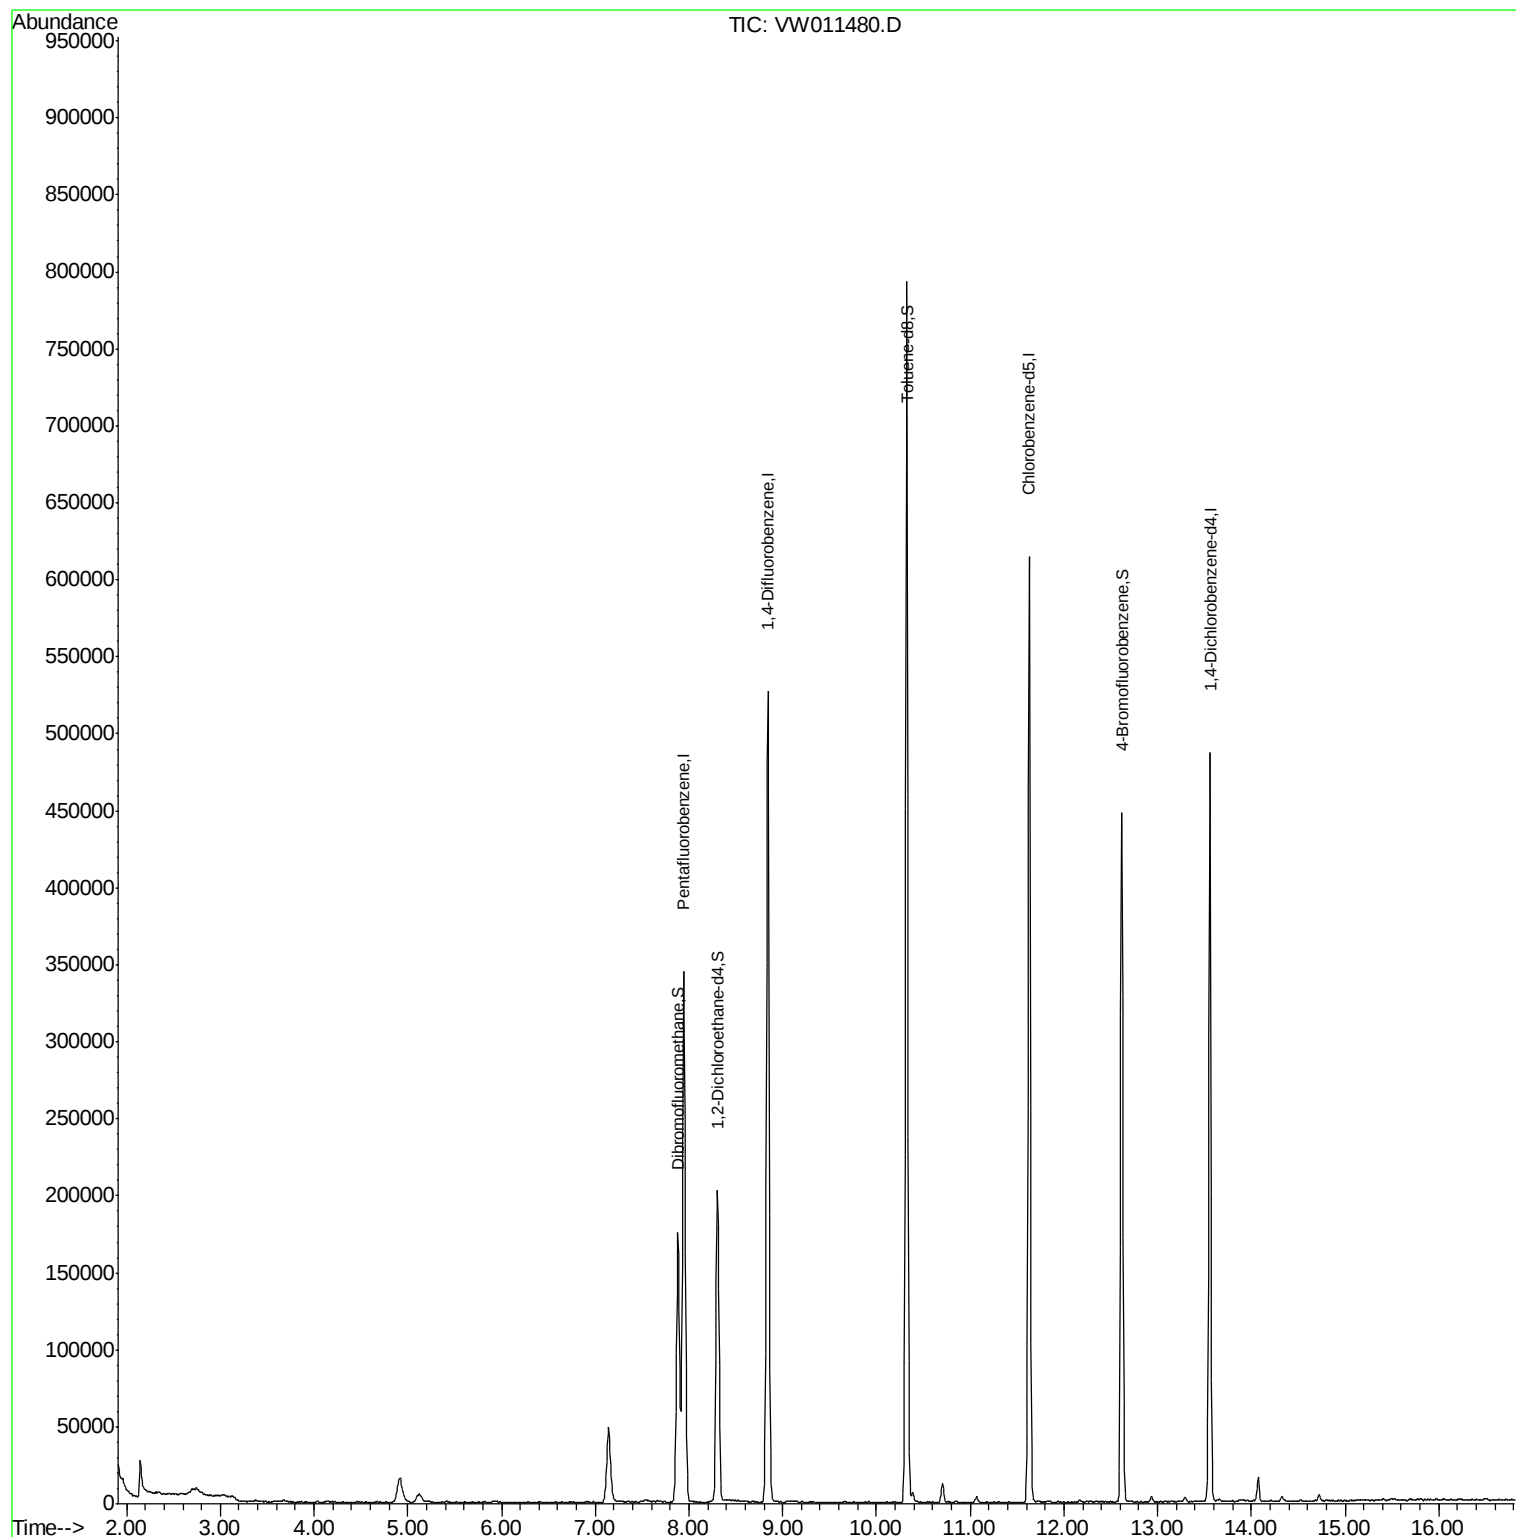

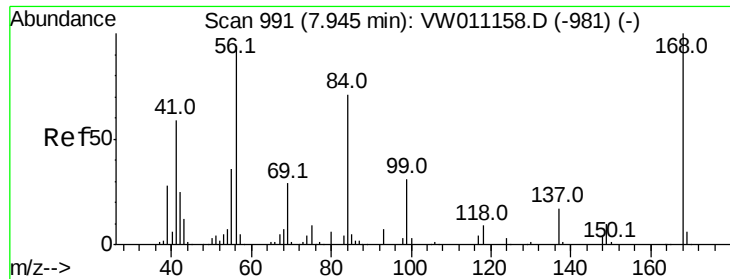

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW011480.D

Acq: 24 Jul 2019 17:32


Instrument :
MSVOA_W
ClientSampled :
SP-4

Tot Ion:168 Resp: 251014

Ion Ratio Lower Upper

168 100

99 61.5 50.1 75.1

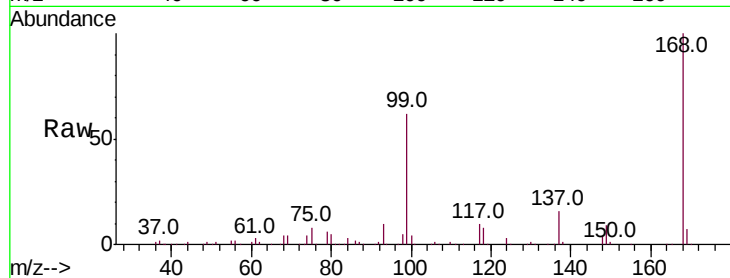

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW



7.95

100000

50000

0

Time--> 7.80 7.90 8.00 8.10

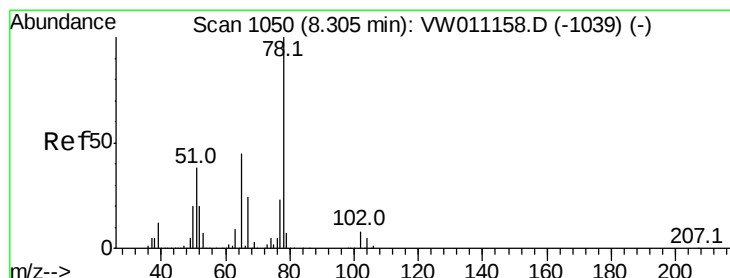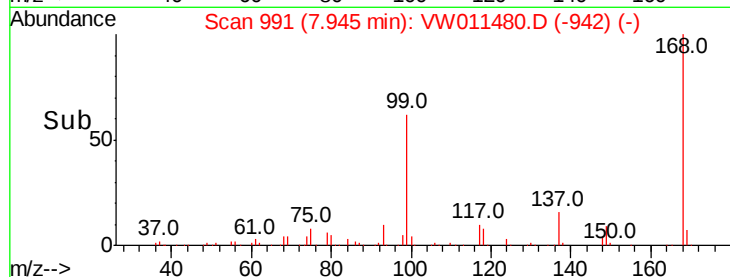

#33

1,2-Dichloroethane-d4

Concen: 50.209 ug/l

RT: 8.30 min Scan# 1050

Delta R.T. 0.00 min

Lab File: VW011480.D


Acq: 24 Jul 2019 17:32

Tgt Ion: 65 Resp: 158364

Ion Ratio Lower Upper

65 100

67 52.5 0.0 104.4

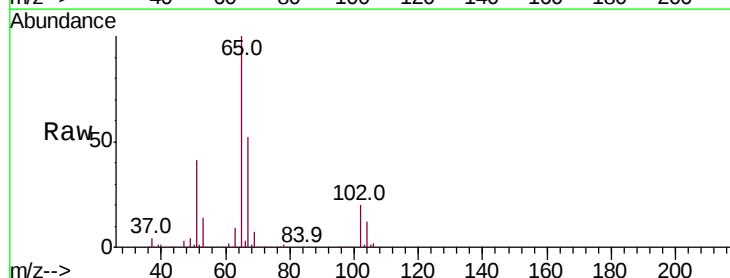

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.30

80000


60000


40000

20000

0

Time--> 8.20 8.30 8.40

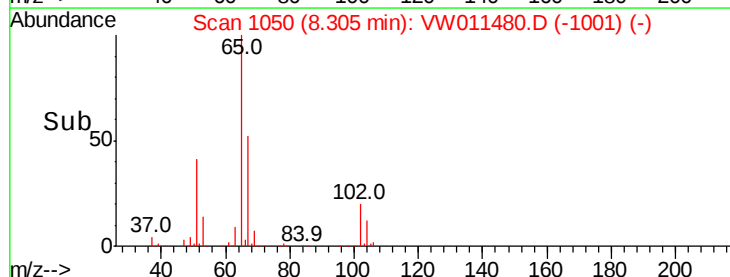


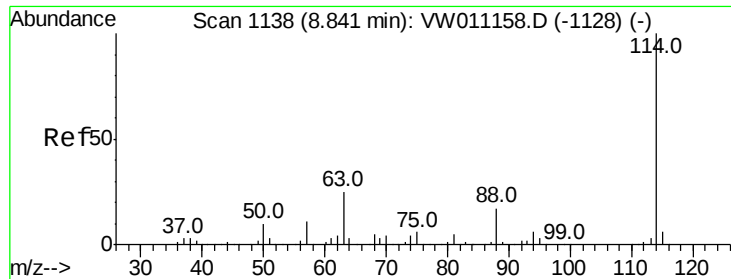




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW011480.D
 Acq: 24 Jul 2019 17:32

Instrument :
 MSVOA_W
 ClientSampleId :
 SP-4

Tot Ion	Ratio	Lower	Upper
114	100		
63	24.1	0.0	50.8
88	16.3	0.0	34.2

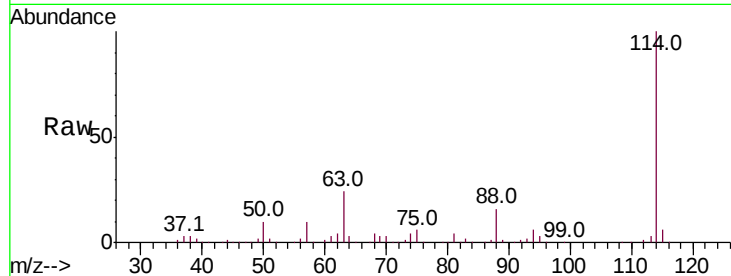


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

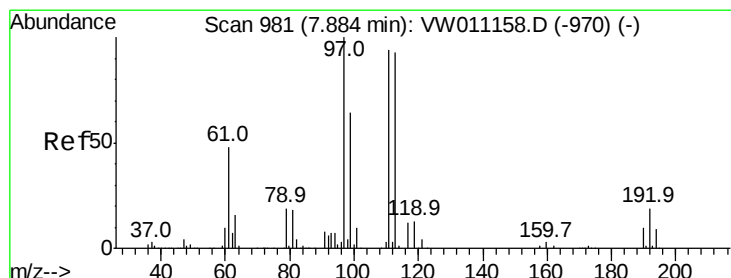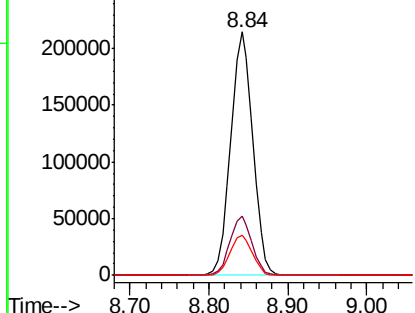
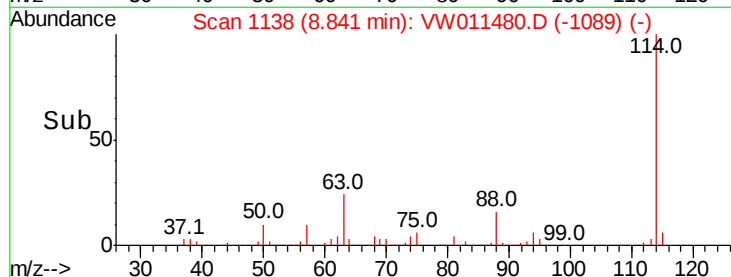



#35
 Dibromofluoromethane
 Concen: 50.608 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.00 min
 Lab File: VW011480.D
 Acq: 24 Jul 2019 17:32

Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.3	82.4	123.6
192	20.5	15.8	23.8

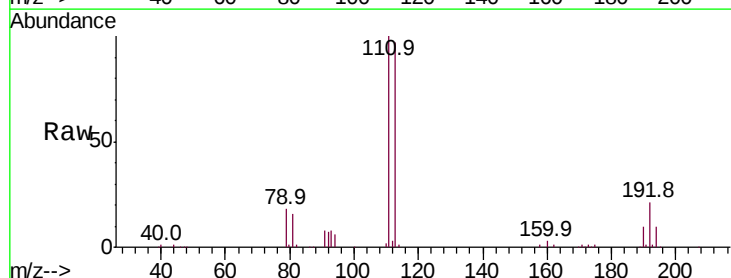

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



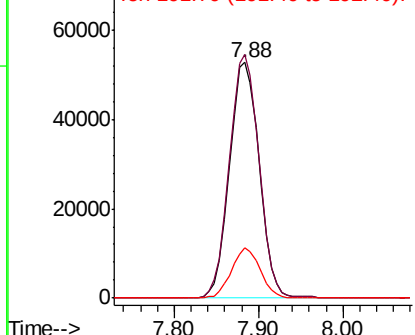
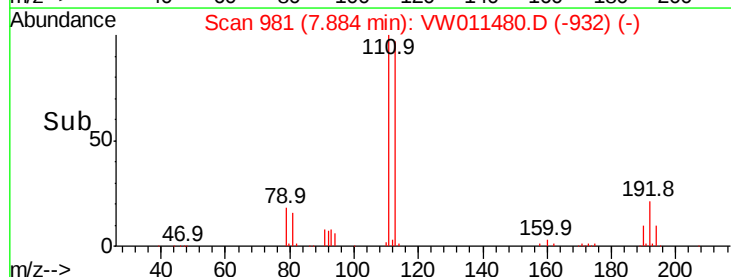


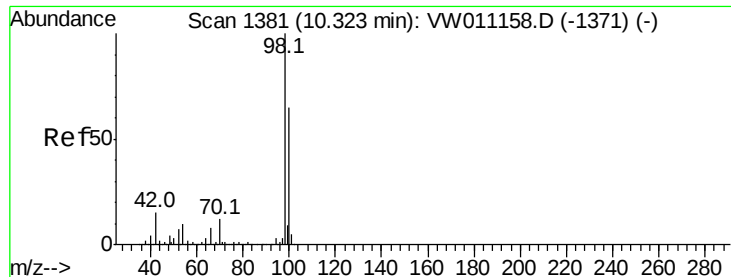

#50
Toluene-d8
Concen: 49.934 ug/l
RT: 10.32 min Scan# 1381
Delta R.T. 0.00 min
Lab File: VW011480.D
Acq: 24 Jul 2019 17:32




Instrument :
MSVOA_W
ClientSampleId :
SP-4


Tot Ion: 98 Resp: 503268
Ion Ratio Lower Upper
98 100
100 65.4 52.4 78.6

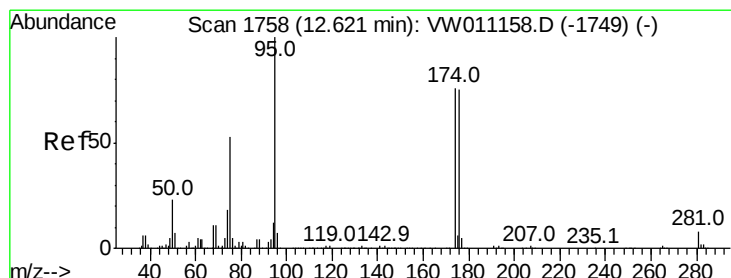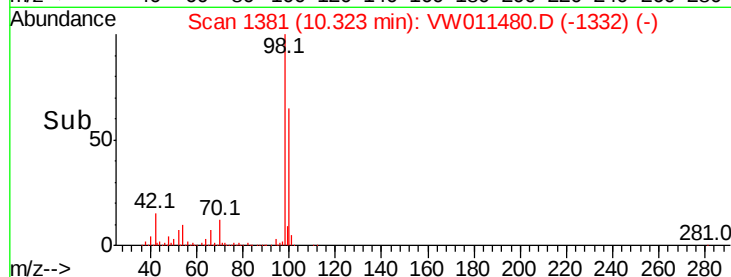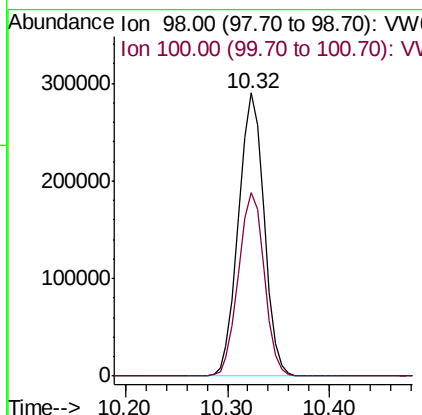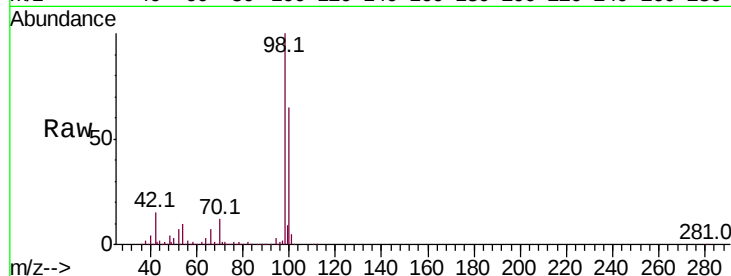

#62
4-Bromofluorobenzene
Concen: 40.427 ug/l
RT: 12.62 min Scan# 1757
Delta R.T. -0.01 min
Lab File: VW011480.D
Acq: 24 Jul 2019 17:32

Tgt Ion: 95 Resp: 149344
Ion Ratio Lower Upper
95 100
174 75.7 0.0 147.6
176 73.9 0.0 144.6


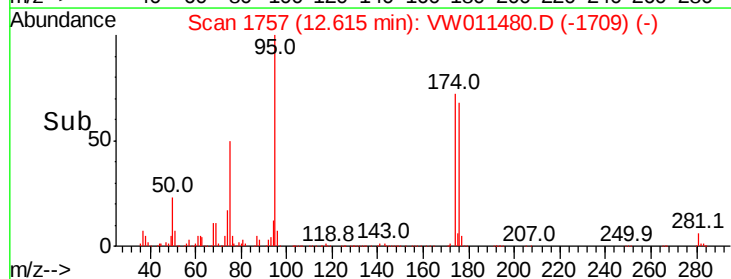
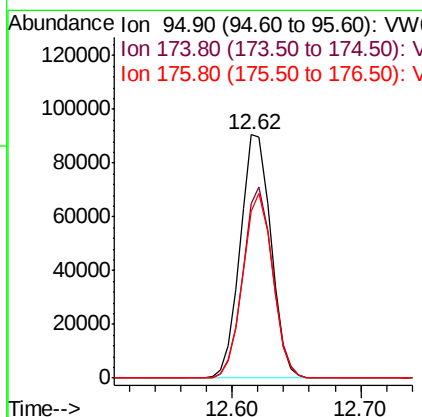
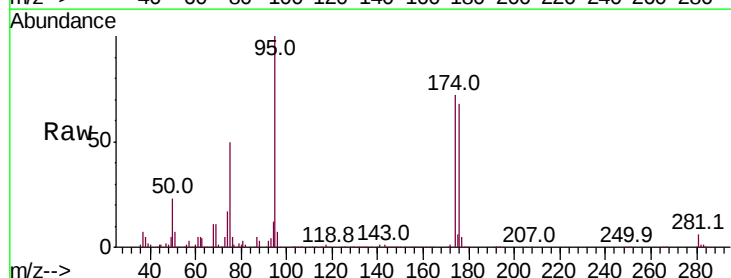


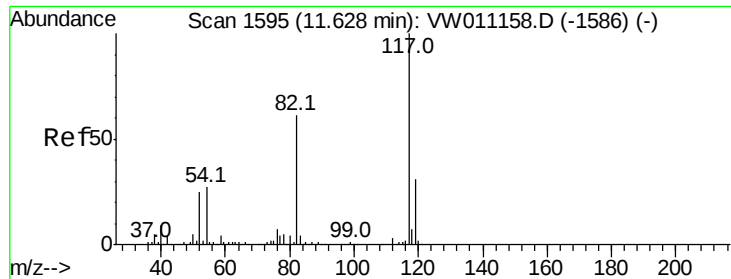

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.01 min
Lab File: VW011480.D
Acq: 24 Jul 2019 17:32

Instrument :
MSVOA_W
ClientSampleId :
SP-4

Tot Ion:117 Resp: 333418
Ion Ratio Lower Upper
117 100
82 59.7 48.9 73.3
119 32.2 25.0 37.6

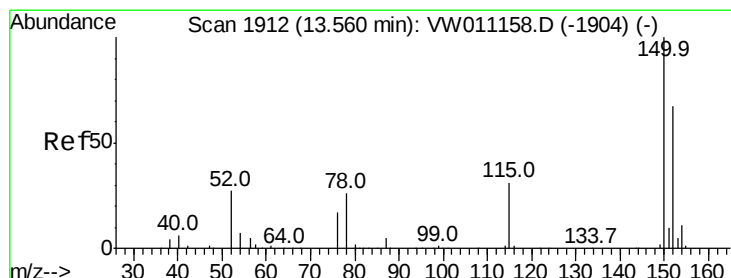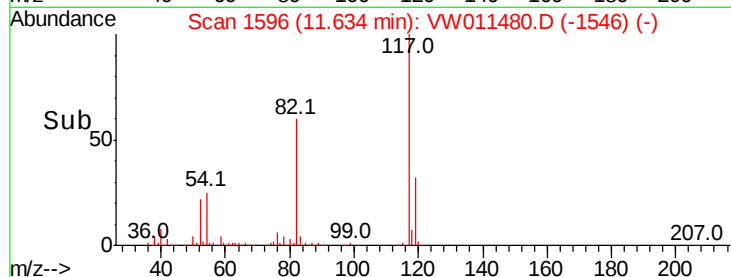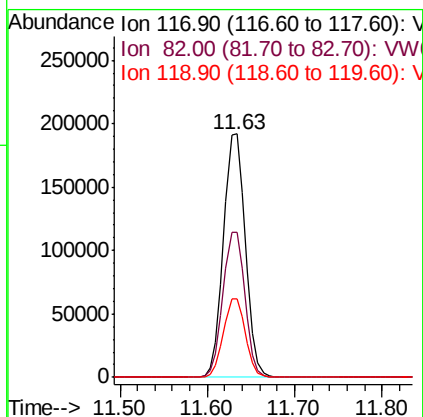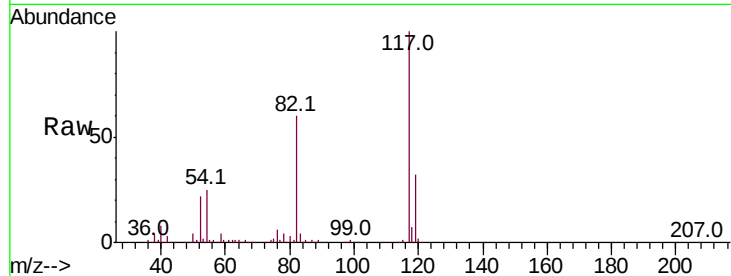

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. 0.00 min
Lab File: VW011480.D
Acq: 24 Jul 2019 17:32

Tgt Ion:152 Resp: 119970
Ion Ratio Lower Upper
152 100
115 59.8 30.1 90.3
150 156.5 0.0 346.0

