


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW072519\  
Data File : VW011463.D  
Acq On : 24 Jul 2019 09:35  
Operator : SY/VA  
Sample : BFB  
Misc : 5.00G/5ML/MSVOA W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W070819S.M  
Title : SW846 8260  
Last Update : Thu Jul 11 08:14:17 2019

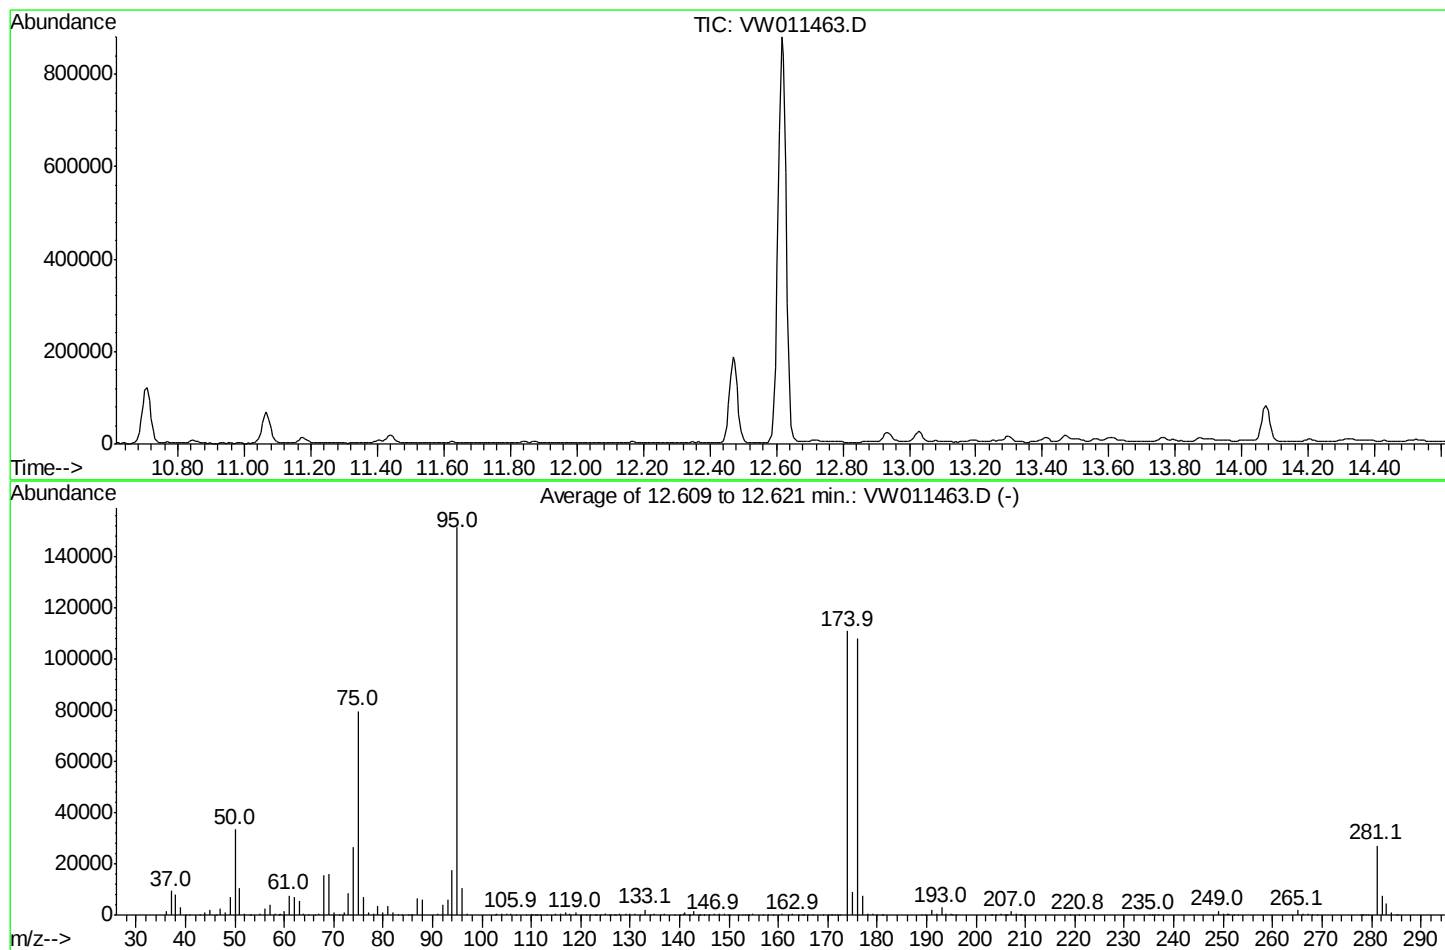

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 22.1      | 33413   | PASS             |
| 75          | 95           | 30           | 60           | 52.5      | 79584   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 151480  | PASS             |
| 96          | 95           | 5            | 9            | 7.1       | 10751   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 73.2      | 110946  | PASS             |
| 175         | 174          | 5            | 9            | 8.1       | 8989    | PASS             |
| 176         | 174          | 95           | 101          | 97.2      | 107882  | PASS             |
| 177         | 176          | 5            | 9            | 7.0       | 7534    | PASS             |