

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024079.D
 Acq On : 25 Jul 2022 19:49
 Operator : SY/VA
 Sample : N3766-05
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Jul 26 01:34:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	202997	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	209580	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	95387	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	133626	30.710	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	122.840%
7) Chloroethane-d5	2.873	69	82170	27.949	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.800%
11) 1,1-Dichloroethene-d2	4.007	63	68419	17.858	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.440%
21) 2-Butanone-d5	7.080	46	39374	50.916	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.840%
24) Chloroform-d	7.647	84	129986	23.292	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.160%
26) 1,2-Dichloroethane-d4	8.305	65	78492	24.481	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.920%
32) Benzene-d6	8.268	84	238740	24.522	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.080%
36) 1,2-Dichloropropane-d6	9.274	67	74762	24.346	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.400%
41) Toluene-d8	10.323	98	224535	23.061	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.240%
43) trans-1,3-Dichloroprop...	10.579	79	30555	22.442	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.760%
47) 2-Hexanone-d5	10.920	63	30731	47.869	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.740%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	76733	21.656	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.640%
66) 1,2-Dichlorobenzene-d4	13.847	152	75321	24.382	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.520%
Target Compounds						
16) Methylene chloride	4.915	84	21531	6.969	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
Data File : VW024079.D
Acq On : 25 Jul 2022 19:49
Operator : SY/VA
Sample : N3766-05
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Jul 26 01:34:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 01:30:33 2022
Response via : Initial Calibration

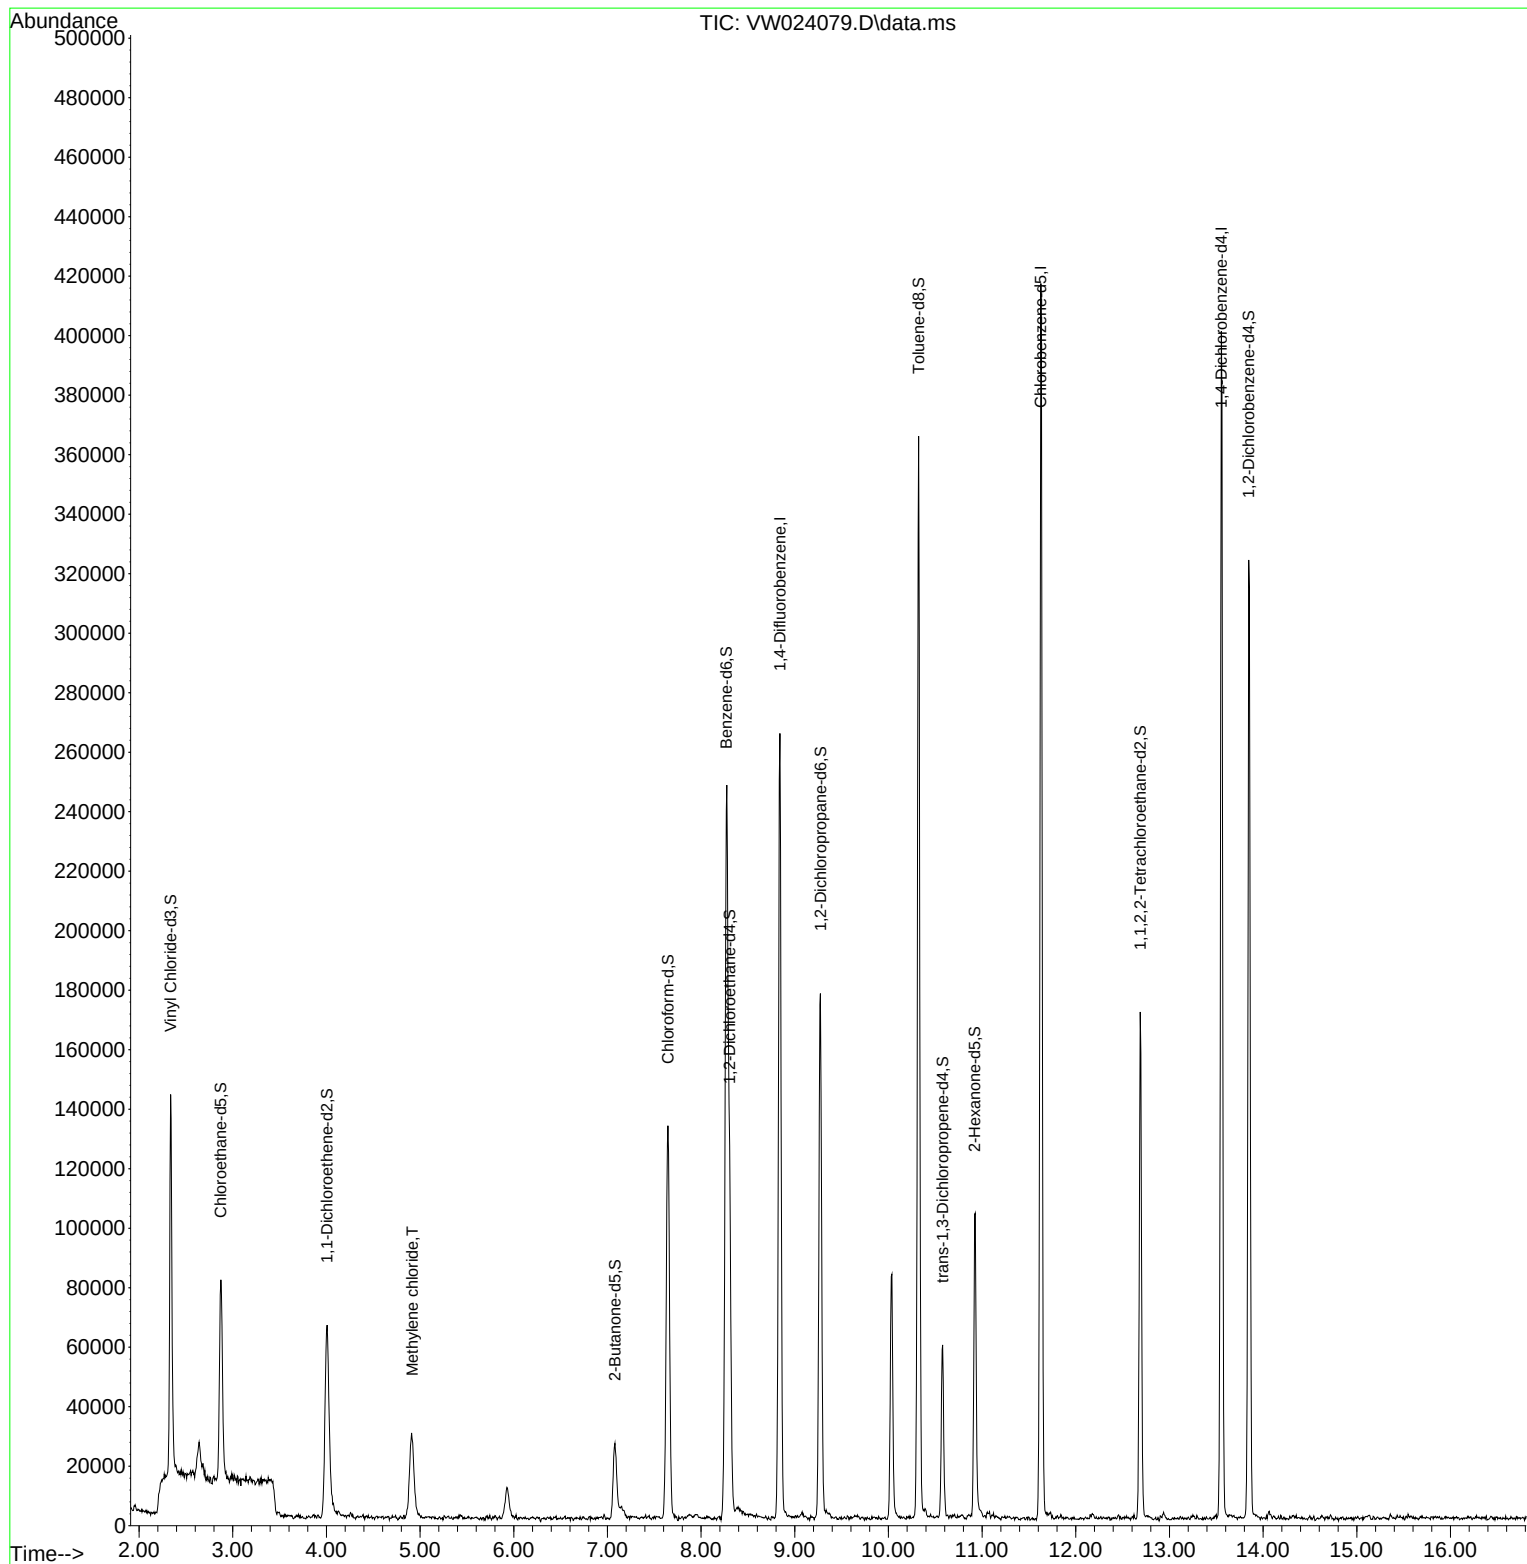

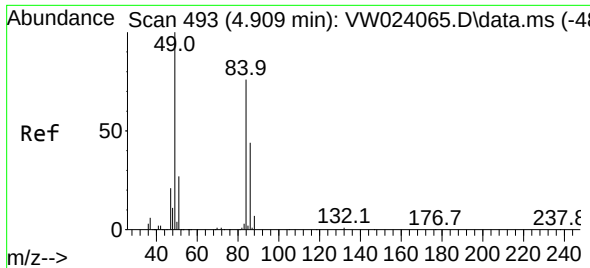

#16
Methylene chloride
Concen: 6.969 ug/L
RT: 4.915 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW024079.D
Acq: 25 Jul 2022 19:49

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Tgt Ion: 84 Resp: 21531
Ion Ratio Lower Upper
84 100
86 66.6 44.7 83.1
49 138.4 83.7 155.4

