

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024083.D
 Acq On : 25 Jul 2022 21:27
 Operator : SY/VA
 Sample : N3743-22
 Misc : 5.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Jul 26 01:35:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	187820	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	198815	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	88695	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	123575	30.695	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	122.760%
7) Chloroethane-d5	2.879	69	75490	27.752	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.000%
11) 1,1-Dichloroethene-d2	4.007	63	62271	17.566	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.280%
21) 2-Butanone-d5	7.080	46	37416	52.293	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.580%
24) Chloroform-d	7.640	84	121538	23.538	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.160%
26) 1,2-Dichloroethane-d4	8.305	65	73969	24.934	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.720%
32) Benzene-d6	8.275	84	220852	23.913	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.640%
36) 1,2-Dichloropropane-d6	9.268	67	68805	23.620	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.480%
41) Toluene-d8	10.323	98	209636	22.697	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.800%
43) trans-1,3-Dichloroprop...	10.579	79	26606	20.599	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.400%
47) 2-Hexanone-d5	10.920	63	28550	46.880	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.760%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	72981	21.713	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	71841	25.010	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.040%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	21674	7.582	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
Data File : VW024083.D
Acq On : 25 Jul 2022 21:27
Operator : SY/VA
Sample : N3743-22
Misc : 5.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Jul 26 01:35:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 01:30:33 2022
Response via : Initial Calibration

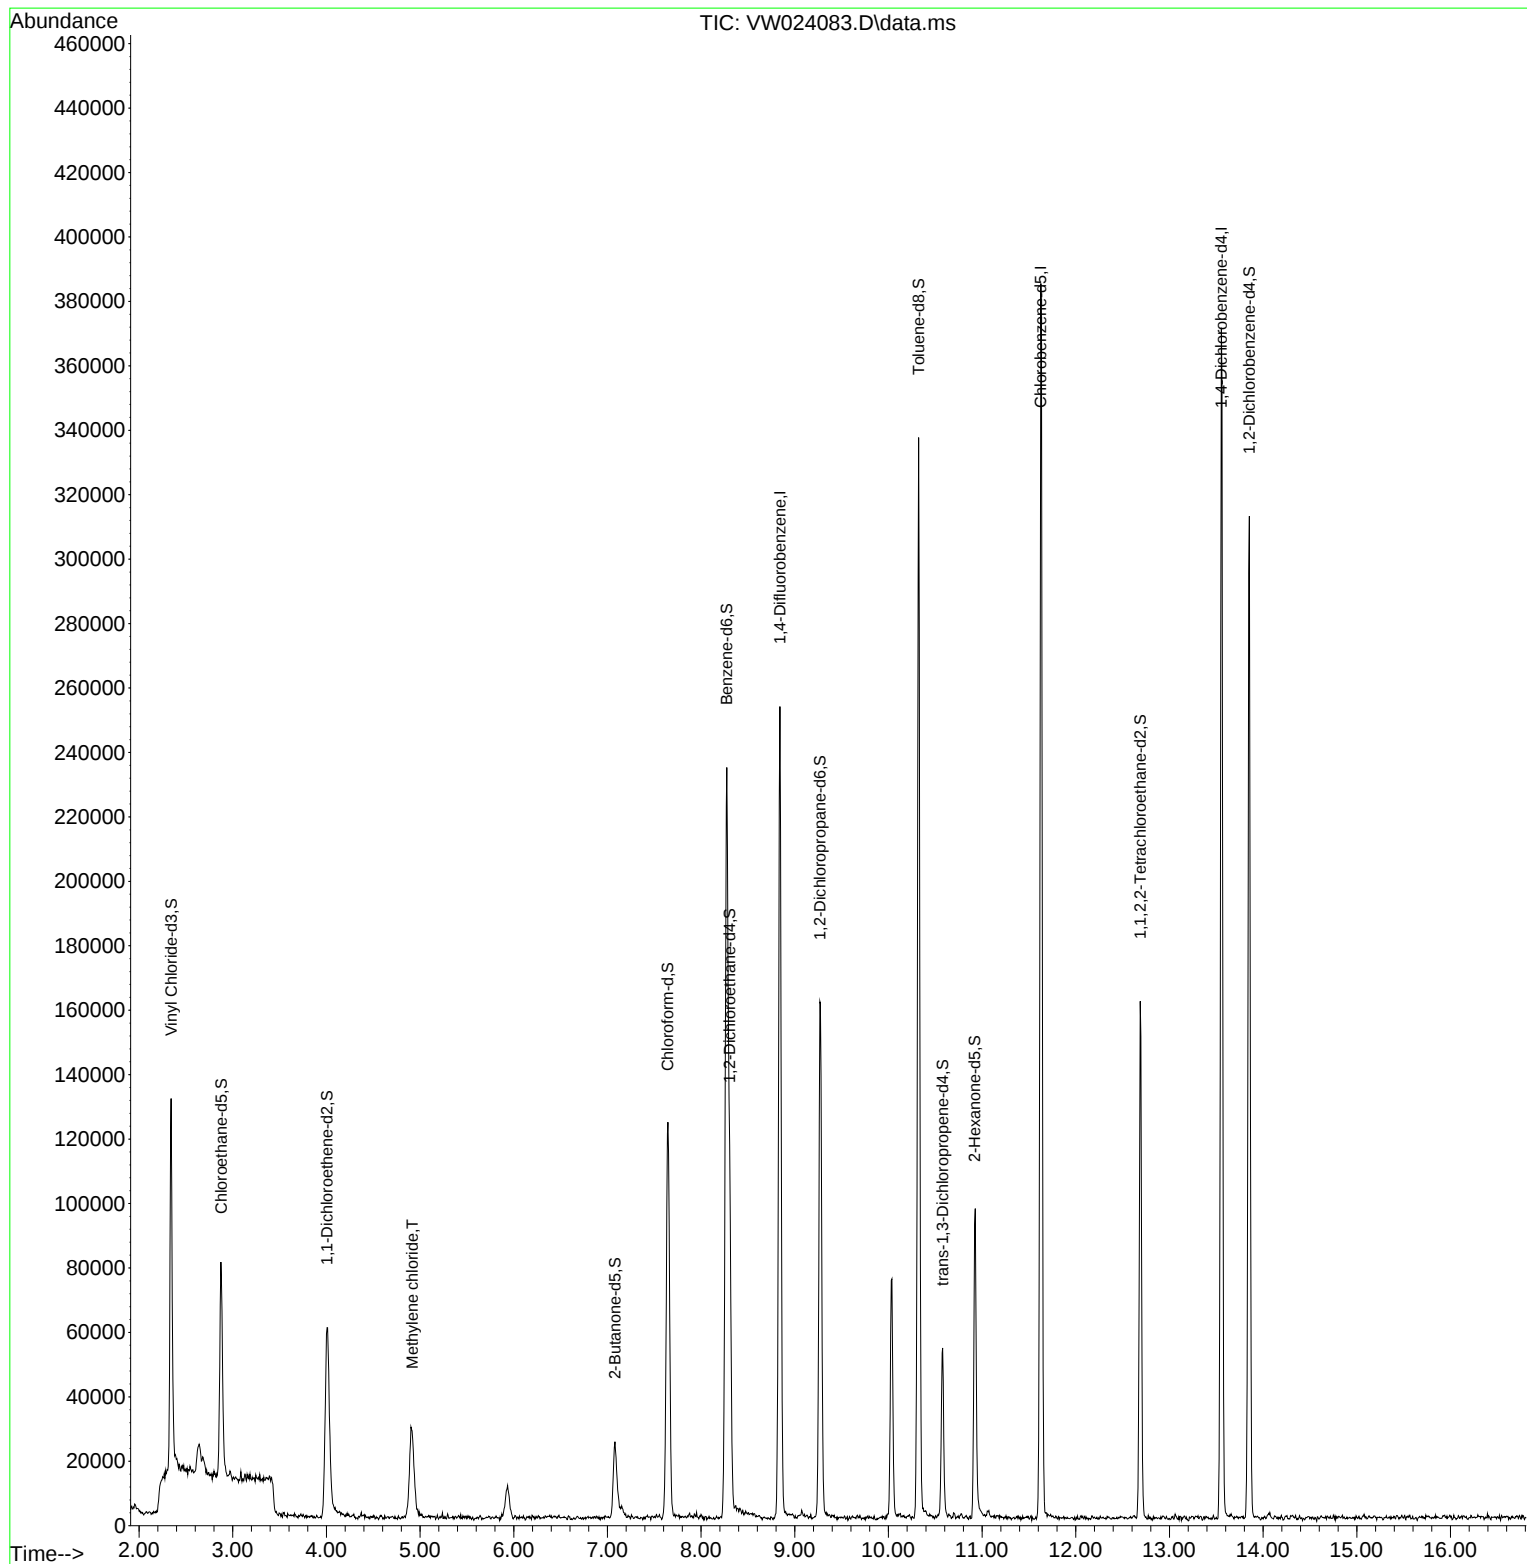

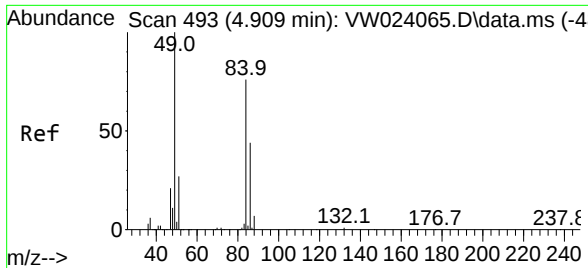

#16
Methylene chloride
Concen: 7.582 ug/L
RT: 4.915 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW024083.D
Acq: 25 Jul 2022 21:27

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Tgt Ion:	84	Resp:	21674
Ion	Ratio	Lower	Upper
84	100		
86	60.2	44.7	83.1
49	134.5	83.7	155.4

