




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW072522\  
 Data File : VW024072.D  
 Acq On : 25 Jul 2022 16:55  
 Operator : SY/VA  
 Sample : N3823-02  
 Misc : 7.01g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 H0B61

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:33:16 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM072522SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Tue Jul 26 01:30:33 2022  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/26/2022  
 Supervised By :Mahesh Dadoda 07/26/2022

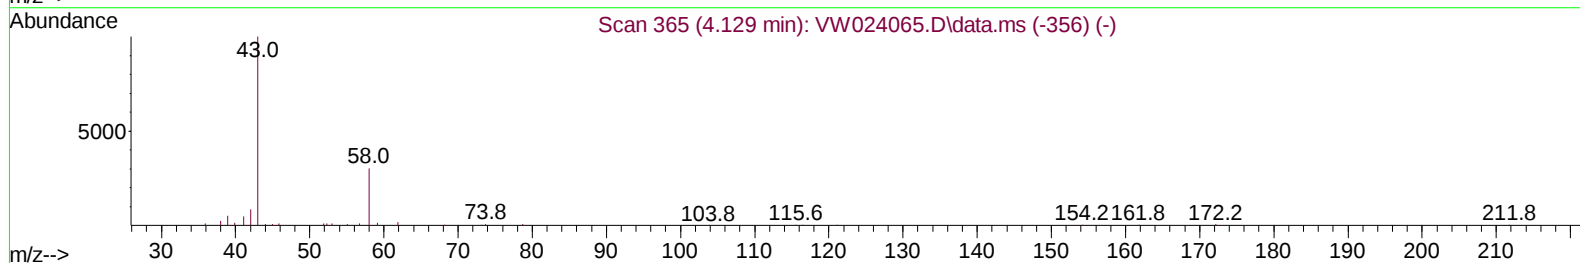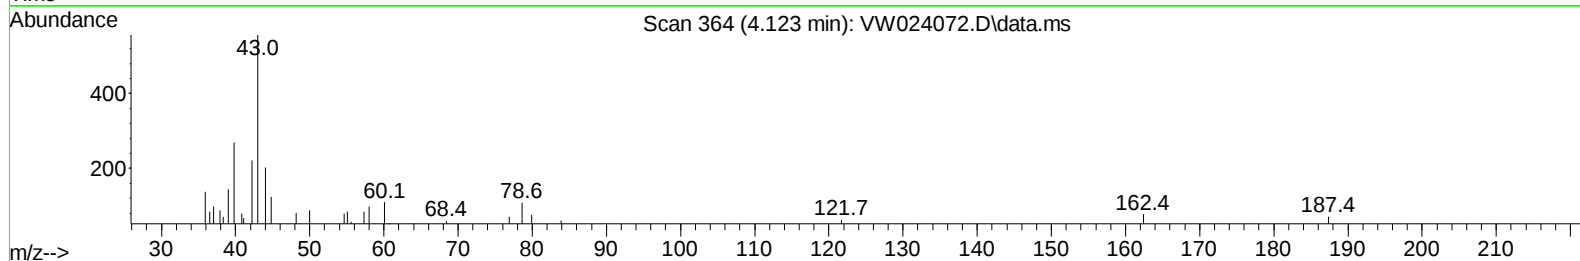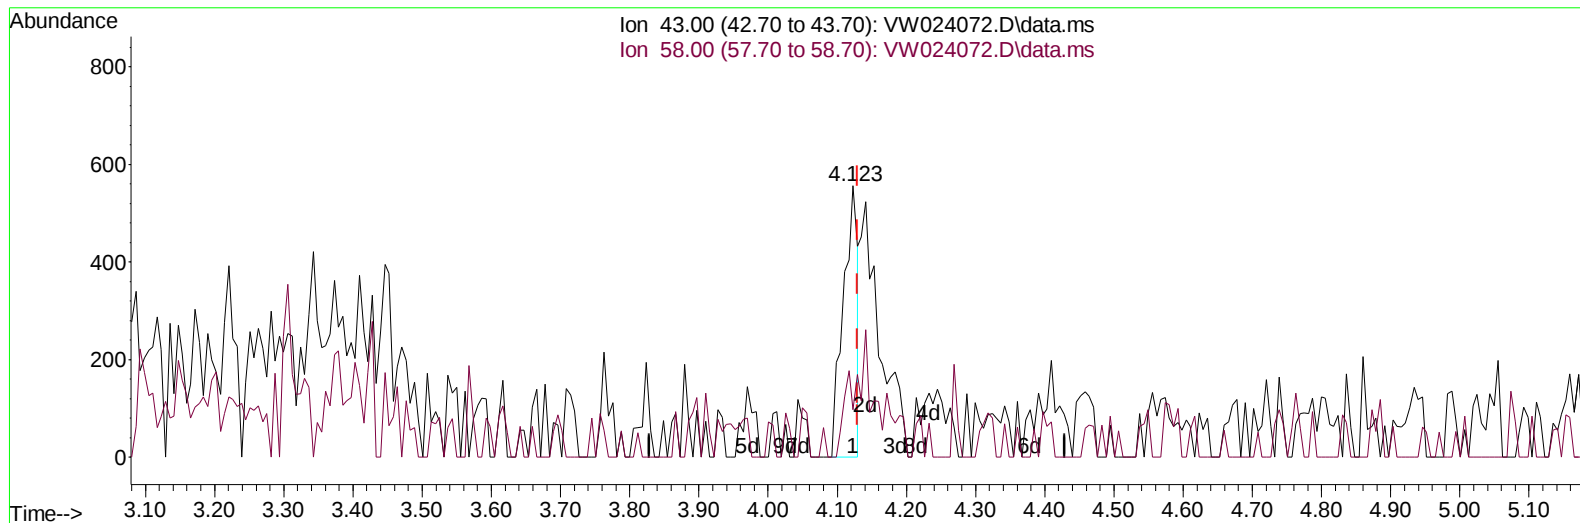

TIC: VW024072.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 4.21 ug/L

response 798

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 58.00 | 30.00  | 20.68  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW072522\  
Data File : VW024072.D  
Acq On : 25 Jul 2022 16:55  
Operator : SY/VA  
Sample : N3823-02  
Misc : 7.01g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
H0B61

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:33:16 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM072522SMA.M  
Quant Title : SFAM01.0  
QLast Update : Tue Jul 26 01:30:33 2022  
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/26/2022  
Supervised By :Mahesh Dadoda 07/26/2022

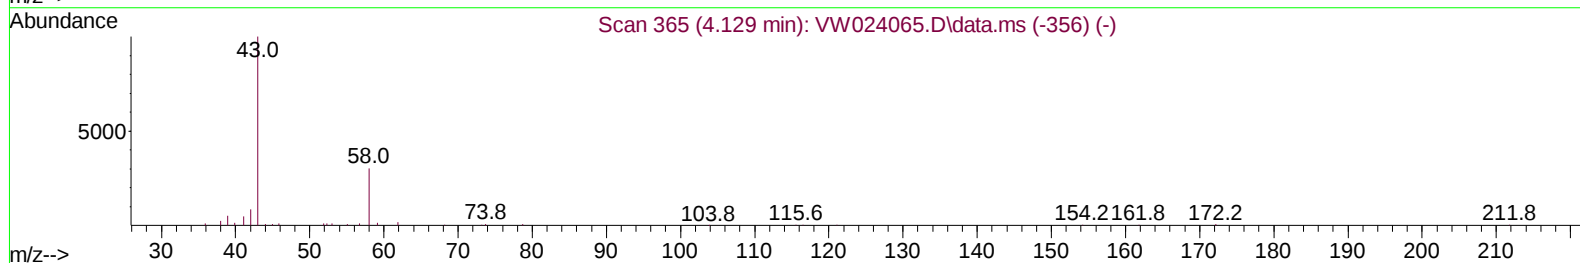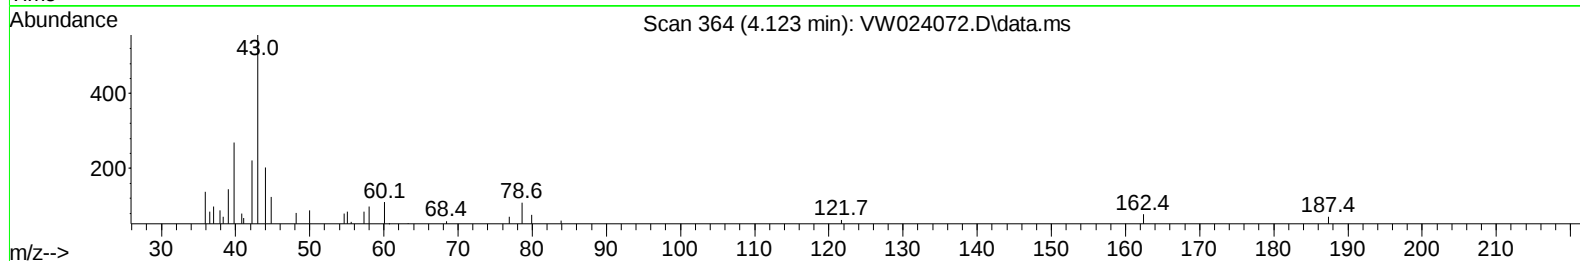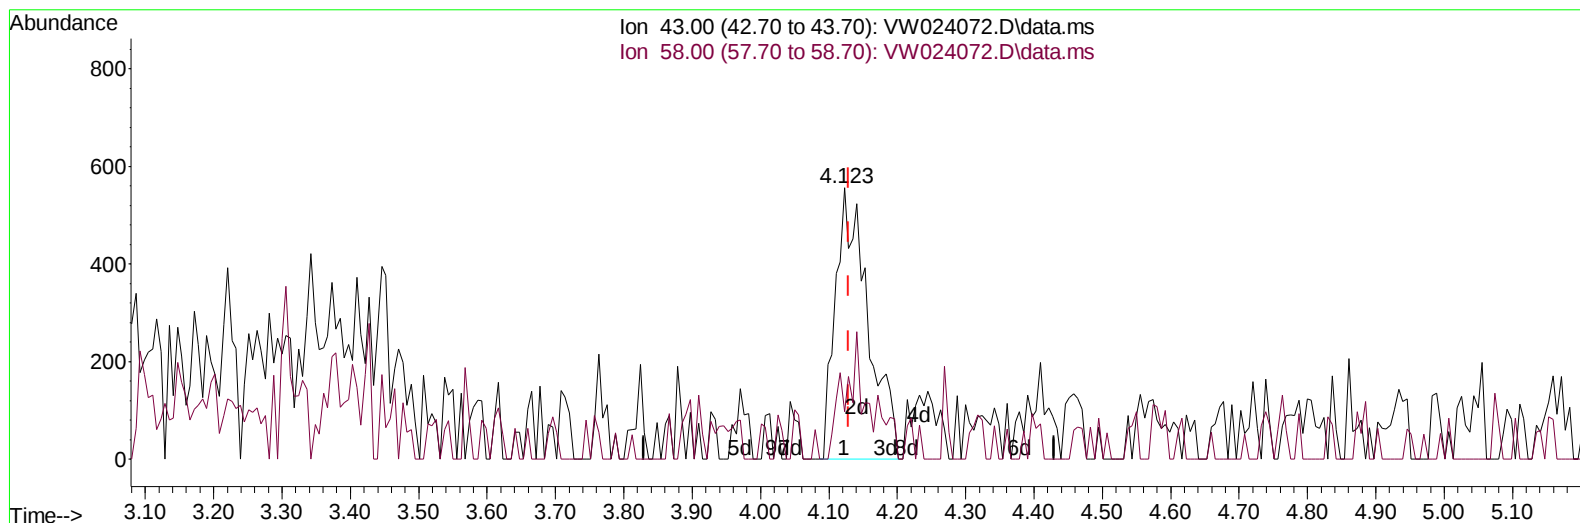

TIC: VW024072.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 9.68 ug/L m

response 1836

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 58.00 | 30.00  | 8.99   |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW072522\  
 Data File : VW024072.D  
 Acq On : 25 Jul 2022 16:55  
 Operator : SY/VA  
 Sample : N3823-02  
 Misc : 7.01g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 H0B61

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:33:16 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM072522SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Tue Jul 26 01:30:33 2022  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/26/2022  
 Supervised By :Mahesh Dadoda 07/26/2022

| Compound                      | R.T.     | QIon  | Response | Conc   | Units     | Dev(Min) |
|-------------------------------|----------|-------|----------|--------|-----------|----------|
| -----                         |          |       |          |        |           |          |
| Internal Standards            |          |       |          |        |           |          |
| 1) 1,4-Difluorobenzene        | 8.841    | 114   | 70192    | 25.000 | ug/L      | 0.00     |
| 28) Chlorobenzene-d5          | 11.634   | 117   | 73140    | 25.000 | ug/L      | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 13.554   | 152   | 30856    | 25.000 | ug/L      | 0.00     |
| System Monitoring Compounds   |          |       |          |        |           |          |
| 4) Vinyl Chloride-d3          | 2.336    | 65    | 45192    | 30.036 | ug/L      | 0.00     |
| Spiked Amount 25.000          | Range 30 | - 150 | Recovery | =      | 120.160%  |          |
| 7) Chloroethane-d5            | 2.873    | 69    | 26722    | 26.286 | ug/L      | 0.00     |
| Spiked Amount 25.000          | Range 30 | - 150 | Recovery | =      | 105.160%  |          |
| 11) 1,1-Dichloroethene-d2     | 4.001    | 63    | 29003    | 21.892 | ug/L      | -0.01    |
| Spiked Amount 25.000          | Range 45 | - 110 | Recovery | =      | 87.560%   |          |
| 21) 2-Butanone-d5             | 7.080    | 46    | 23833    | 89.130 | ug/L      | 0.00     |
| Spiked Amount 50.000          | Range 20 | - 135 | Recovery | =      | 178.260%# |          |
| 24) Chloroform-d              | 7.647    | 84    | 53327    | 27.635 | ug/L      | 0.00     |
| Spiked Amount 25.000          | Range 40 | - 150 | Recovery | =      | 110.520%  |          |
| 26) 1,2-Dichloroethane-d4     | 8.305    | 65    | 34919    | 31.496 | ug/L      | 0.00     |
| Spiked Amount 25.000          | Range 70 | - 130 | Recovery | =      | 126.000%  |          |
| 32) Benzene-d6                | 8.268    | 84    | 87464    | 25.743 | ug/L      | 0.00     |
| Spiked Amount 25.000          | Range 20 | - 135 | Recovery | =      | 102.960%  |          |
| 36) 1,2-Dichloropropane-d6    | 9.268    | 67    | 29382    | 27.417 | ug/L      | 0.00     |
| Spiked Amount 25.000          | Range 70 | - 120 | Recovery | =      | 109.680%  |          |
| 41) Toluene-d8                | 10.323   | 98    | 71866    | 21.150 | ug/L      | 0.00     |
| Spiked Amount 25.000          | Range 30 | - 130 | Recovery | =      | 84.600%   |          |
| 43) trans-1,3-Dichloroprop... | 10.579   | 79    | 11950    | 25.150 | ug/L      | 0.00     |
| Spiked Amount 25.000          | Range 30 | - 135 | Recovery | =      | 100.600%  |          |
| 47) 2-Hexanone-d5             | 10.926   | 63    | 14806    | 66.086 | ug/L      | 0.00     |
| Spiked Amount 50.000          | Range 20 | - 135 | Recovery | =      | 132.180%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 12.694   | 84    | 37817    | 30.584 | ug/L      | 0.00     |
| Spiked Amount 25.000          | Range 45 | - 120 | Recovery | =      | 122.320%# |          |
| 66) 1,2-Dichlorobenzene-d4    | 13.853   | 152   | 28382    | 28.402 | ug/L      | 0.00     |
| Spiked Amount 25.000          | Range 75 | - 120 | Recovery | =      | 113.600%  |          |
| Target Compounds              |          |       |          |        |           |          |
| 13) Acetone                   | 4.123    | 43    | 1836m    | 9.676  | ug/L      |          |
| 16) Methylene chloride        | 4.903    | 84    | 5908     | 5.530  | ug/L      | 97       |
| -----                         |          |       |          |        |           |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW072522\  
Data File : VW024072.D  
Acq On : 25 Jul 2022 16:55  
Operator : SY/VA  
Sample : N3823-02  
Misc : 7.01g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
H0B61

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/26/2022  
Supervised By :Mahesh Dadoda 07/26/2022

Quant Time: Jul 26 01:33:16 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM072522SMA.M  
Quant Title : SFAM01.0  
QLast Update : Tue Jul 26 01:30:33 2022  
Response via : Initial Calibration

