




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024073.D
 Acq On : 25 Jul 2022 17:20
 Operator : SY/VA
 Sample : N3823-03
 Misc : 7.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B62

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:33:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/26/2022
 Supervised By :Mahesh Dadoda 07/26/2022

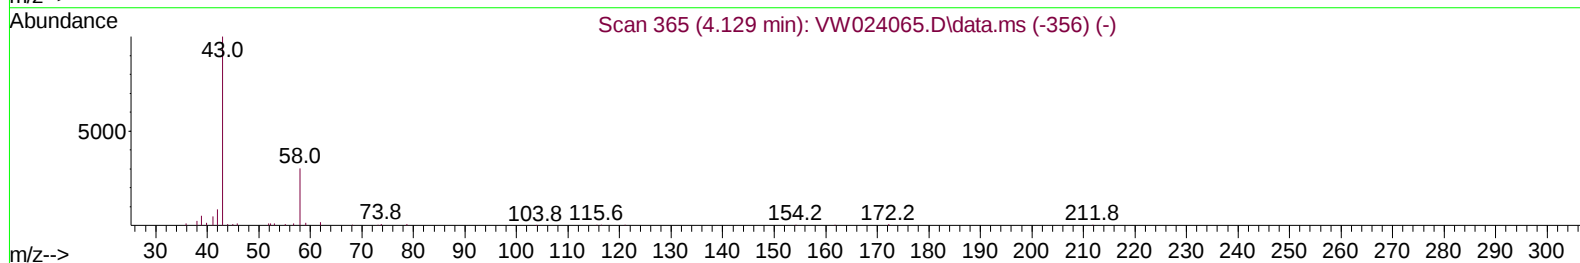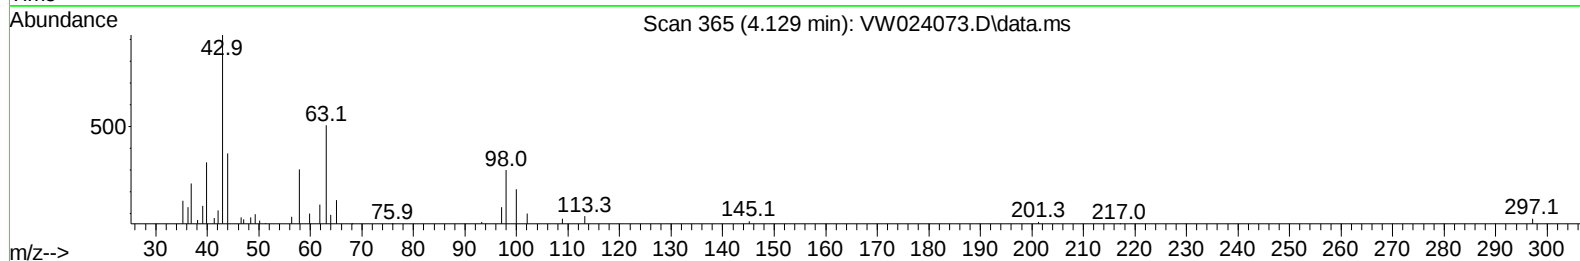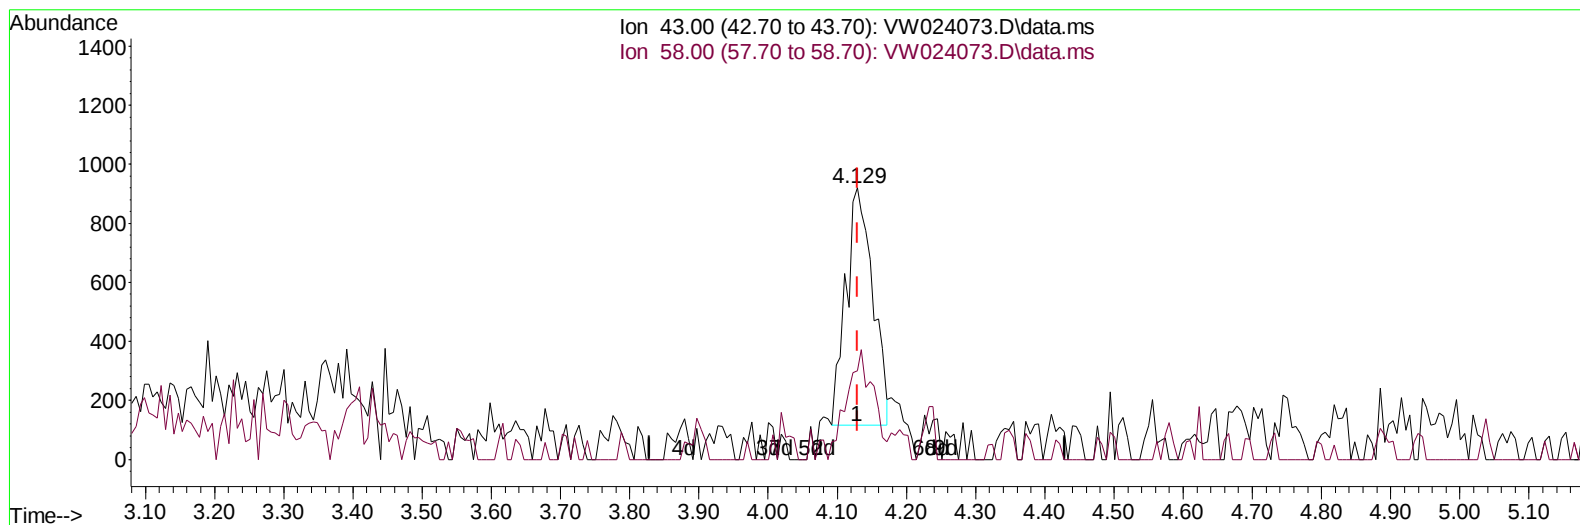

TIC: VW024073.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 3.50 ug/L

response 2163

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.00	32.18
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024073.D
 Acq On : 25 Jul 2022 17:20
 Operator : SY/VA
 Sample : N3823-03
 Misc : 7.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B62

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:33:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/26/2022
 Supervised By :Mahesh Dadoda 07/26/2022

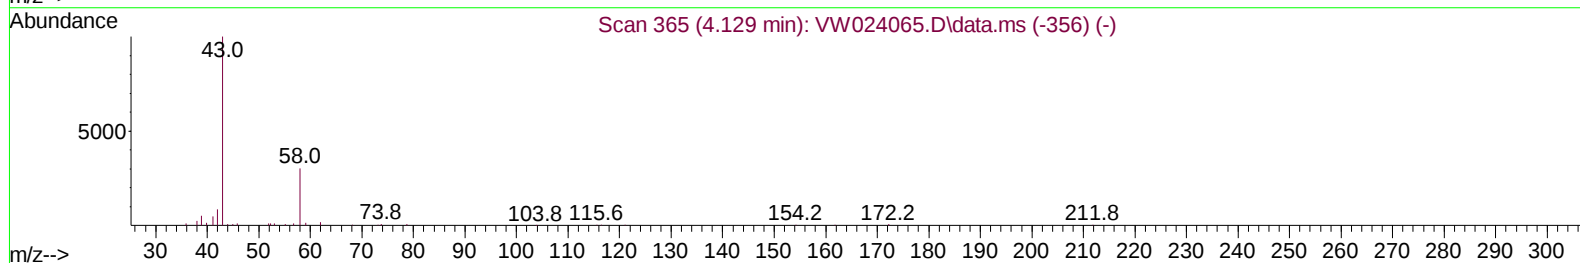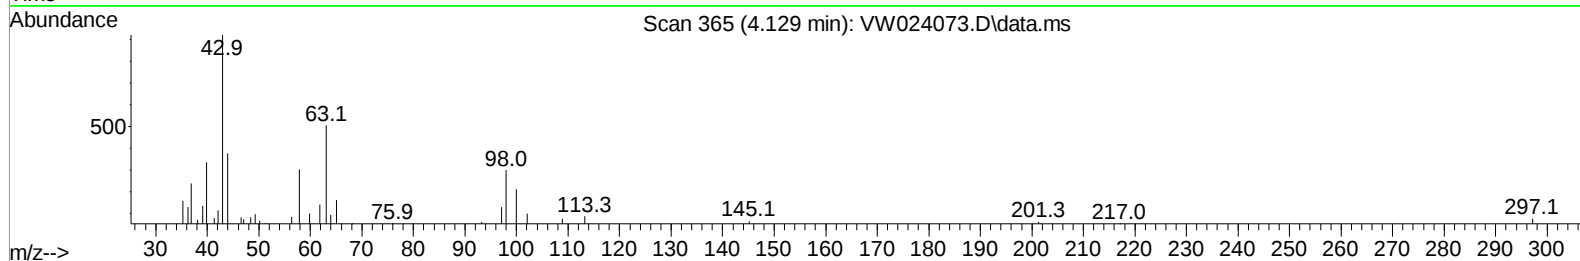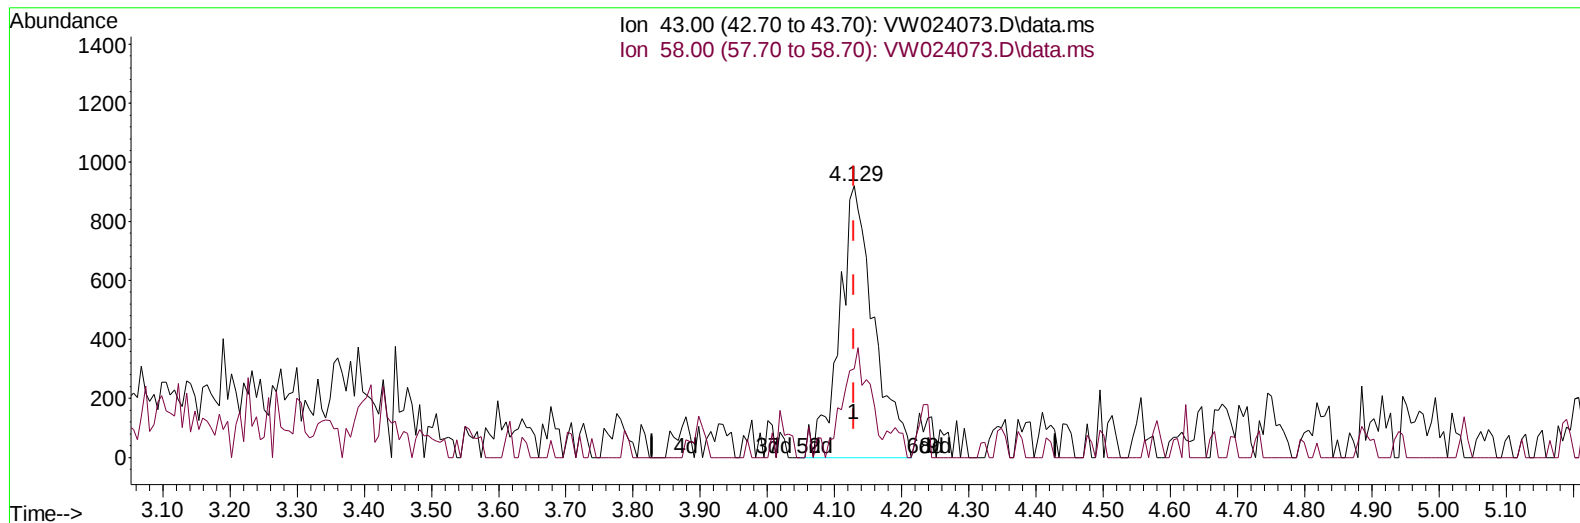

TIC: VW024073.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 5.32 ug/L m

response 3282

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.00	21.21
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024073.D
 Acq On : 25 Jul 2022 17:20
 Operator : SY/VA
 Sample : N3823-03
 Misc : 7.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B62

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:33:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/26/2022
 Supervised By :Mahesh Dadoda 07/26/2022

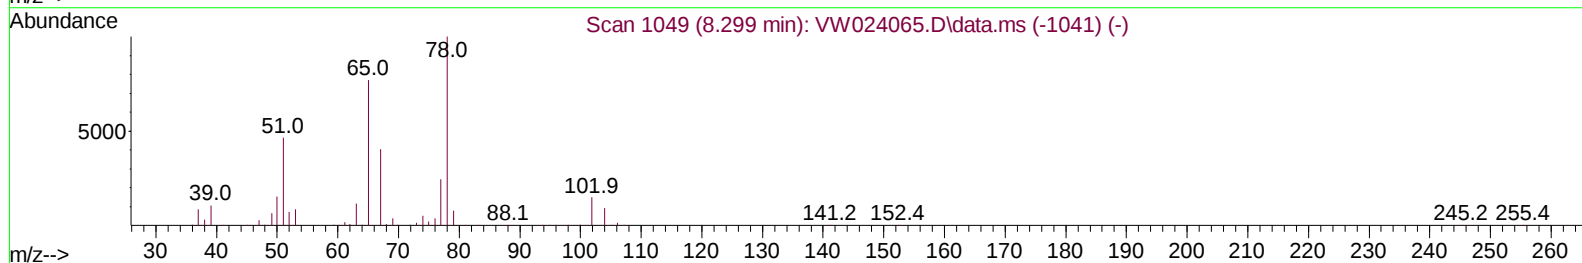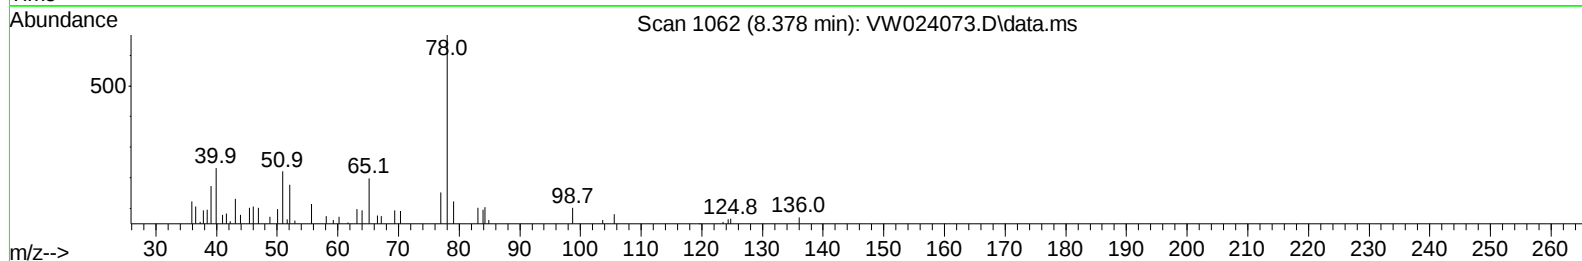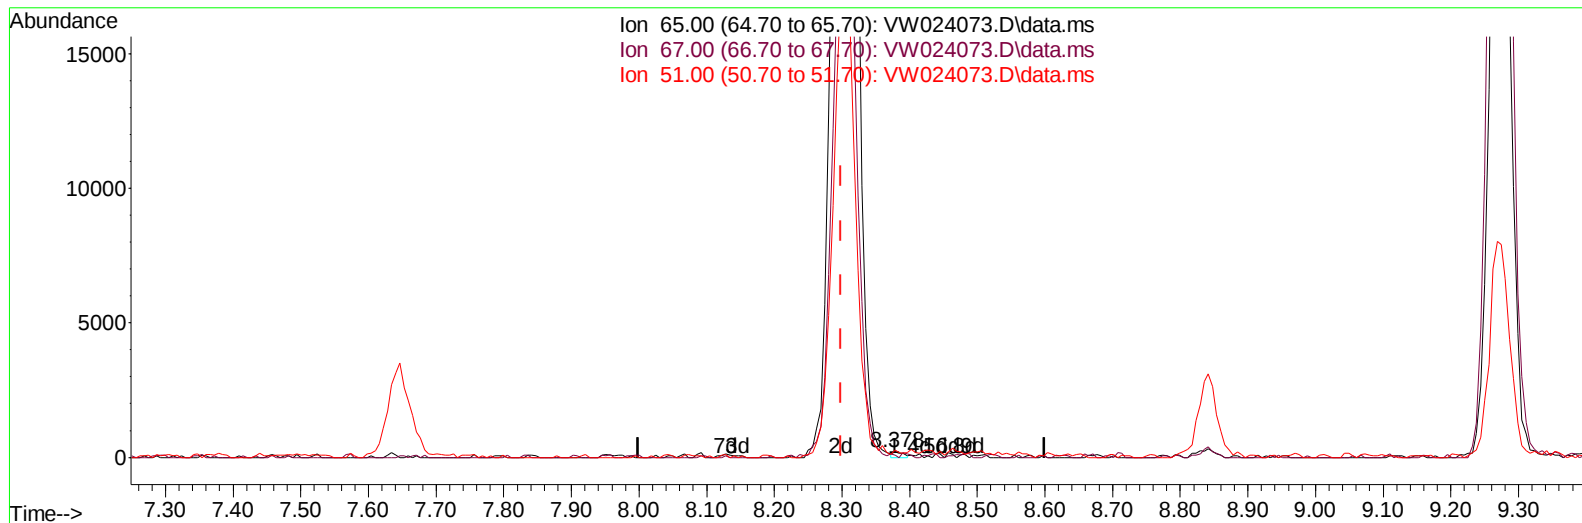

TIC: VW024073.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.378min (+ 0.079) 0.06 ug/L

response 208

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	50.40	37.50
51.00	101.90	75.96
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
Data File : VW024073.D
Acq On : 25 Jul 2022 17:20
Operator : SY/VA
Sample : N3823-03
Misc : 7.36g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
H0B62

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/26/2022
Supervised By :Mahesh Dadoda 07/26/2022

Quant Time: Jul 26 01:33:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 01:30:33 2022
Response via : Initial Calibration

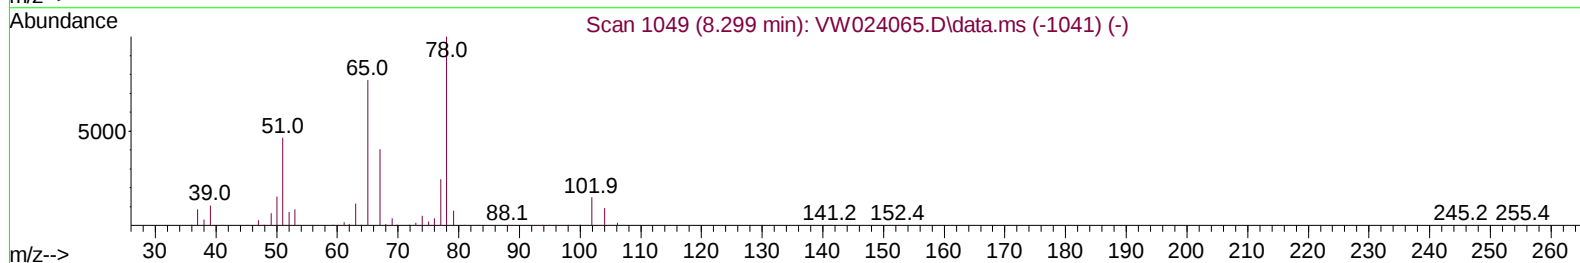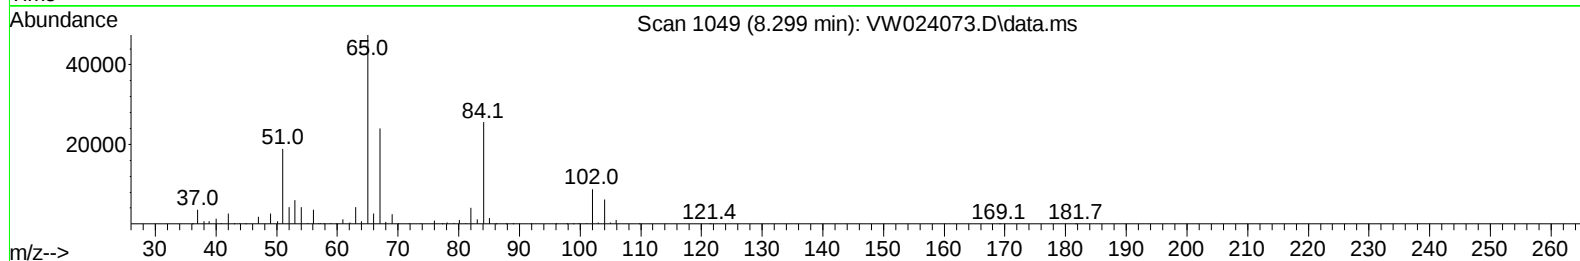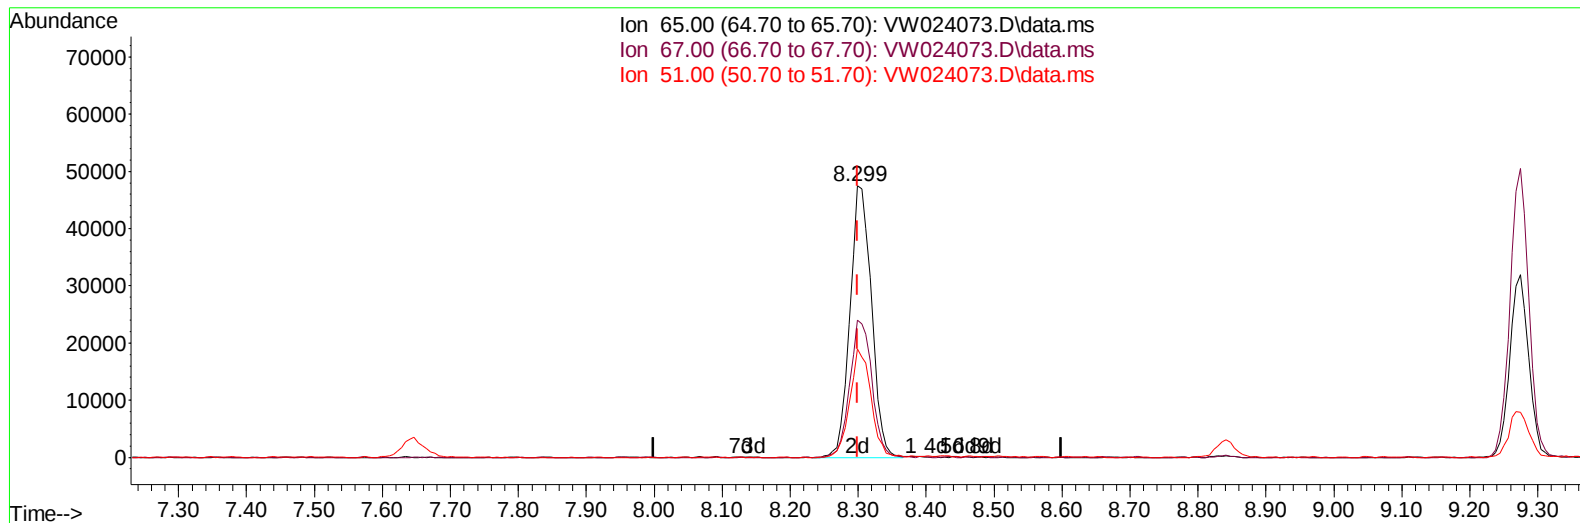

TIC: VW024073.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.000) 28.96 ug/L m

response 104463

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	50.40	0.07#
51.00	101.90	0.15#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024073.D
 Acq On : 25 Jul 2022 17:20
 Operator : SY/VA
 Sample : N3823-03
 Misc : 7.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B62

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:33:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/26/2022
 Supervised By :Mahesh Dadoda 07/26/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		228355	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		235895	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		113272	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.337	65		139802	28.561	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	114.240%	
7) Chloroethane-d5	2.873	69		97200	29.390	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	117.560%	
11) 1,1-Dichloroethene-d2	4.007	63		78111	18.123	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	72.480%	
21) 2-Butanone-d5	7.080	46		60708	69.786	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	139.580%#	
24) Chloroform-d	7.647	84		164276	26.167	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	104.680%	
26) 1,2-Dichloroethane-d4	8.299	65		104463m	28.963	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	115.840%	
32) Benzene-d6	8.275	84		297996	27.194	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	108.760%	
36) 1,2-Dichloropropane-d6	9.274	67		98208	28.414	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	113.640%	
41) Toluene-d8	10.323	98		279988	25.549	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	102.200%	
43) trans-1,3-Dichloroprop...	10.579	79		41066	26.797	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	107.200%	
47) 2-Hexanone-d5	10.927	63		51475	71.237	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	142.480%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		109237	27.391	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	109.560%	
66) 1,2-Dichlorobenzene-d4	13.853	152		108607	29.606	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	118.440%	
Target Compounds							
13) Acetone	4.129	43		3282m	5.317	ug/L	
16) Methylene chloride	4.915	84		14688	4.226	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
Data File : VW024073.D
Acq On : 25 Jul 2022 17:20
Operator : SY/VA
Sample : N3823-03
Misc : 7.36g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
H0B62

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/26/2022
Supervised By :Mahesh Dadoda 07/26/2022

Quant Time: Jul 26 01:33:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 01:30:33 2022
Response via : Initial Calibration

