




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024077.D
 Acq On : 25 Jul 2022 18:59
 Operator : SY/VA
 Sample : N3823-10
 Misc : 6.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B67

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:34:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/26/2022
 Supervised By :Mahesh Dadoda 07/26/2022

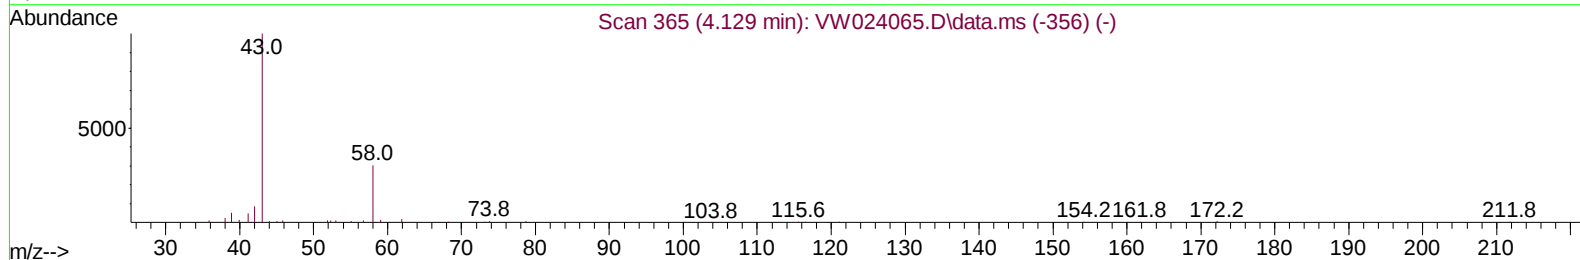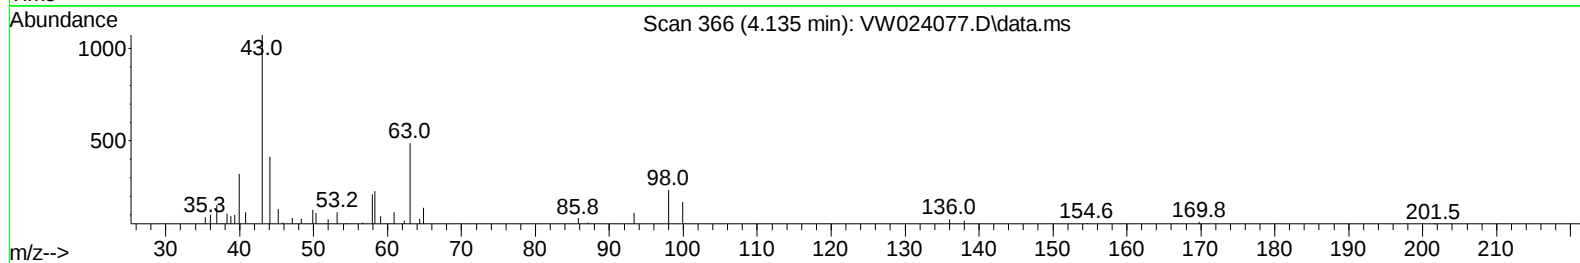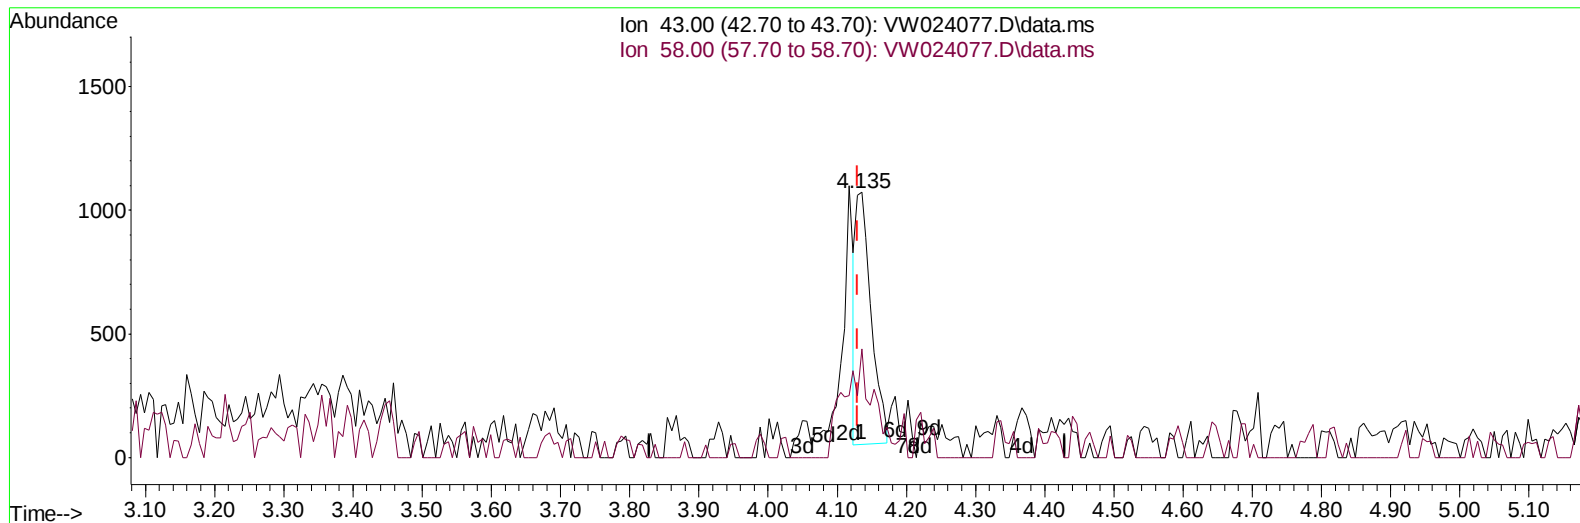

TIC: VW024077.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 2.49 ug/L

response 1556

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.00	20.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024077.D
 Acq On : 25 Jul 2022 18:59
 Operator : SY/VA
 Sample : N3823-10
 Misc : 6.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B67

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:34:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/26/2022
 Supervised By :Mahesh Dadoda 07/26/2022

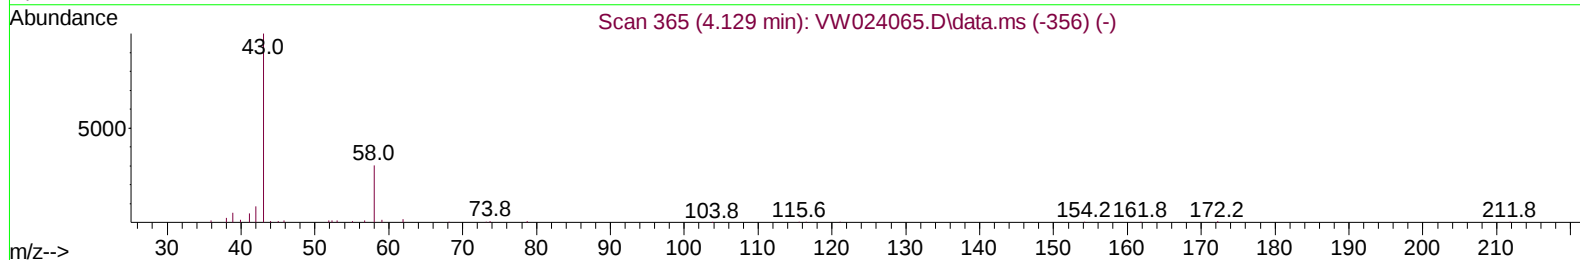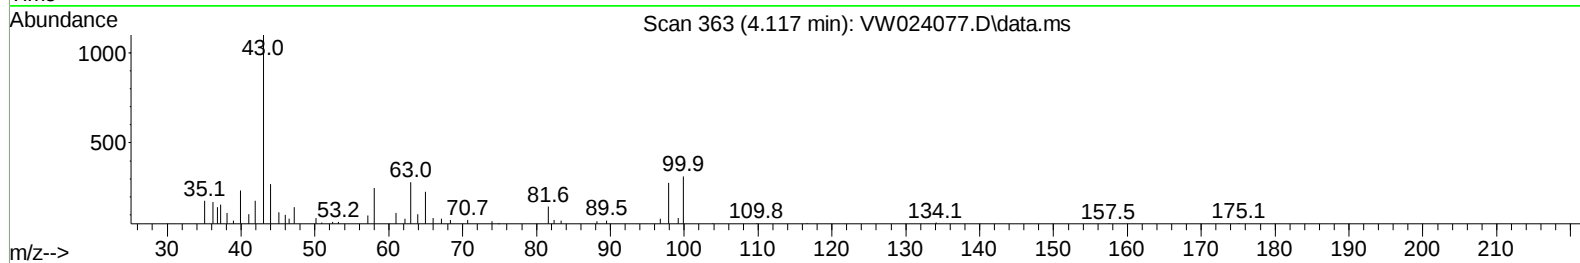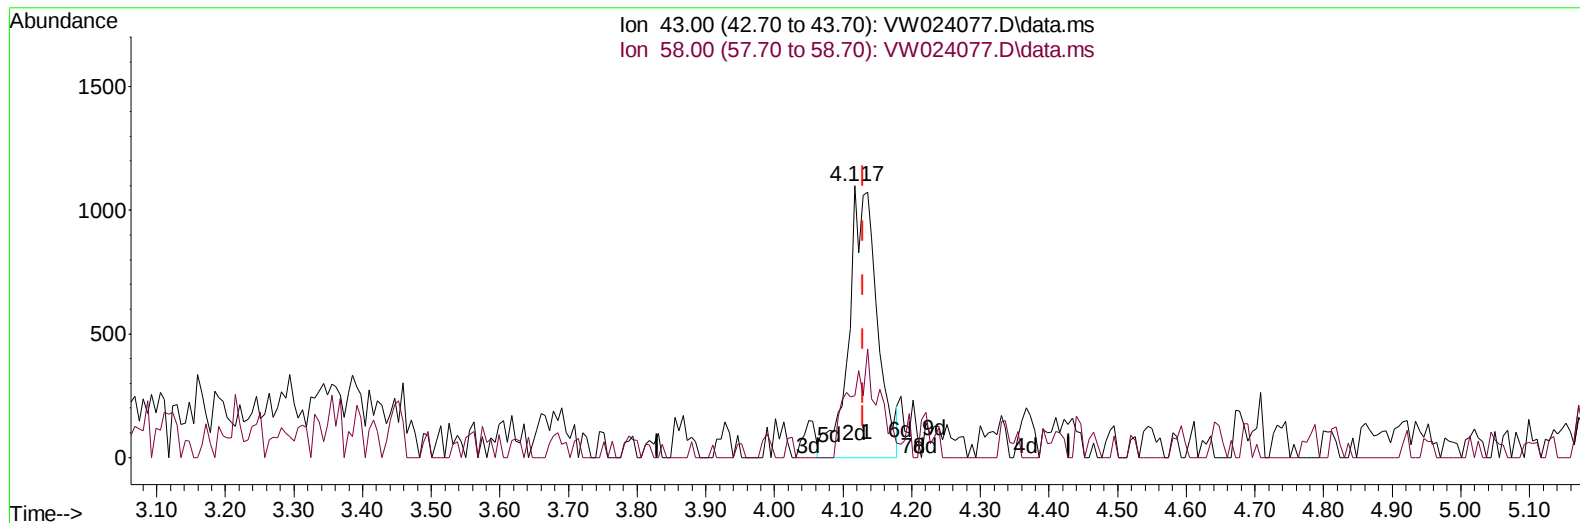

TIC: VW024077.D\data.ms

(13) Acetone (T)

4.117min (-0.012) 4.99 ug/L m

response 3118

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.00	10.39
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
Data File : VW024077.D
Acq On : 25 Jul 2022 18:59
Operator : SY/VA
Sample : N3823-10
Misc : 6.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
H0B67

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/26/2022
Supervised By :Mahesh Dadoda 07/26/2022

Quant Time: Jul 26 01:34:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 01:30:33 2022
Response via : Initial Calibration

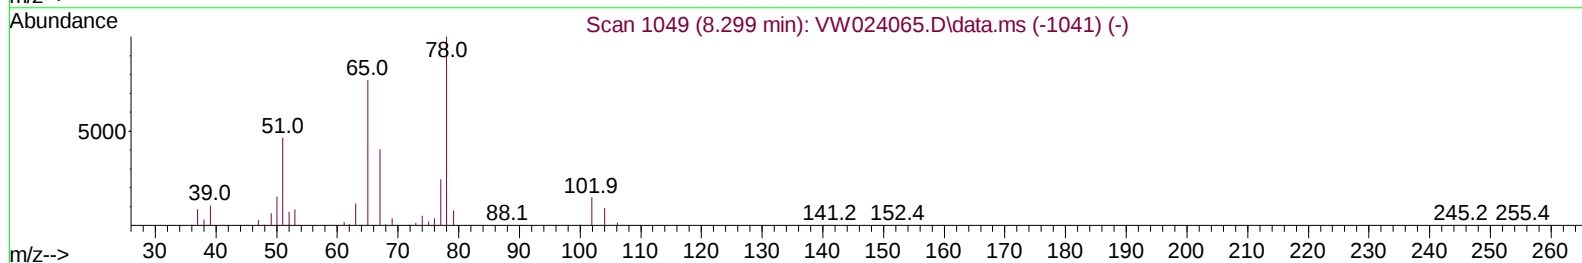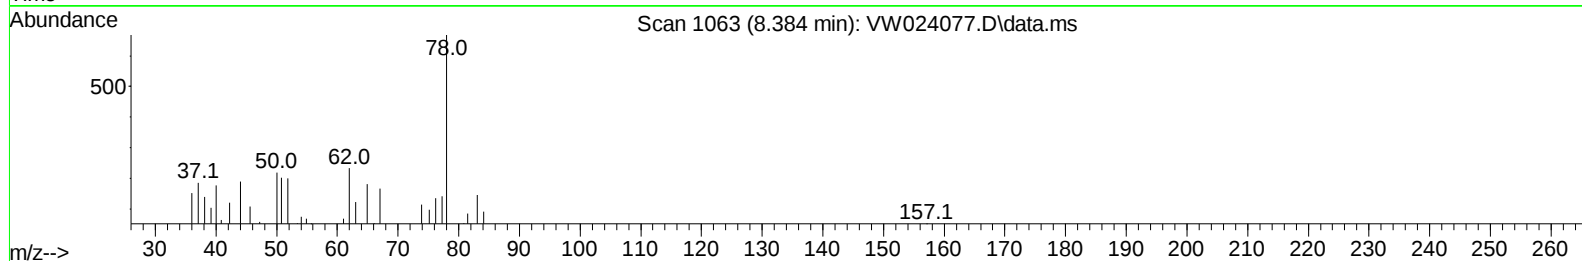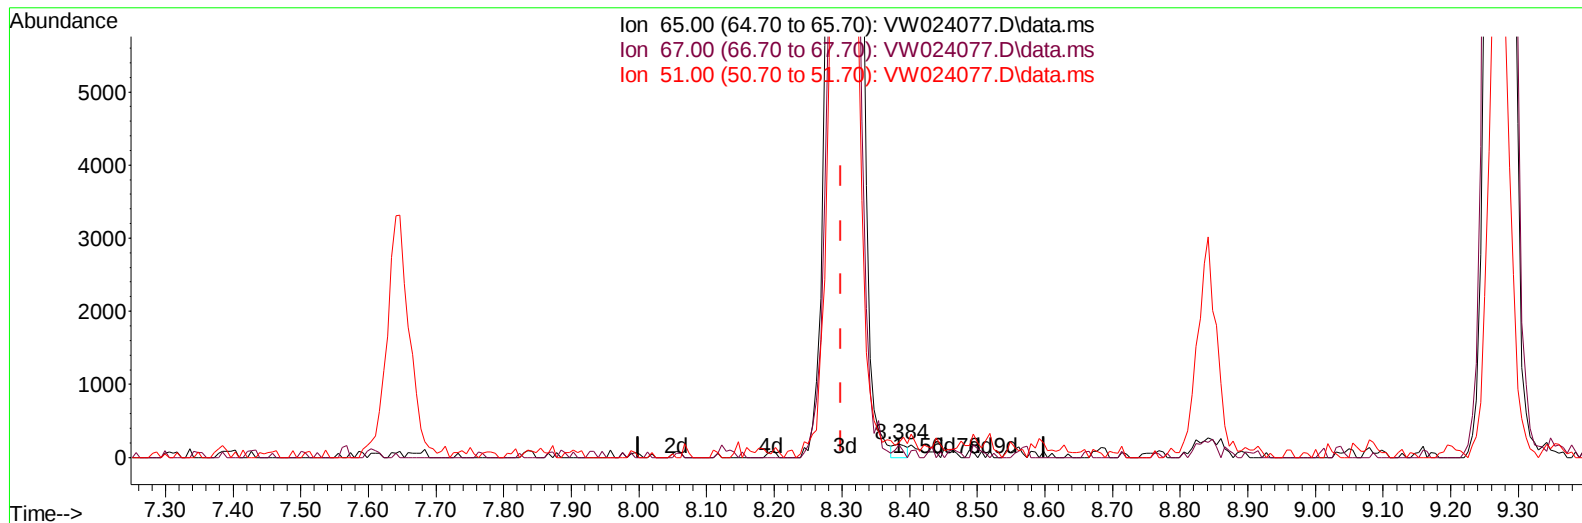

TIC: VW024077.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.384min (+ 0.085) 0.07 ug/L

response 239

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	50.40	53.14
51.00	101.90	74.48
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024077.D
 Acq On : 25 Jul 2022 18:59
 Operator : SY/VA
 Sample : N3823-10
 Misc : 6.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B67

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/26/2022
 Supervised By :Mahesh Dadoda 07/26/2022

Quant Time: Jul 26 01:34:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

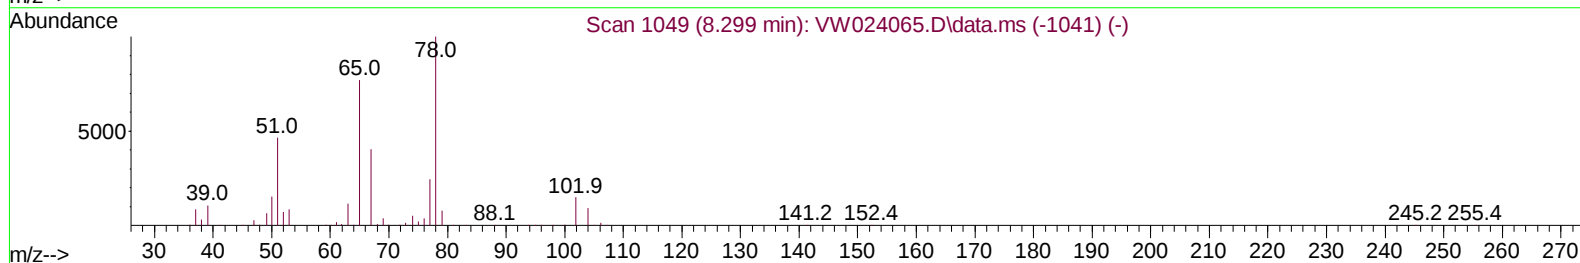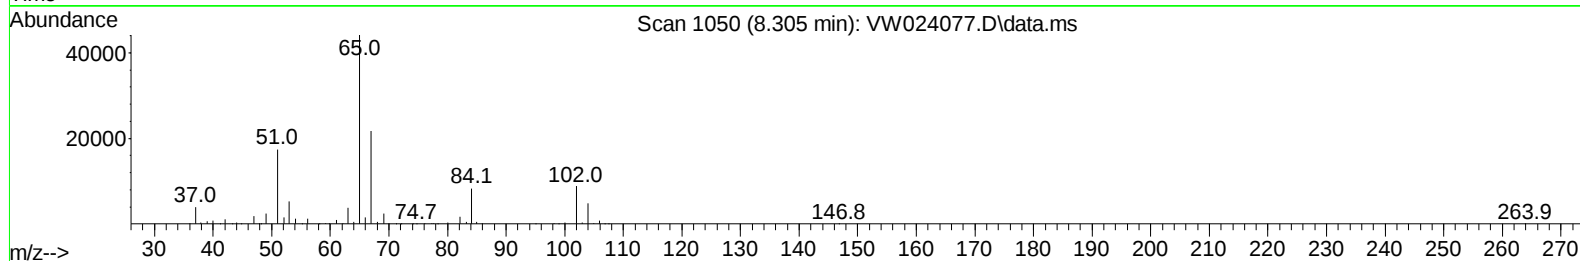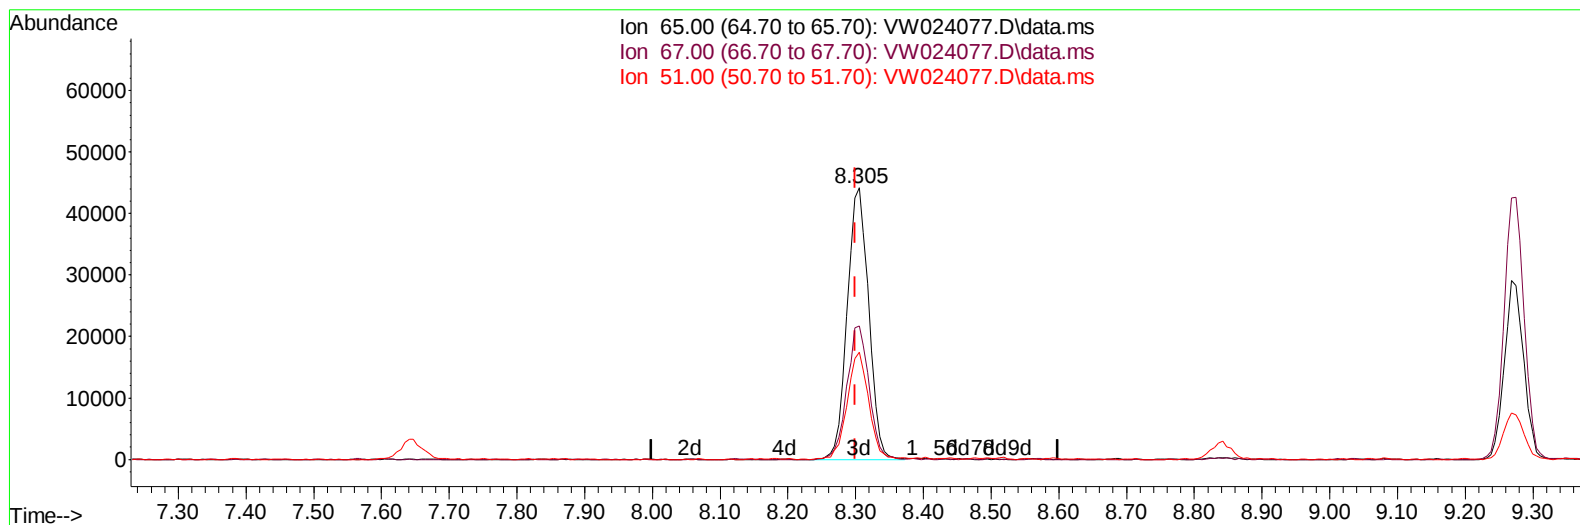

TIC: VW024077.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.006) 26.55 ug/L m

response 96911

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	50.40	0.13#
51.00	101.90	0.18#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024077.D
 Acq On : 25 Jul 2022 18:59
 Operator : SY/VA
 Sample : N3823-10
 Misc : 6.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B67

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/26/2022
 Supervised By :Mahesh Dadoda 07/26/2022

Quant Time: Jul 26 01:34:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	231065	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	235819	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	105081	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	127926	25.828	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.320%
7) Chloroethane-d5	2.873	69	83535	24.962	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.840%
11) 1,1-Dichloroethene-d2	4.007	63	66502	15.249	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.000%
21) 2-Butanone-d5	7.074	46	58882	66.893	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	133.780%
24) Chloroform-d	7.647	84	150565	23.702	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	8.305	65	96911m	26.554	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.200%
32) Benzene-d6	8.275	84	267769	24.444	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.760%
36) 1,2-Dichloropropane-d6	9.275	67	87556	25.340	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.360%
41) Toluene-d8	10.323	98	247356	22.578	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.320%
43) trans-1,3-Dichloroprop...	10.579	79	35539	23.198	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.800%
47) 2-Hexanone-d5	10.921	63	47231	65.385	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	130.780%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	100002	25.083	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	95300	28.004	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	112.000%
Target Compounds					Qvalue	
13) Acetone	4.117	43	3118m	4.992	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
Data File : VW024077.D
Acq On : 25 Jul 2022 18:59
Operator : SY/VA
Sample : N3823-10
Misc : 6.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
H0B67

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/26/2022
Supervised By :Mahesh Dadoda 07/26/2022

Quant Time: Jul 26 01:34:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 01:30:33 2022
Response via : Initial Calibration

