

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024067.D
 Acq On : 25 Jul 2022 14:51
 Operator : SY/VA
 Sample : VIBLK516
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK516

Quant Time: Jul 26 01:31:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	197888	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	203324	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	87610	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	148830	35.087	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	140.360%
7) Chloroethane-d5	2.873	69	90384	31.537	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	126.160%
11) 1,1-Dichloroethene-d2	4.001	63	77498	20.749	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.000%
21) 2-Butanone-d5	7.080	46	41876	55.549	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.100%
24) Chloroform-d	7.641	84	143866	26.444	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	105.760%
26) 1,2-Dichloroethane-d4	8.299	65	89279	28.564	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	114.240%
32) Benzene-d6	8.268	84	273043	28.909	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	115.640%
36) 1,2-Dichloropropane-d6	9.268	67	84149	28.246	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	113.000%
41) Toluene-d8	10.323	98	264003	27.949	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	111.800%
43) trans-1,3-Dichloroprop...	10.573	79	35312	26.734	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	106.920%
47) 2-Hexanone-d5	10.920	63	34604	55.561	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.120%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	85009	24.730	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.920%
66) 1,2-Dichlorobenzene-d4	13.853	152	87234	30.745	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	123.000%#
Target Compounds						Qvalue
16) Methylene chloride	4.909	84	26976	8.956	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
Data File : VW024067.D
Acq On : 25 Jul 2022 14:51
Operator : SY/VA
Sample : VIBLK516
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK516


Quant Time: Jul 26 01:31:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 01:30:33 2022
Response via : Initial Calibration

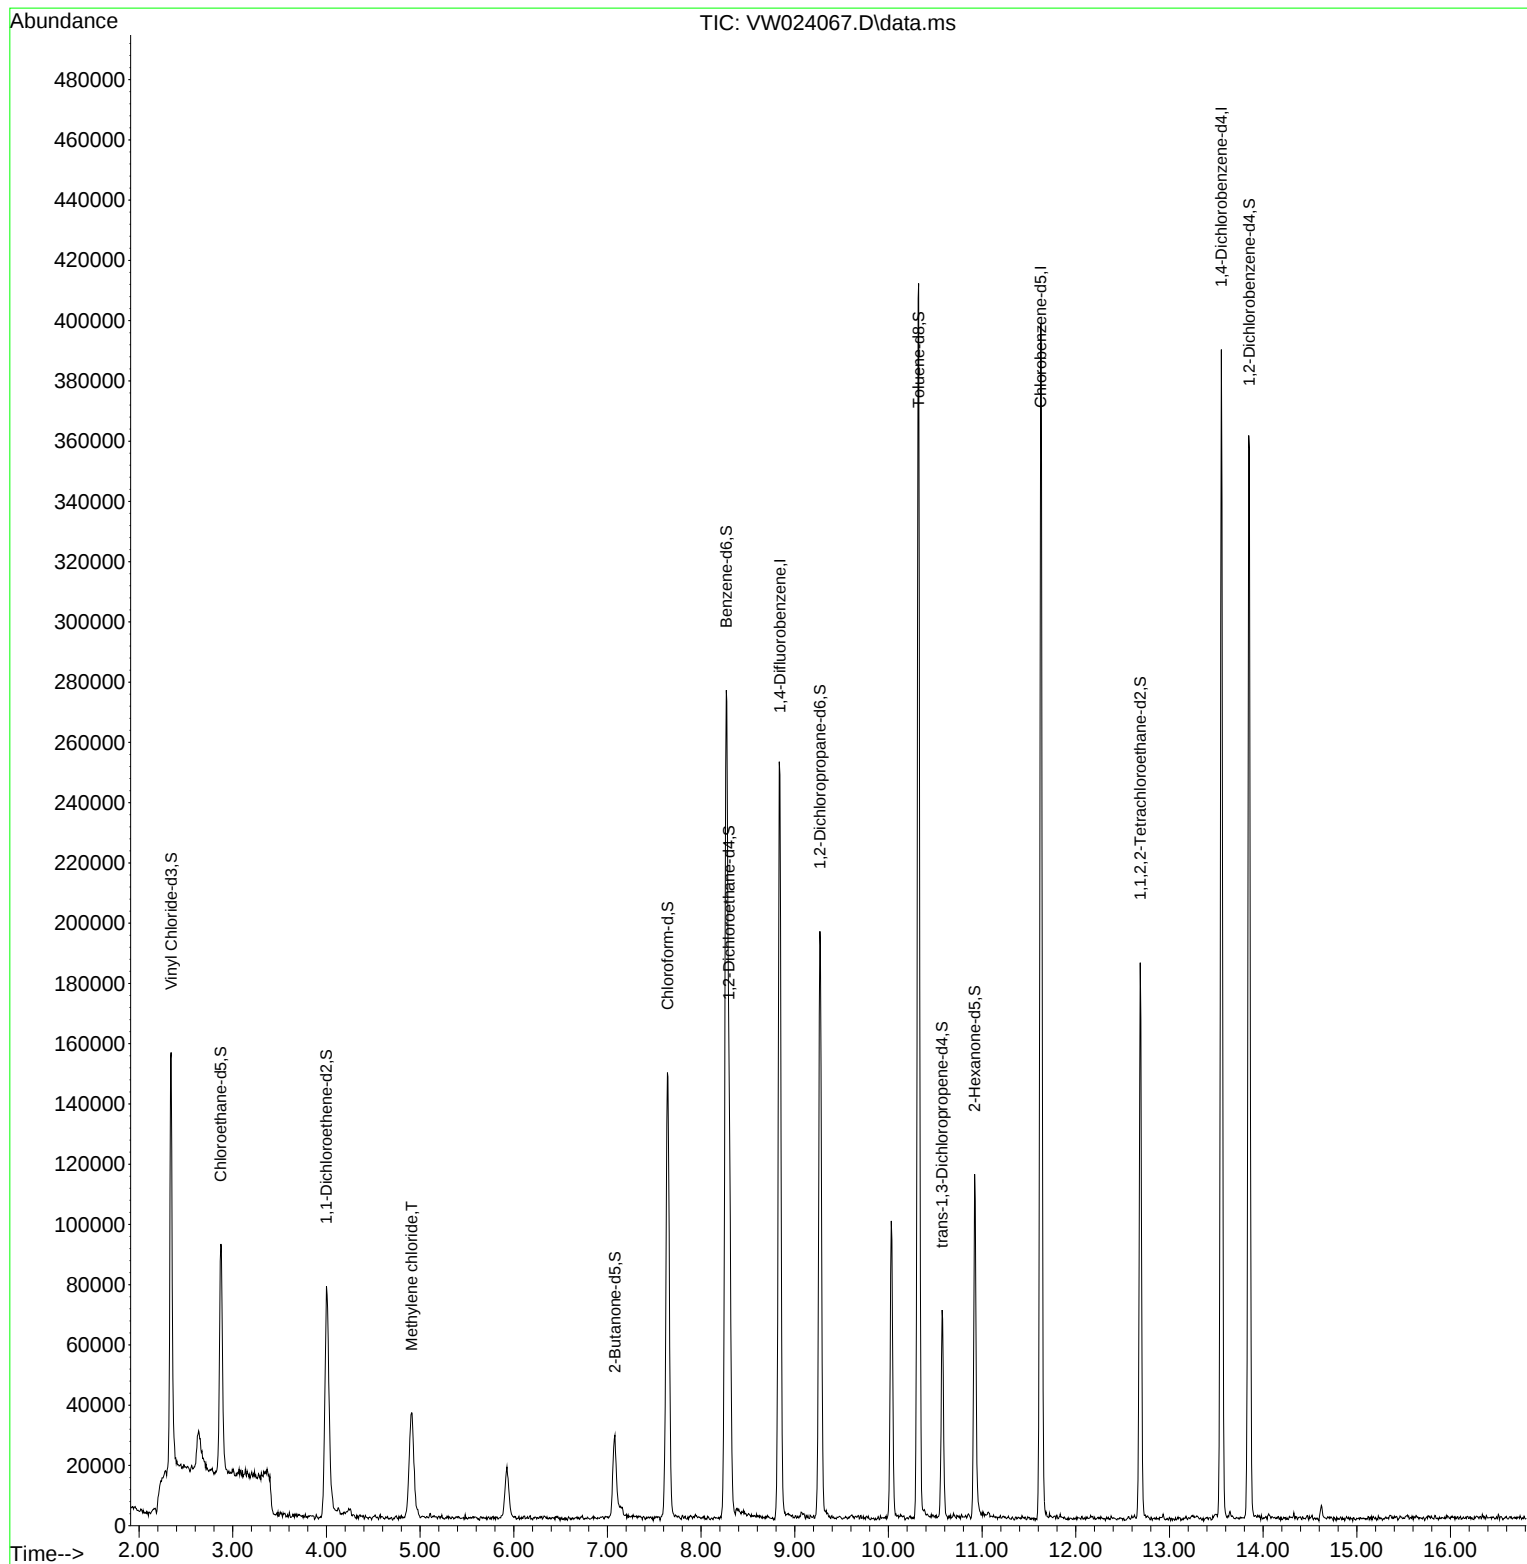

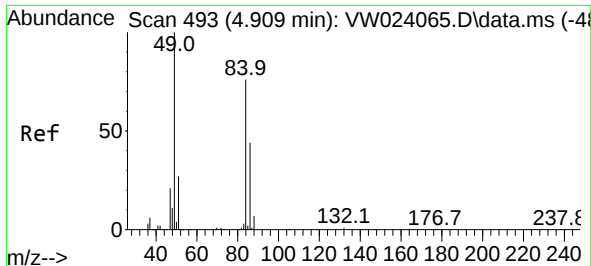

#16
Methylene chloride
Concen: 8.956 ug/L
RT: 4.909 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW024067.D
Acq: 25 Jul 2022 14:51

Instrument :
MSVOA_W
ClientSampleId :
VIBLK516

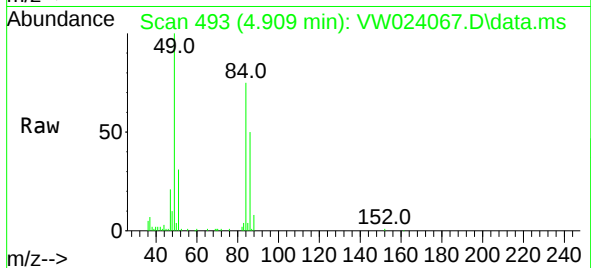

Tgt Ion: 84 Resp: 26976

Ion	Ratio	Lower	Upper
84	100		
86	66.7	44.7	83.1
49	134.0	83.7	155.4

