

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024077.D
 Acq On : 25 Jul 2022 18:59
 Operator : SY/VA
 Sample : N3823-10
 Misc : 6.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B67

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/26/2022
 Supervised By :Mahesh Dadoda 07/26/2022

Quant Time: Jul 26 01:34:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	231065	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	235819	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	105081	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	127926	25.828	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 103.320%			
7) Chloroethane-d5	2.873	69	83535	24.962	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 99.840%			
11) 1,1-Dichloroethene-d2	4.007	63	66502	15.249	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 61.000%			
21) 2-Butanone-d5	7.074	46	58882	66.893	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 133.780%			
24) Chloroform-d	7.647	84	150565	23.702	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 94.800%			
26) 1,2-Dichloroethane-d4	8.305	65	96911m	26.554	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 106.200%			
32) Benzene-d6	8.275	84	267769	24.444	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 97.760%			
36) 1,2-Dichloropropane-d6	9.275	67	87556	25.340	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 101.360%			
41) Toluene-d8	10.323	98	247356	22.578	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 90.320%			
43) trans-1,3-Dichloroprop...	10.579	79	35539	23.198	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 92.800%			
47) 2-Hexanone-d5	10.921	63	47231	65.385	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 130.780%			
56) 1,1,2,2-Tetrachloroeth...	12.689	84	100002	25.083	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 100.320%			
66) 1,2-Dichlorobenzene-d4	13.853	152	95300	28.004	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 112.000%			
Target Compounds					Qvalue	
13) Acetone	4.117	43	3118m	4.992	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
Data File : VW024077.D
Acq On : 25 Jul 2022 18:59
Operator : SY/VA
Sample : N3823-10
Misc : 6.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
H0B67

Quant Time: Jul 26 01:34:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 01:30:33 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/26/2022
Supervised By :Mahesh Dadoda 07/26/2022

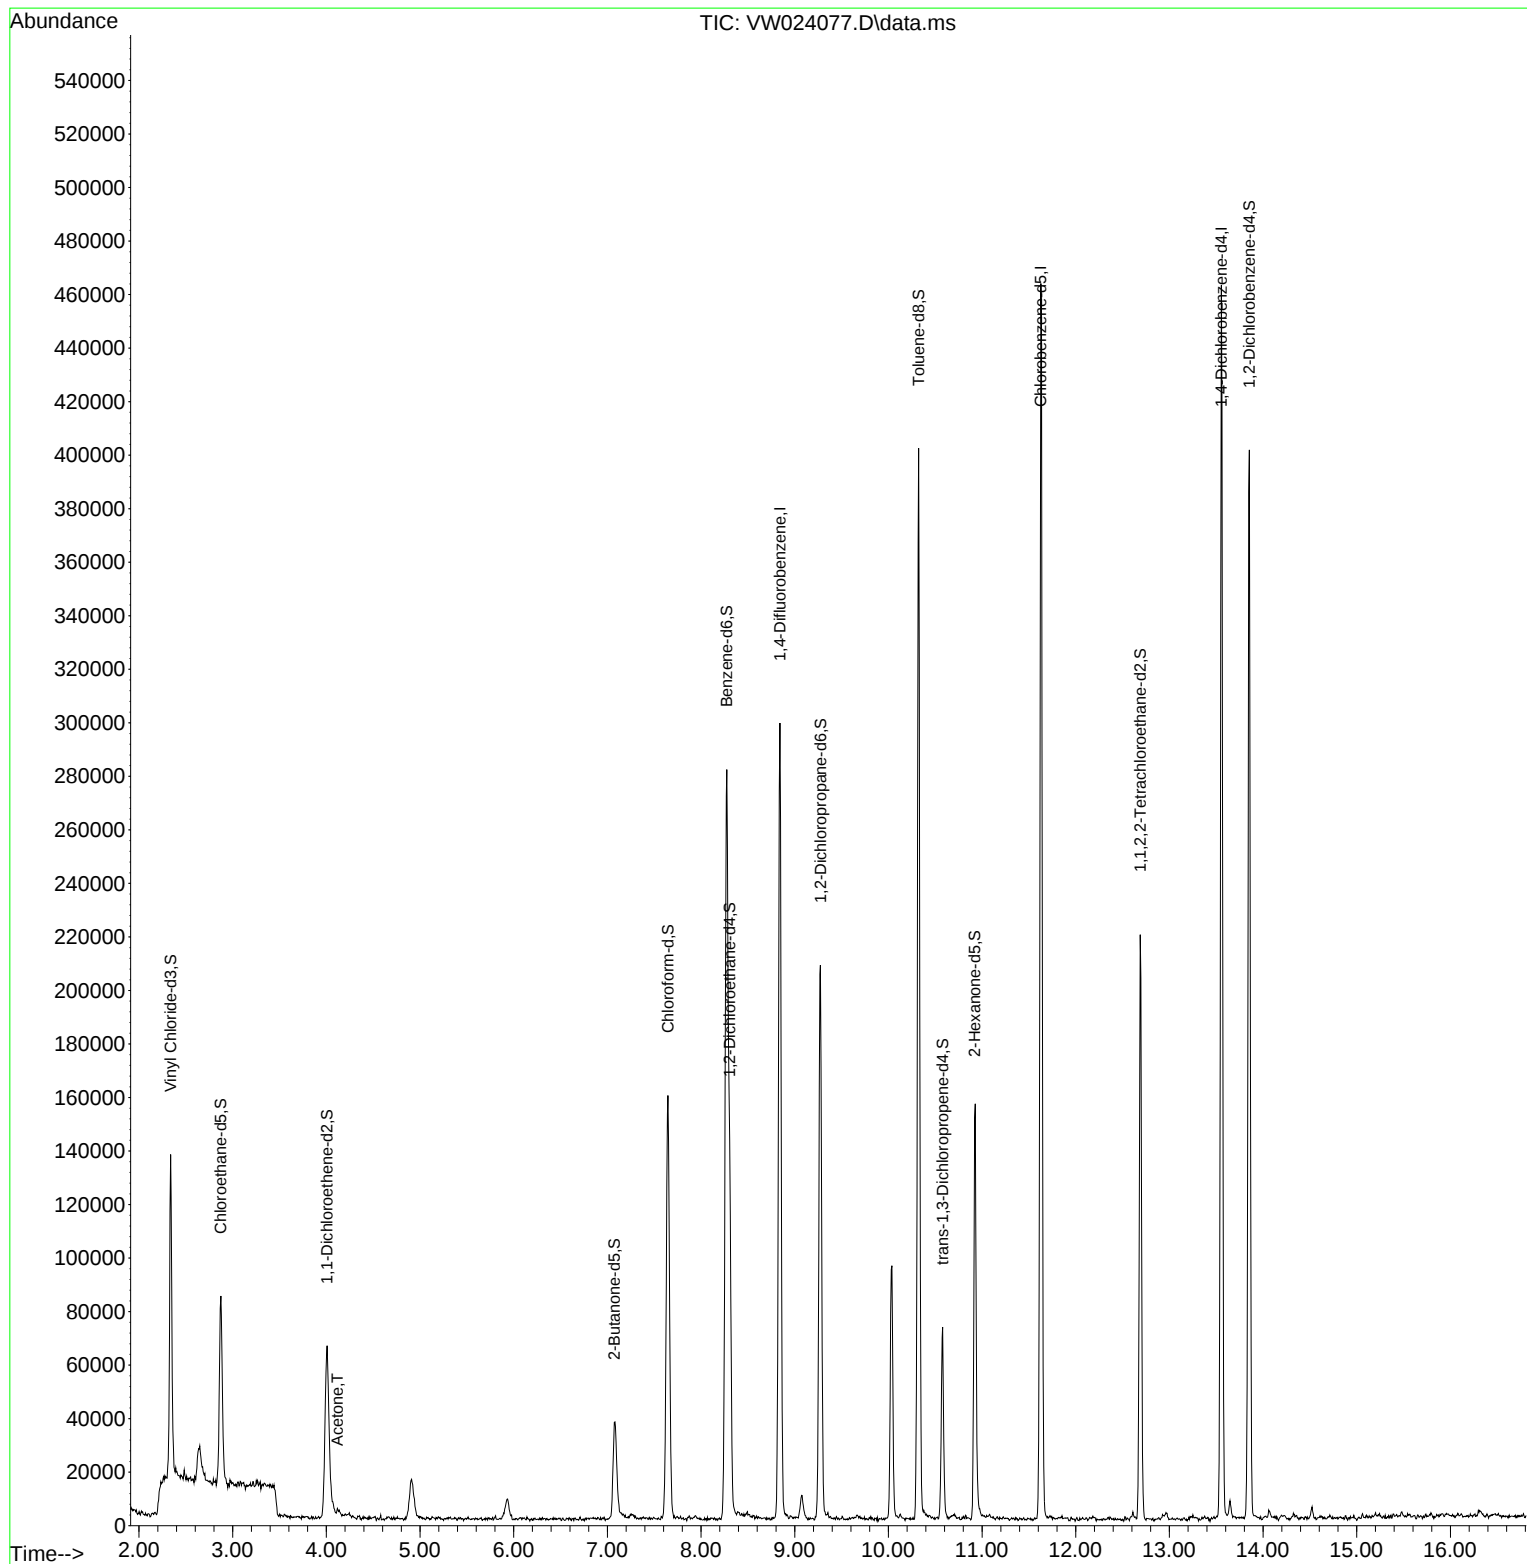

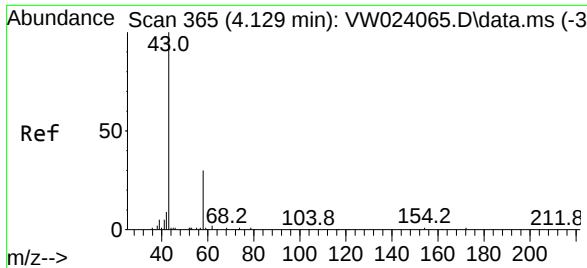

#13
 Acetone
 Concen: 4.992 ug/L m
 RT: 4.117 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: VW024077.D
 Acq: 25 Jul 2022 18:59

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B67

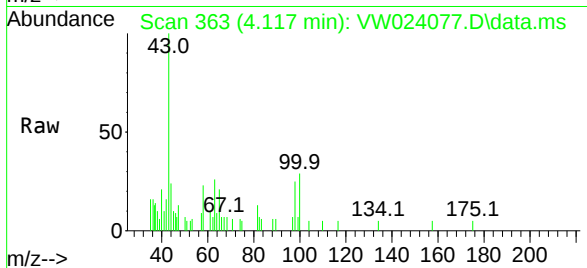

Tgt Ion: 43 Resp: 3118
 Ion Ratio Lower Upper
 43 100
 58 10.4 0.0 60.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/26/2022
 Supervised By :Mahesh Dadoda 07/26/2022

