

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
 Data File : VW024078.D
 Acq On : 25 Jul 2022 19:24
 Operator : SY/VA
 Sample : N3709-05
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Jul 26 01:34:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	193171	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	203842	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	90146	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	135889	32.818	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	131.280%
7) Chloroethane-d5	2.873	69	83667	29.906	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	119.640%
11) 1,1-Dichloroethene-d2	4.007	63	67208	18.434	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.720%
21) 2-Butanone-d5	7.086	46	38521	52.346	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.700%
24) Chloroform-d	7.647	84	128298	24.159	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.640%
26) 1,2-Dichloroethane-d4	8.305	65	79932	26.198	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.800%
32) Benzene-d6	8.275	84	236509	24.977	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.920%
36) 1,2-Dichloropropane-d6	9.274	67	74451	24.927	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.720%
41) Toluene-d8	10.323	98	227453	24.019	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.080%
43) trans-1,3-Dichloroprop...	10.579	79	31092	23.479	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.920%
47) 2-Hexanone-d5	10.920	63	32906	52.700	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.400%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	77578	22.511	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.040%
66) 1,2-Dichlorobenzene-d4	13.847	152	79142	27.108	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.440%
Target Compounds						Qvalue
16) Methylene chloride	4.909	84	20479	6.965	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072522\
Data File : VW024078.D
Acq On : 25 Jul 2022 19:24
Operator : SY/VA
Sample : N3709-05
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001


Quant Time: Jul 26 01:34:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 01:30:33 2022
Response via : Initial Calibration

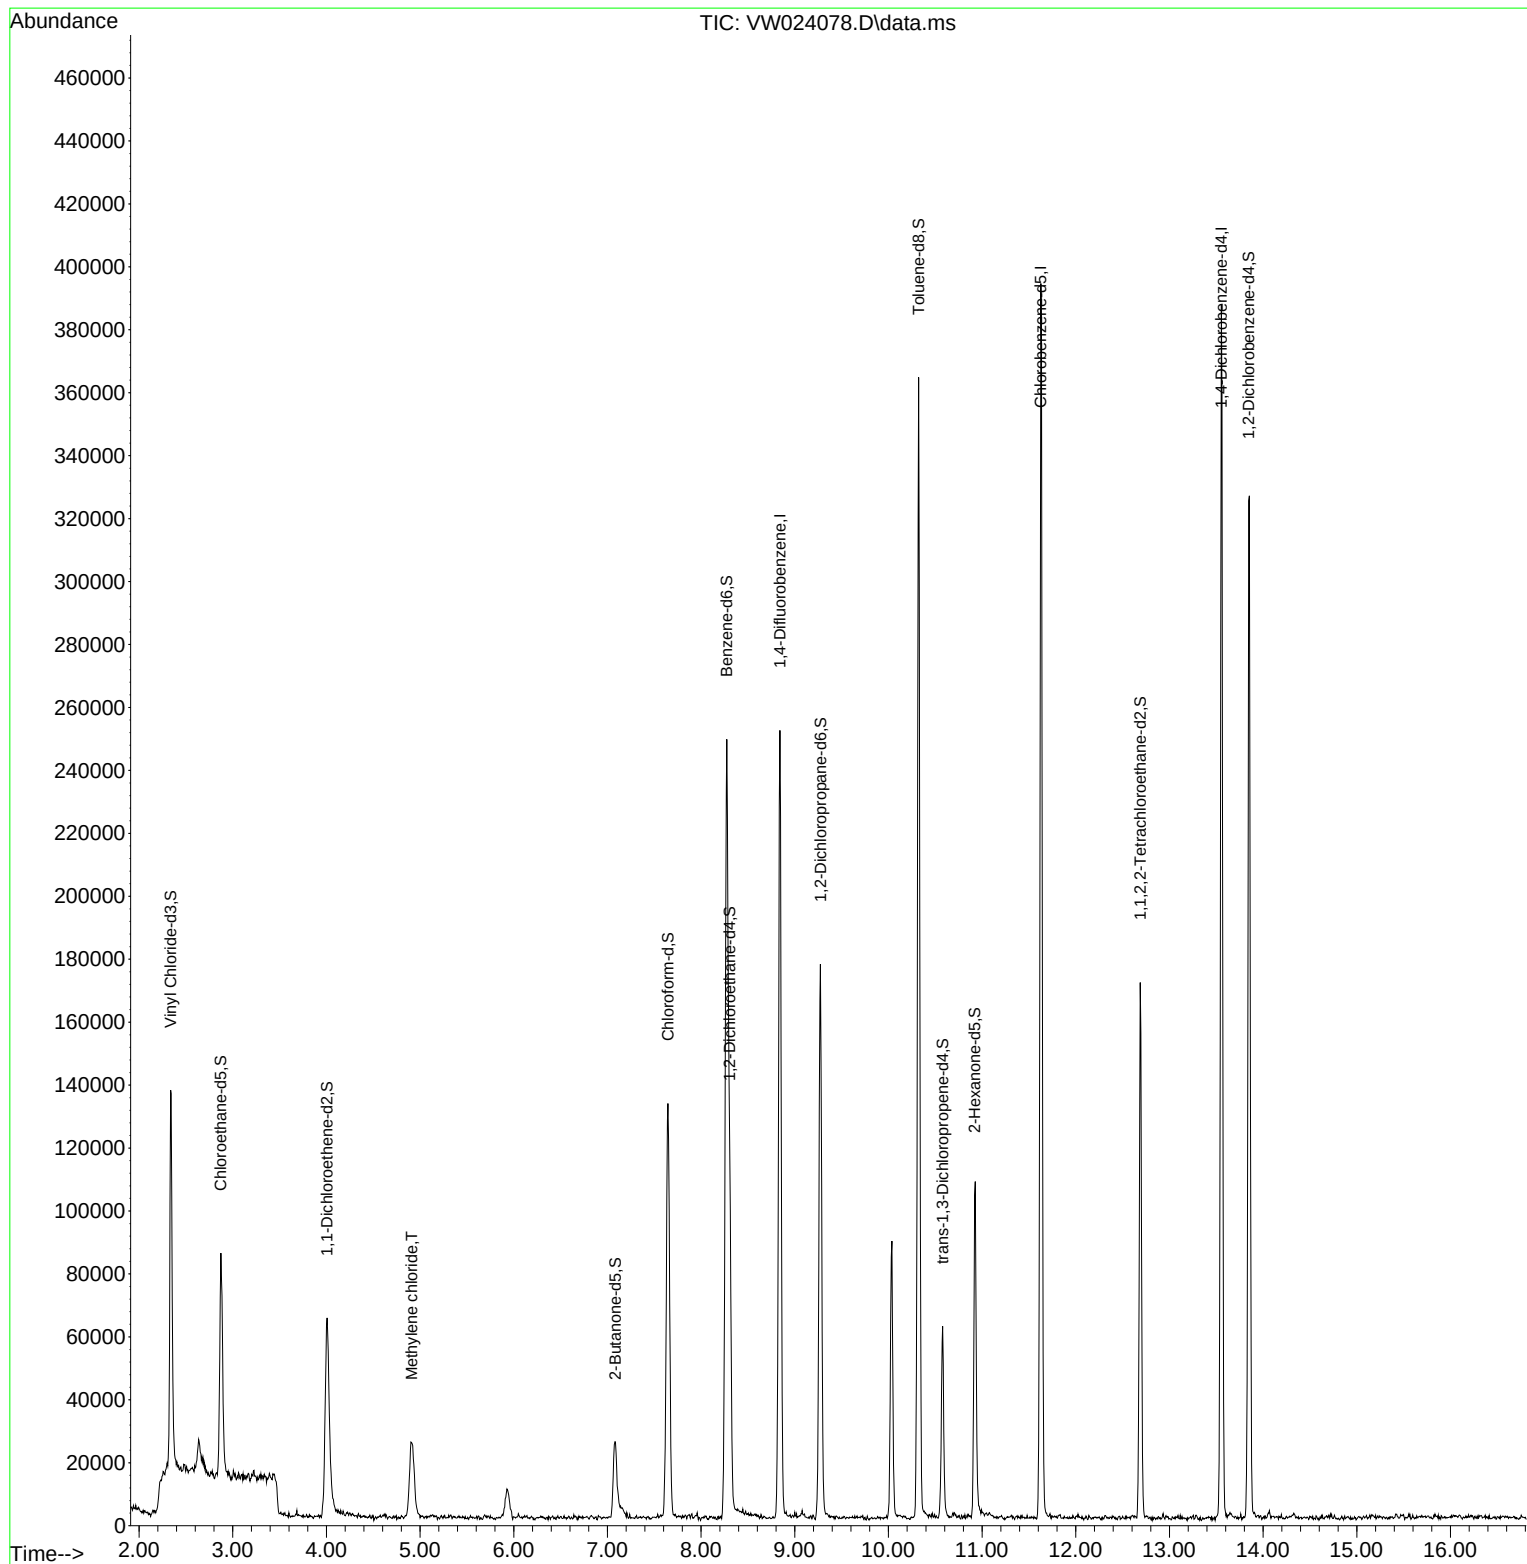

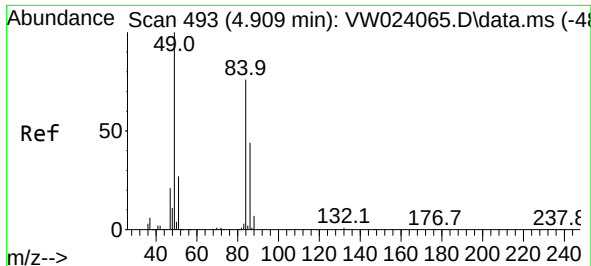

#16
Methylene chloride
Concen: 6.965 ug/L
RT: 4.909 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW024078.D
Acq: 25 Jul 2022 19:24

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

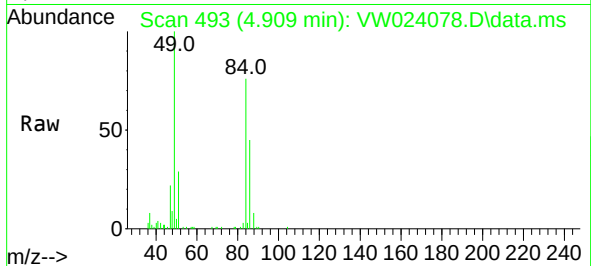

Tgt Ion: 84 Resp: 20479

Ion	Ratio	Lower	Upper
84	100		
86	59.7	44.7	83.1
49	131.9	83.7	155.4

