

Data File : VW011497.D
Acq On : 25 Jul 2019 14:25
Operator : SY/VA
Sample : K3979-07
Misc : 5.47G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB927

Quant Time: Jul 26 01:09:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 26 01:06:02 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	291246	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	261163	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	120075	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	87672	22.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.20%
7) Chloroethane-d5	2.89	69	63441	22.40	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.60%
10) 1,1-Dichloroethene-d2	4.01	63	148435	16.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.40%
20) 2-Butanone-d5	7.07	46	78365	47.33	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.66%
24) Chloroform-d	7.65	84	169861	22.77	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.08%
26) 1,2-Dichloroethane-d4	8.31	65	109400	24.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.68%
29) Benzene-d6	8.27	84	355944	22.79	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.16%
33) 1,2-Dichloropropane-d6	9.27	67	119065	23.53	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.12%
37) Toluene-d8	10.32	98	312726	22.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.36%
38) trans-1,3-Dichloropropene-	10.58	79	47443	21.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.80%
39) 2-Hexanone-d5	10.93	63	52807	48.13	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.26%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	96708	23.92	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.68%
61) 1,2-Dichlorobenzene-d4	13.85	152	104467	23.17	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.68%


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	13.56	75	15650	5.172 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011497.D
Acq On : 25 Jul 2019 14:25
Operator : SY/VA
Sample : K3979-07
Misc : 5.47G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB927

Quant Time: Jul 26 01:09:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 26 01:06:02 2019
Response via : Initial Calibration

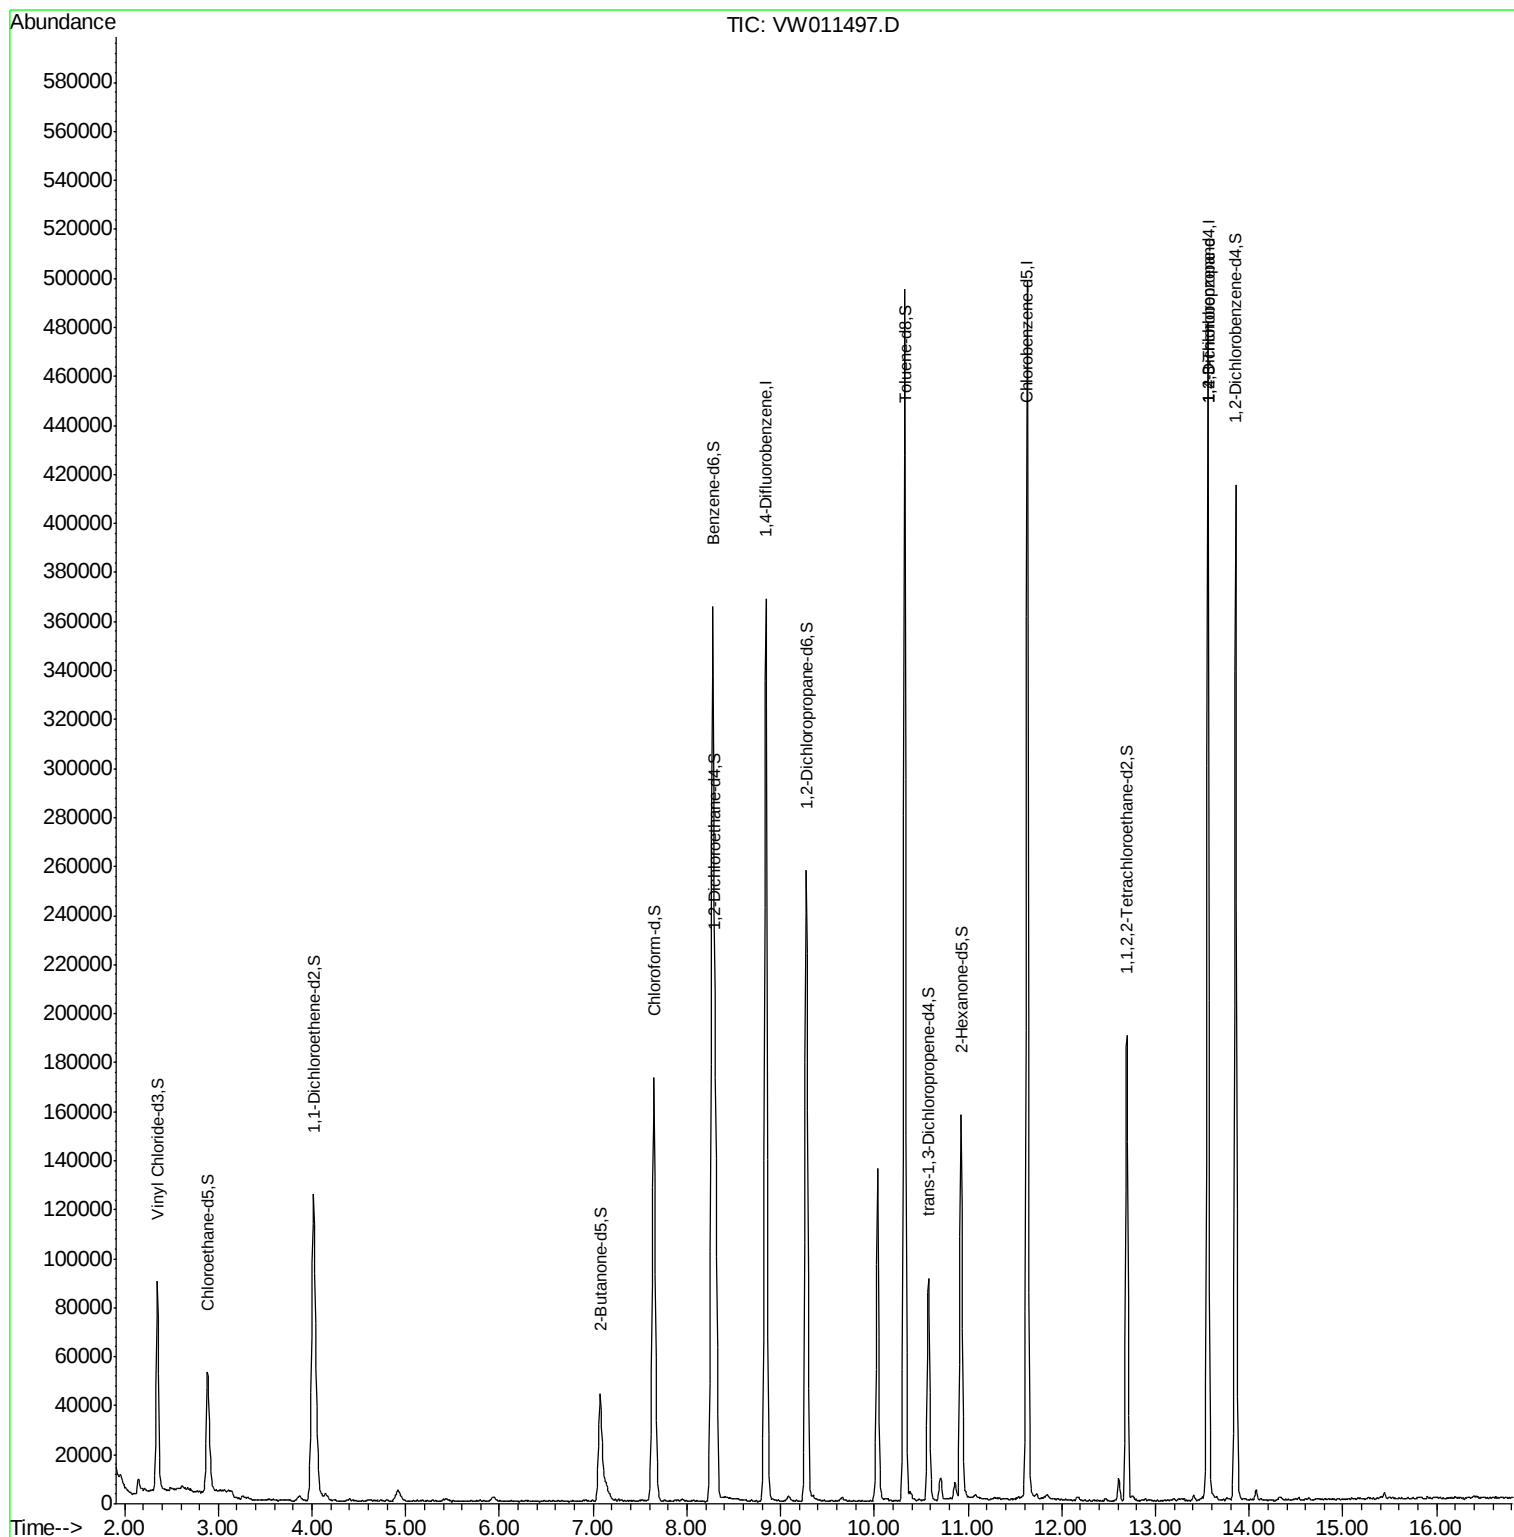

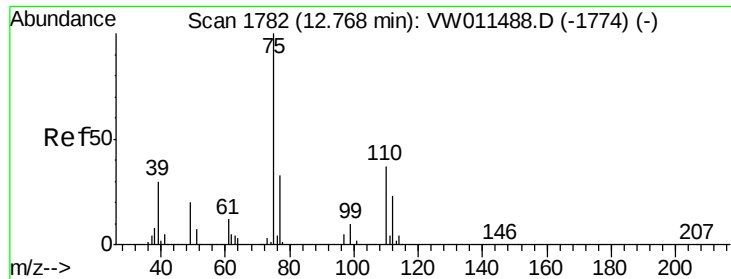

#59

1,2,3-Trichloropropane

Concen: 5.172 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW011497.D

Acq: 25 Jul 2019 14:25

Instrument :

MSVOA_W

ClientSampleId :

DB927

Tgt Ion: 75 Resp: 15650

Ion Ratio Lower Upper

75 100

77 38.0 25.8 38.8

