

Data File : VW011505.D
Acq On : 25 Jul 2019 17:59
Operator : SY/VA
Sample : K3979-15
Misc : 5.42G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB935

Quant Time: Jul 26 01:10:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 26 01:06:02 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	330383	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	297239	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	136866	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	97042	22.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.00%
7) Chloroethane-d5	2.89	69	70072	21.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.24%
10) 1,1-Dichloroethene-d2	4.01	63	166248	16.64	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.56%
20) 2-Butanone-d5	7.07	46	86575	46.09	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.18%
24) Chloroform-d	7.65	84	190268	22.49	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.96%
26) 1,2-Dichloroethane-d4	8.43	65	121	0.02	ug/L	0.13
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.08%#
29) Benzene-d6	8.27	84	397305	22.35	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.40%
33) 1,2-Dichloropropane-d6	9.27	67	130502	22.66	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.64%
37) Toluene-d8	10.32	98	346228	21.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.92%
38) trans-1,3-Dichloropropene-	10.58	79	52561	21.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.48%
39) 2-Hexanone-d5	10.93	63	57744	46.24	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.48%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	106472	23.13	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.52%
61) 1,2-Dichlorobenzene-d4	13.85	152	118129	22.99	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.96%


Target Compounds					Qvalue
47) Tetrachloroethene	10.86	164	4595	1.221 ug/L	83
50) Dibromochloromethane	10.86	129	4129	1.075 ug/L #	11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011505.D
Acq On : 25 Jul 2019 17:59
Operator : SY/VA
Sample : K3979-15
Misc : 5.42G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB935

Quant Time: Jul 26 01:10:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 26 01:06:02 2019
Response via : Initial Calibration

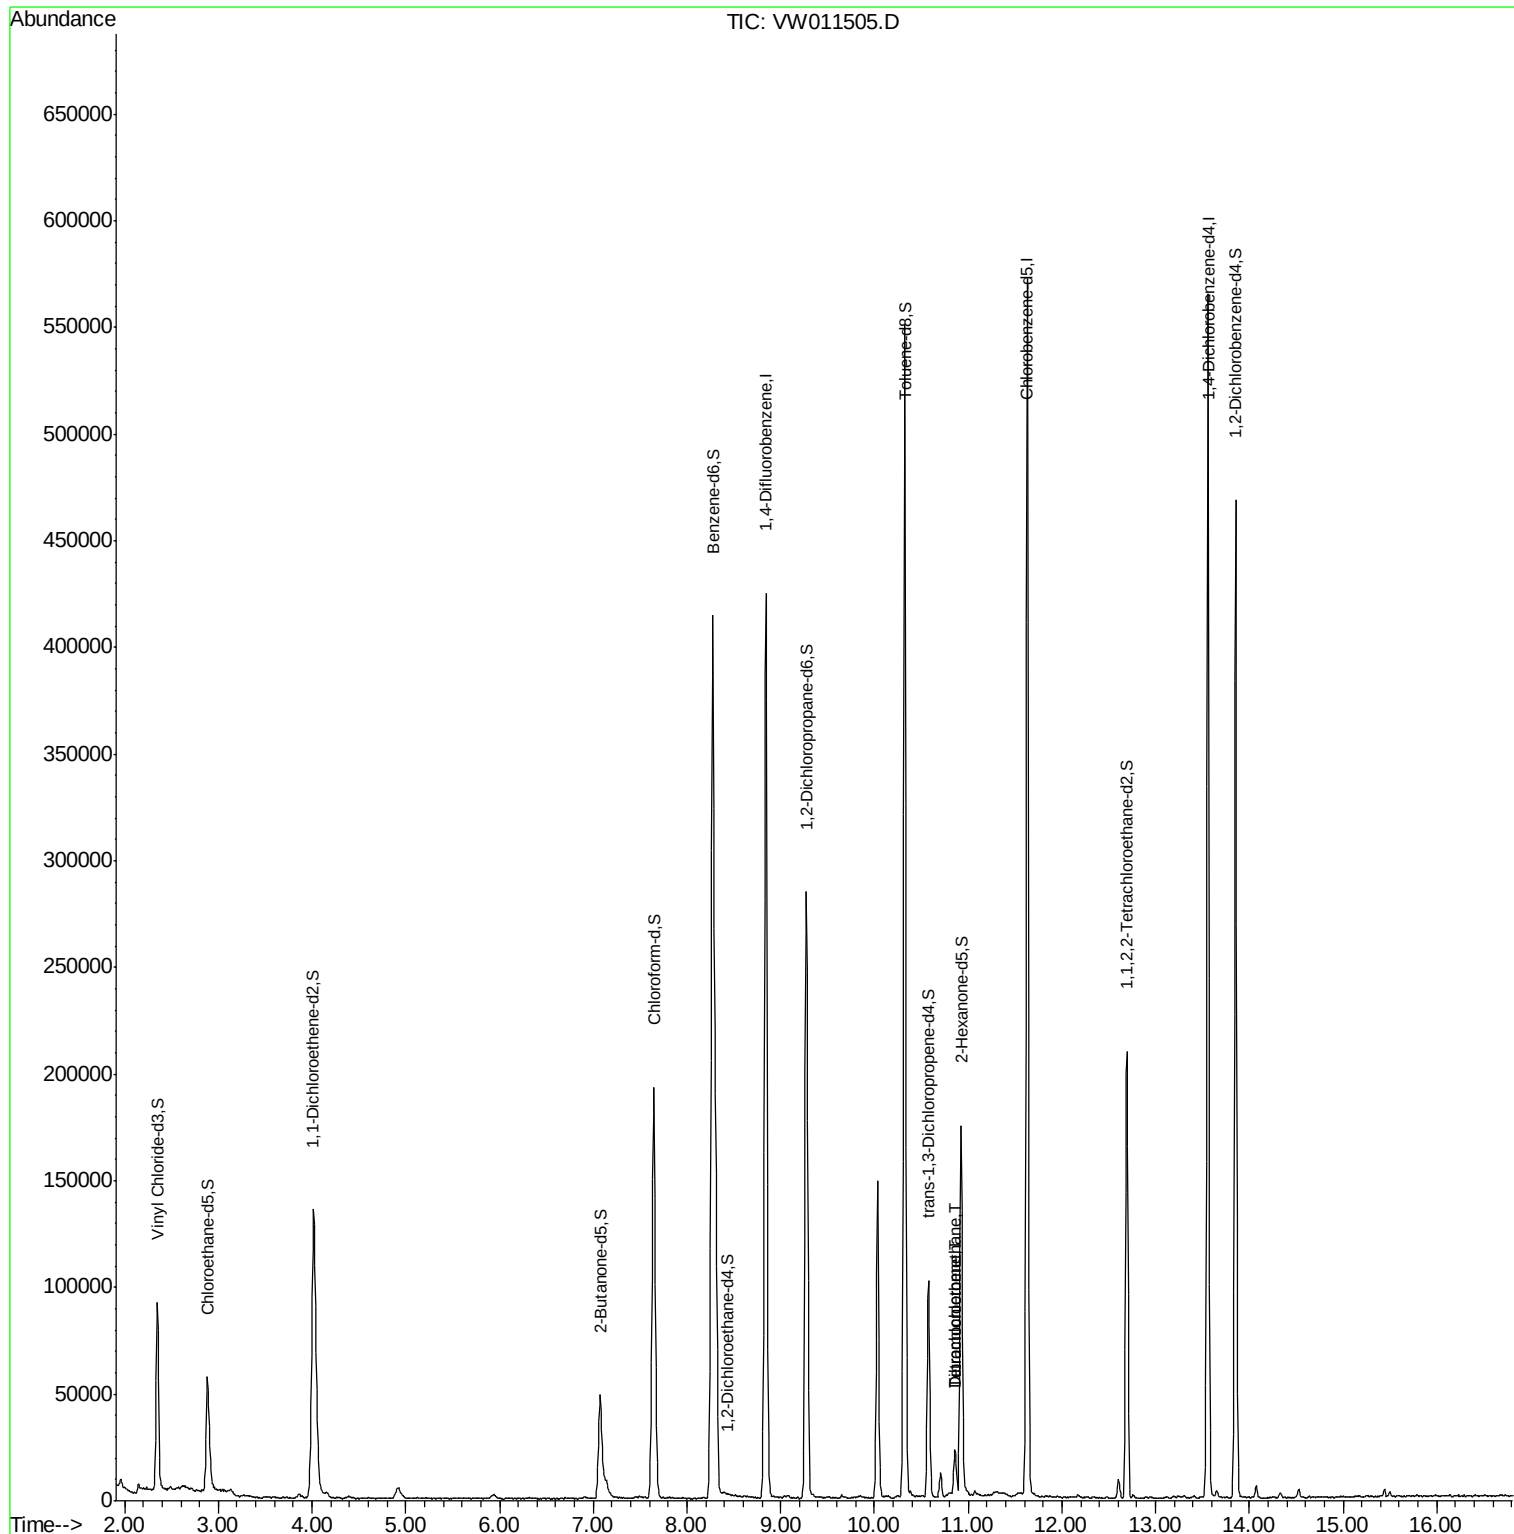

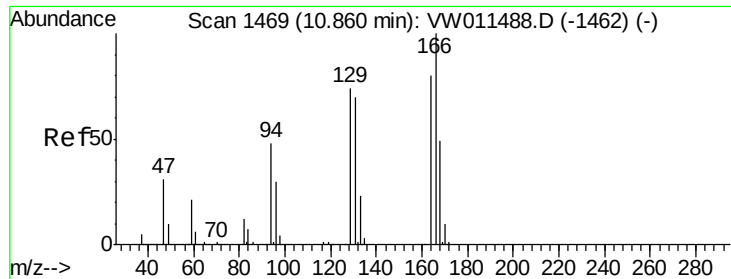

#47

Tetrachloroethene

Concen: 1.221 ug/L

RT: 10.86 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VW011505.D

Acq: 25 Jul 2019 17:59


Instrument :

MSVOA_W

ClientSampleId :

DB935

Tgt Ion:	164	Resp:	4595
Ion	Ratio	Lower	Upper
164	100		
129	78.6	69.0	128.1
131	83.3	64.5	119.7
166	104.5	89.2	165.6



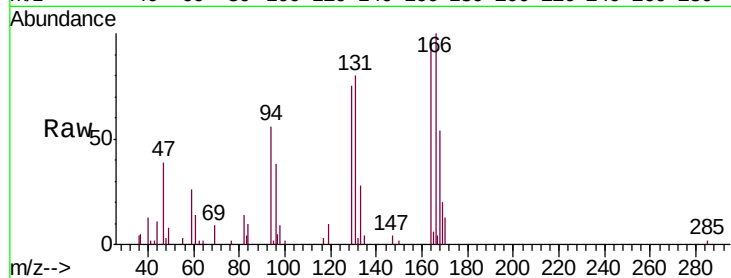


Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

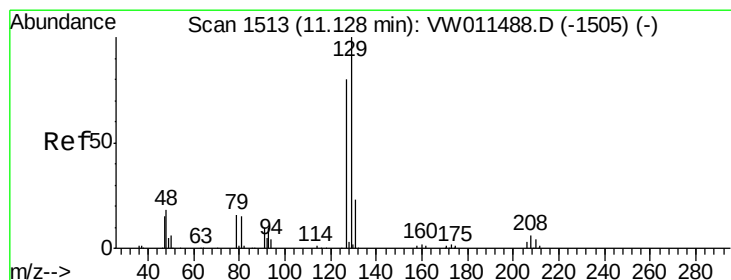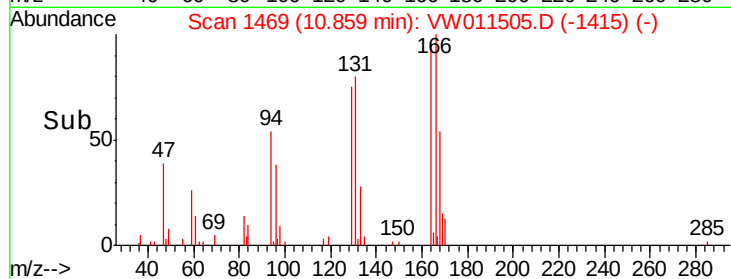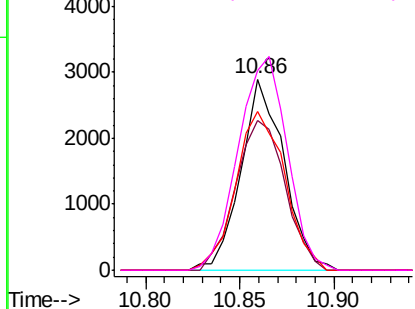

#50

Dibromochloromethane

Concen: 1.075 ug/L


RT: 10.86 min Scan# 1469

Delta R.T. -0.27 min

Lab File: VW011505.D

Acq: 25 Jul 2019 17:59

Tgt Ion:	129	Resp:	4129
Ion	Ratio	Lower	Upper
129	100		
127	0.0	53.9	100.1#

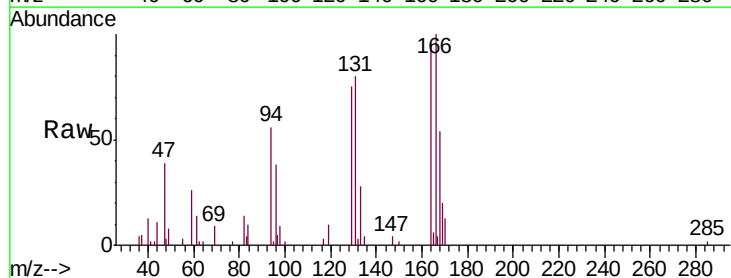

Abundance Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

