

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW072619\
 Data File : VW011492.D
 Acq On : 25 Jul 2019 12:12
 Operator : SY/VA
 Sample : K3979-02
 Misc : 4.54G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DB922

Quant Time: Jul 26 01:27:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 26 01:06:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	453383	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	398736	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	186815	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	137001	22.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.56%
7) Chloroethane-d5	2.89	69	100913	22.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.56%
10) 1,1-Dichloroethene-d2	4.01	63	234726	17.12	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.48%
20) 2-Butanone-d5	7.07	46	118853	46.11	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.22%
24) Chloroform-d	7.65	84	275687	23.75	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	8.31	65	169247	24.52	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.08%
29) Benzene-d6	8.27	84	586667	24.60	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.40%
33) 1,2-Dichloropropane-d6	9.27	67	191563	24.79	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.16%
37) Toluene-d8	10.32	98	515765	24.13	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.52%
38) trans-1,3-Dichloropropene-	10.58	79	79481	23.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.24%
39) 2-Hexanone-d5	10.93	63	81006	48.36	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.72%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	148648	24.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.32%
61) 1,2-Dichlorobenzene-d4	13.85	152	171653	24.47	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.88%


Target Compounds					Ovalue
13) Acetone	4.12	43	4929	1.808 ug/L	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW072619\
Data File : VW011492.D
Acq On : 25 Jul 2019 12:12
Operator : SY/VA
Sample : K3979-02
Misc : 4.54G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB922

Quant Time: Jul 26 01:27:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 26 01:06:02 2019
Response via : Initial Calibration

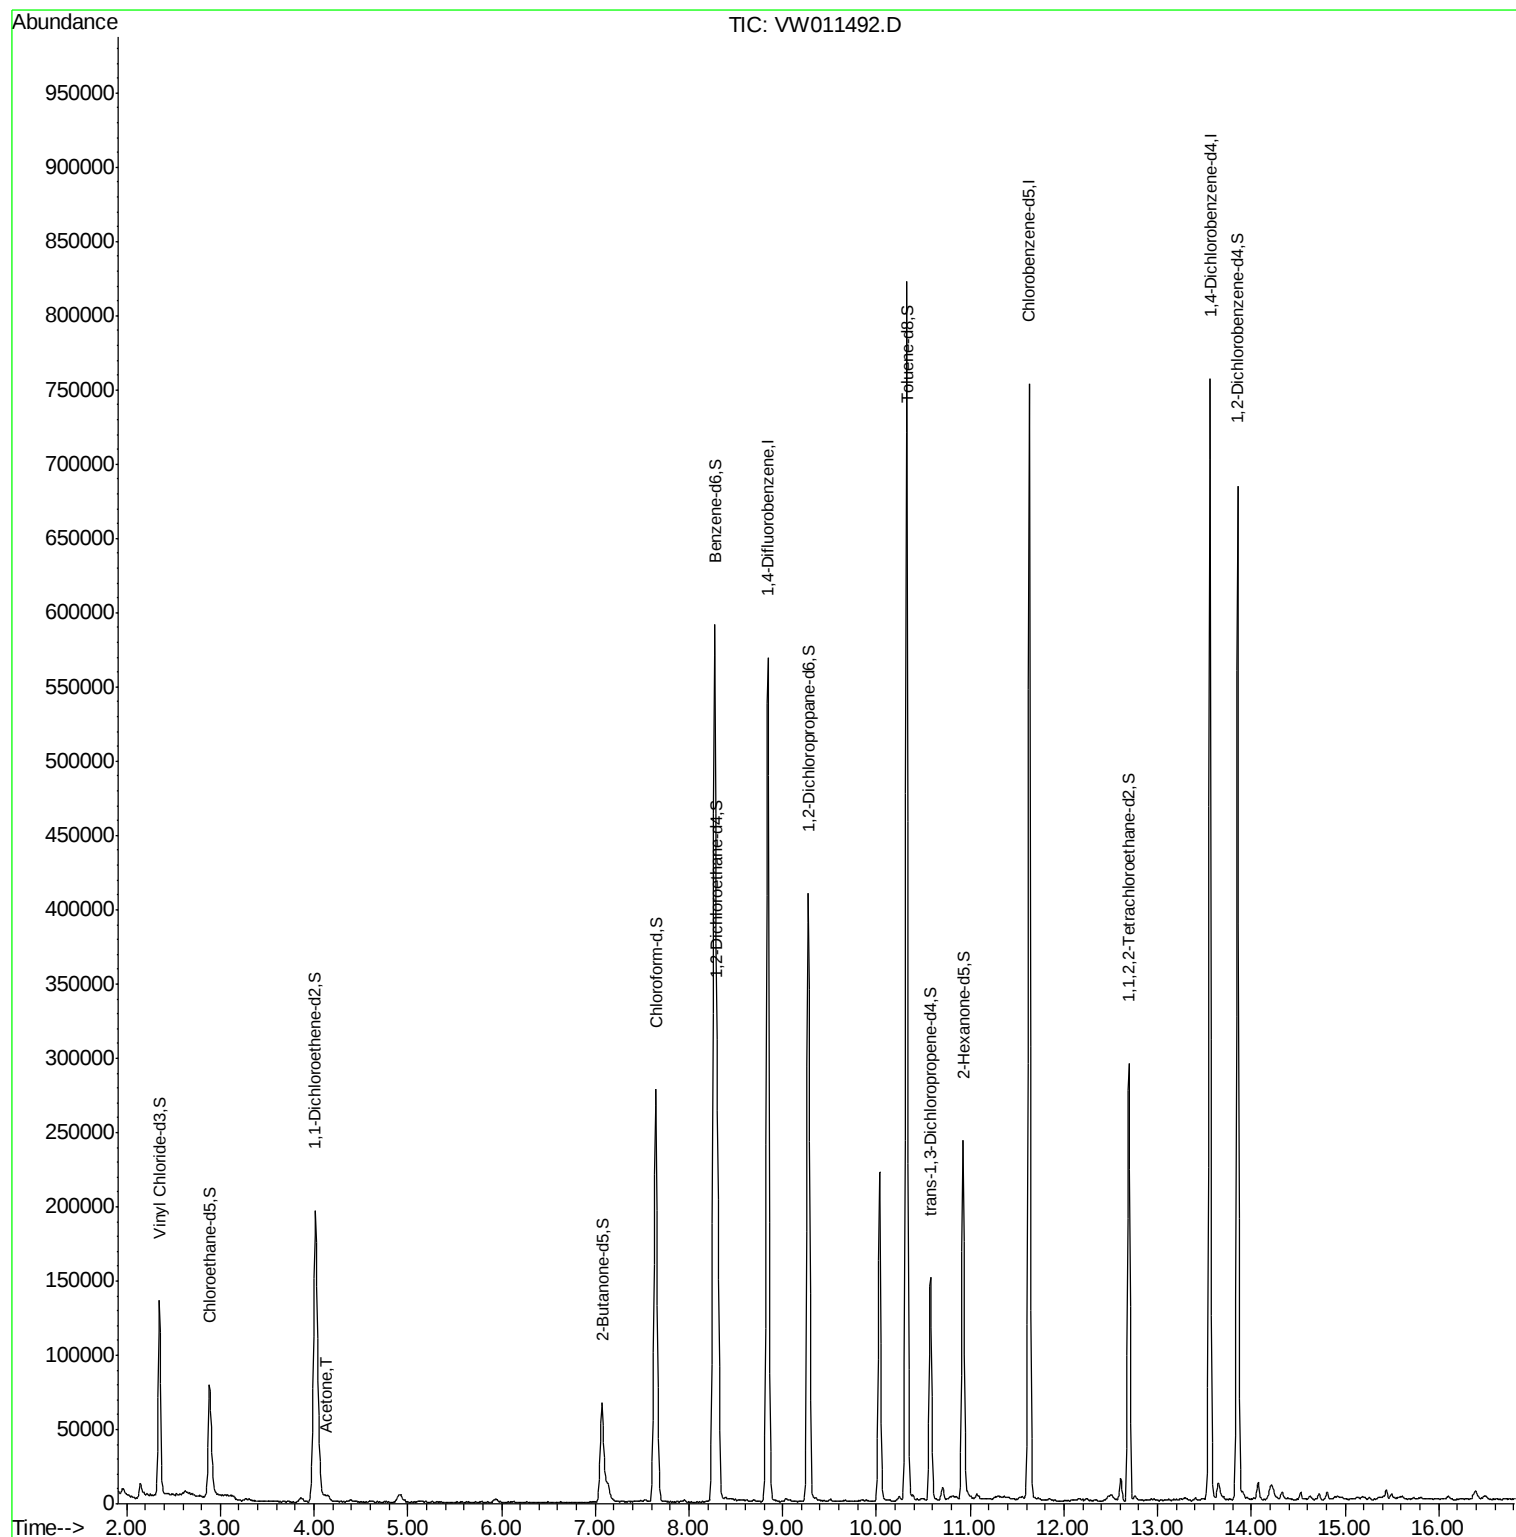

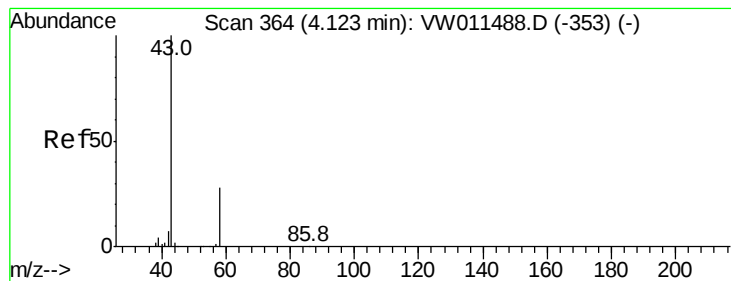

#13

Acetone

Concen: 1.808 ug/L

RT: 4.12 min Scan# 364

Delta R.T. -0.00 min

Lab File: VW011492.D

Acq: 25 Jul 2019 12:12

Instrument :

MSVOA_W

ClientSampleId :

DB922

Tot Ion: 43 Resp: 4929

Ion Ratio Lower Upper

43 100

58 2.5 0.0 57.2

