




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072623\
 Data File : VW026659.D
 Acq On : 26 Jul 2023 14:26
 Operator : SY/MD
 Sample : 03754-12
 Misc : 3.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BH2T5

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 07/27/2023
 Supervised By : Mahesh Dadoda 07/27/2023

Quant Time: Jul 27 03:02:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMLM071123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 27 03:01:27 2023
 Response via : Initial Calibration

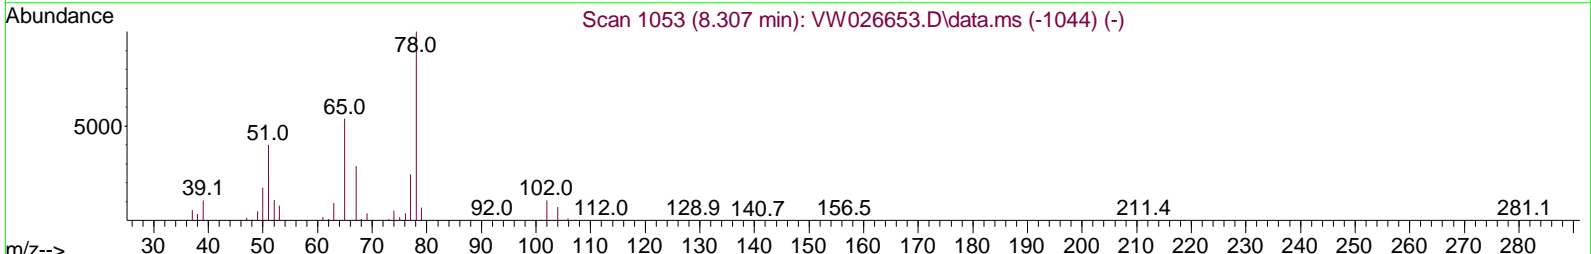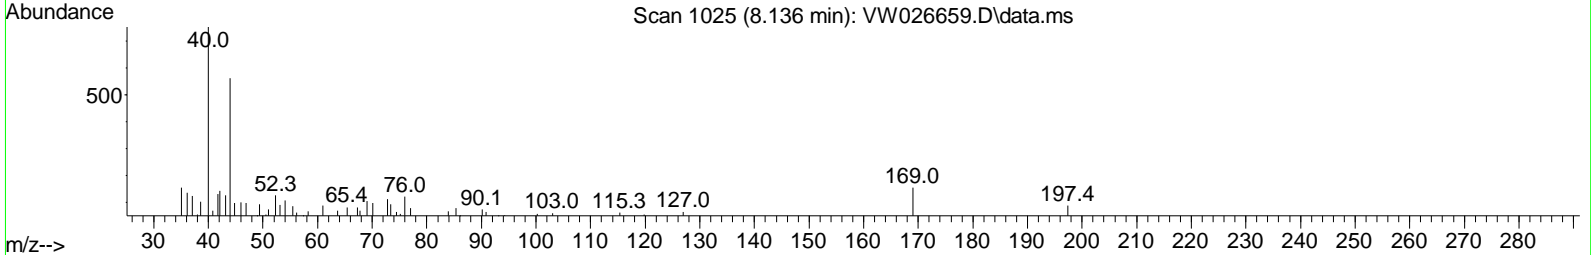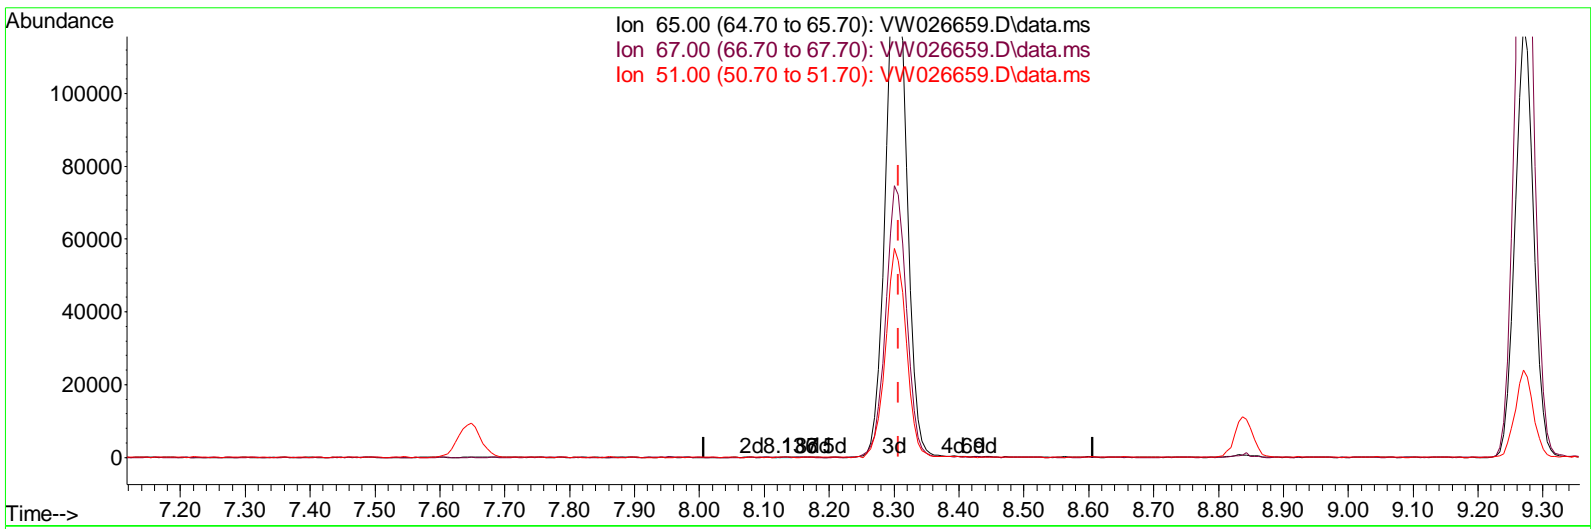

TIC: VW026659.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.136min (-0.171) 0.01 ug/L

response	90	
Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.00	57.78
51.00	100.50	80.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072623\
 Data File : VW026659.D
 Acq On : 26 Jul 2023 14:26
 Operator : SY/MD
 Sample : 03754-12
 Mi sc : 3.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BH2T5

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 07/27/2023
 Supervised By : Mahesh Dadoda 07/27/2023

Quant Time: Jul 27 03:02:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMLM071123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 27 03:01:27 2023
 Response via : Initial Calibration

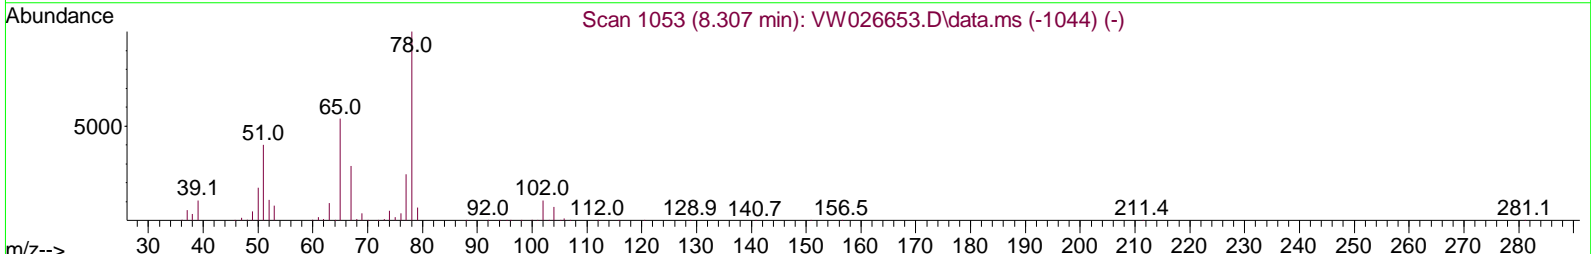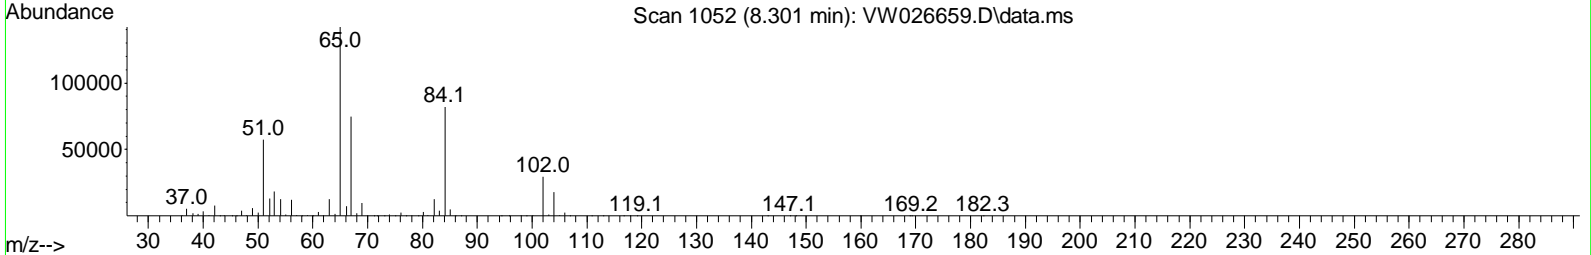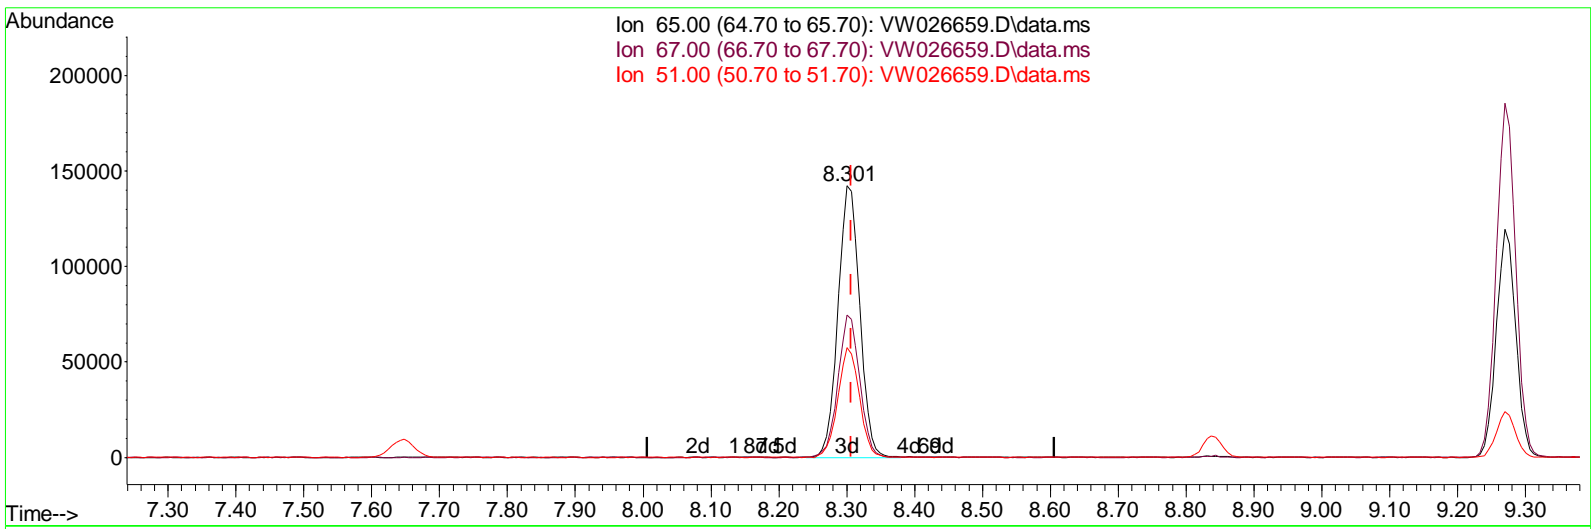

TIC: VW026659.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.301min (-0.006) 20.19 ug/L m

response	315136
Ion	Exp% Act%
65.00	100.00 100.00
67.00	53.00 0.02#
51.00	100.50 0.02#
0.00	0.00 0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\WV072623\
 Data File : WV026659.D
 Acq On : 26 Jul 2023 14:26
 Operator : SY/MD
 Sample : 03754-12
 Mi sc : 3.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BH2T5

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 07/27/2023
 Supervised By : Mahesh Dadoda 07/27/2023

Quant Time: Jul 27 03:02:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 27 03:01:27 2023
 Response via : Initial Calibration

Compound	R.T.	QI on	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	971022	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	869879	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	393333	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	246613	15.056	ug/L	0.00
Spike Amount	25.000	Range 30 - 150	Recovery =	60.240%		
7) Chloroethane-d5	2.893	69	199331	17.343	ug/L	0.00
Spike Amount	25.000	Range 30 - 150	Recovery =	69.360%		
11) 1,1-Dichloroethene-d2	4.021	65	124060	16.128	ug/L	0.00
Spike Amount	25.000	Range 45 - 110	Recovery =	64.520%		
21) 2-Butanone-d5	7.075	46	166276	31.411	ug/L	0.00
Spike Amount	50.000	Range 20 - 135	Recovery =	62.820%		
24) Chloroform-d	7.648	84	570709	20.414	ug/L	0.00
Spike Amount	25.000	Range 40 - 150	Recovery =	81.640%		
26) 1,2-Dichloroethane-d4	8.301	65	315136m	20.189	ug/L	0.00
Spike Amount	25.000	Range 70 - 130	Recovery =	80.760%		
32) Benzene-d6	8.270	84	1129538	18.915	ug/L	0.00
Spike Amount	25.000	Range 20 - 135	Recovery =	75.680%		
36) 1,2-Dichloropropane-d6	9.270	67	367773	20.030	ug/L	0.00
Spike Amount	25.000	Range 70 - 120	Recovery =	80.120%		
41) Toluene-d8	10.319	98	942912	18.410	ug/L	0.00
Spike Amount	25.000	Range 30 - 130	Recovery =	73.640%		
43) trans-1,3-Dichloroprop...	10.575	79	133781	18.181	ug/L	0.00
Spike Amount	25.000	Range 30 - 135	Recovery =	72.720%		
47) 2-Hexanone-d5	10.922	63	109085	30.446	ug/L	0.00
Spike Amount	50.000	Range 20 - 135	Recovery =	60.900%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	273080	17.562	ug/L	0.00
Spike Amount	25.000	Range 45 - 120	Recovery =	70.240%		
66) 1,2-Dichlorobenzene-d4	13.848	152	285729	19.786	ug/L	0.00
Spike Amount	25.000	Range 75 - 120	Recovery =	79.160%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072623\
 Data File : VW026659.D
 Acq On : 26 Jul 2023 14:26
 Operator : SY/MD
 Sample : 03754-12
 Mi sc : 3.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BH2T5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/27/2023
 Supervised By :Mahesh Dadoda 07/27/2023

Quant Time: Jul 27 03:02:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMLM071123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 27 03:01:27 2023
 Response via : Initial Calibration

