

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW072718\
 Data File : VW004232.D
 Acq On : 26 Jul 2018 17:07
 Operator : SY/AP
 Sample : J4040-04
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 27 02:55:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 27 02:54:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	375536	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	352394	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	160433	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.34	65	96127	25.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.68%
7) Chloroethane-d5	2.89	69	68815	25.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.12%
10) 1,1-Dichloroethene-d2	4.00	63	172225	19.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.32%
20) 2-Butanone-d5	7.08	46	115107	53.78	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.56%
24) Chloroform-d	7.65	84	247020	25.69	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.76%
26) 1,2-Dichloroethane-d4	8.31	65	153872	26.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.44%
29) Benzene-d6	8.27	84	500317	26.79	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.16%
33) 1,2-Dichloropropane-d6	9.27	67	164698	26.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.04%
37) Toluene-d8	10.33	98	467961	26.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	106.04%
38) trans-1,3-Dichloropropene-	10.58	79	72789	25.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	103.28%
39) 2-Hexanone-d5	10.93	63	83996	51.46	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.92%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	162692	25.65	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.60%
61) 1,2-Dichlorobenzene-d4	13.86	152	170525	28.43	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	113.72%


Target Compounds					Ovalue
13) Acetone	4.12	43	4475	2.071 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW072718\
Data File : VW004232.D
Acq On : 26 Jul 2018 17:07
Operator : SY/AP
Sample : J4040-04
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jul 27 02:55:46 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 27 02:54:01 2018
Response via : Initial Calibration

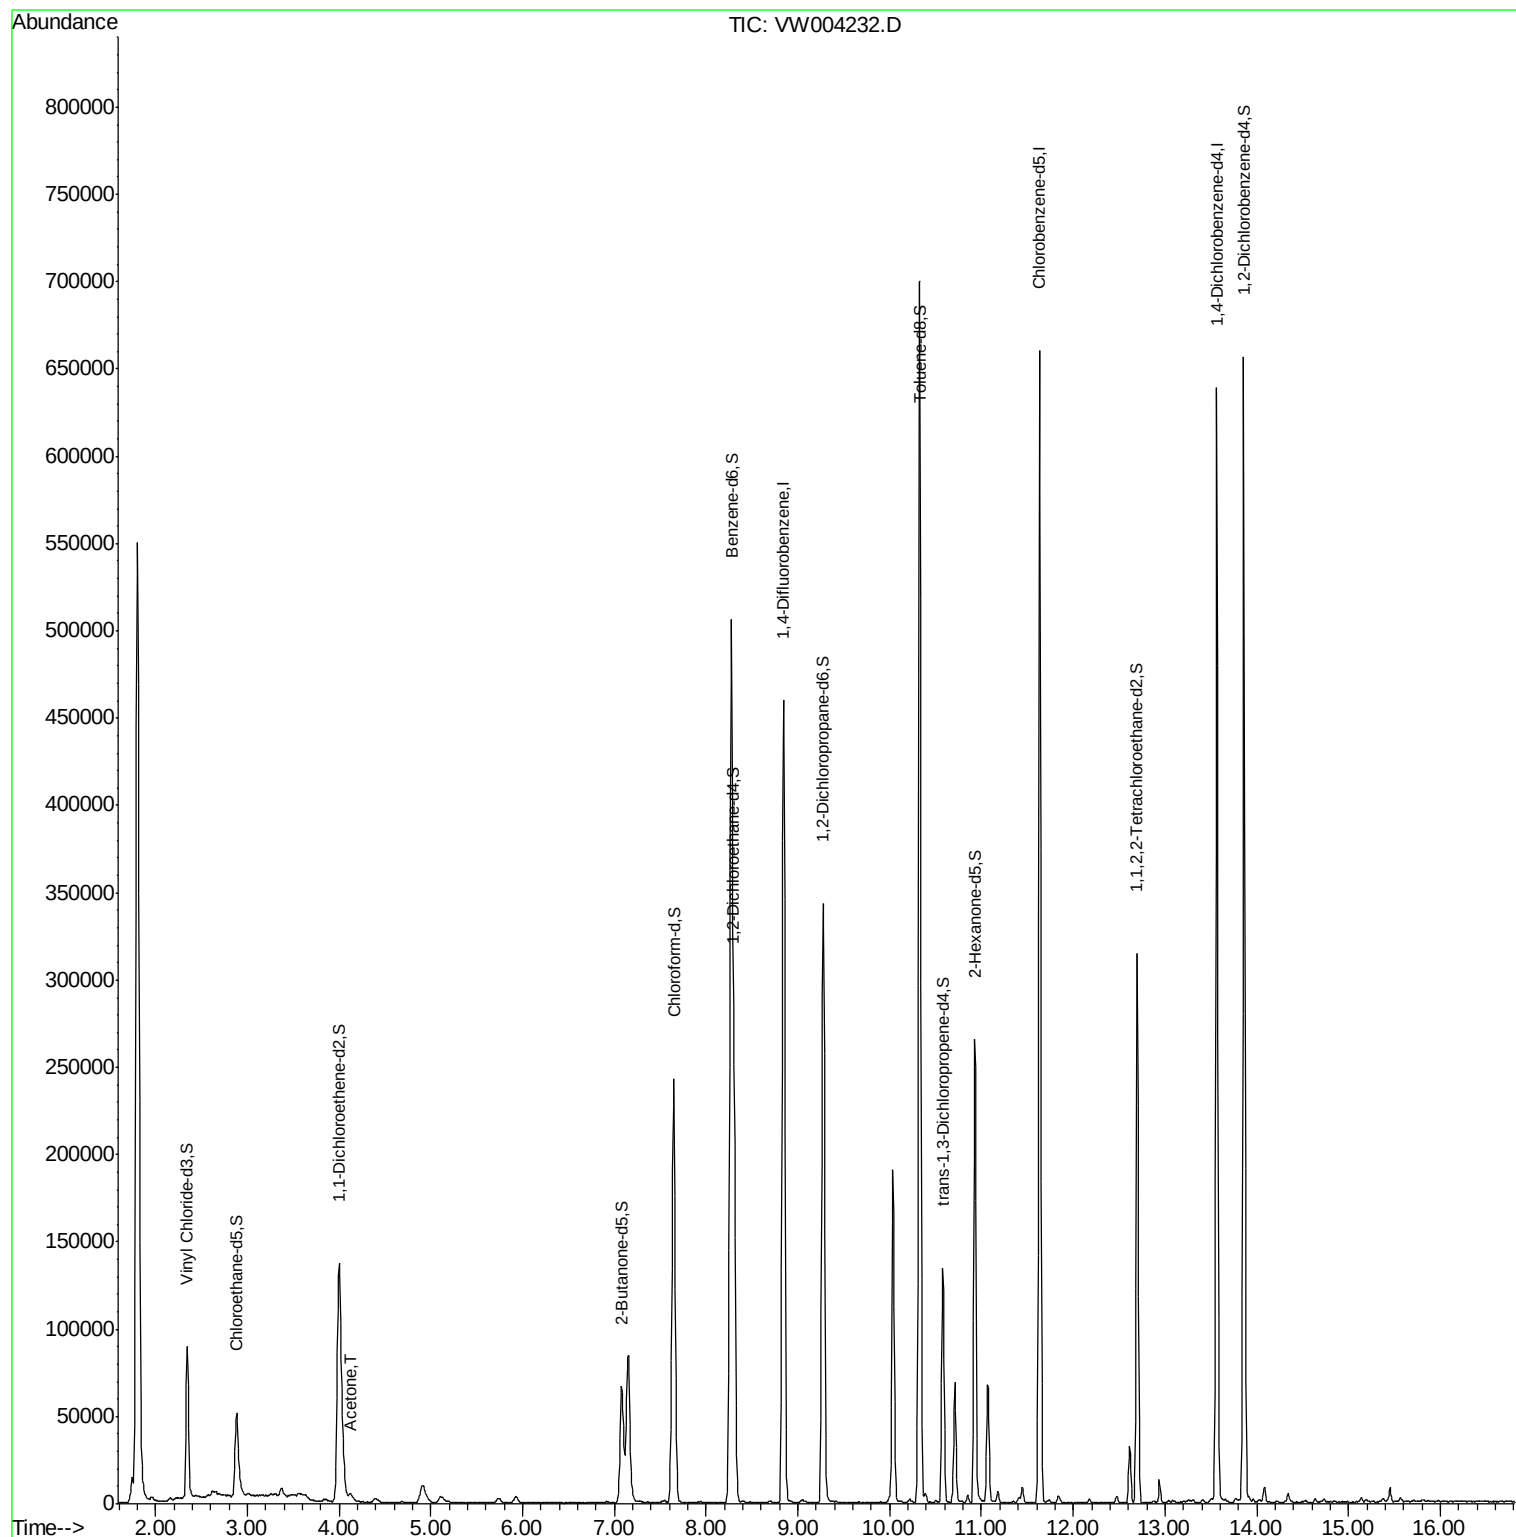

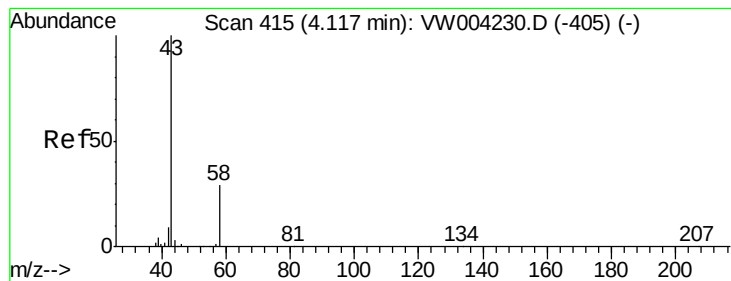

#13

Acetone

Concen: 2.071 ug/L

RT: 4.12 min Scan# 415

Delta R.T. -0.00 min

Lab File: VW004232.D

Acq: 26 Jul 2018 17:07

Instrument :
MSVOA_W
ClientSampleId :

Tot Ion: 43 Resp: 4475

Ion Ratio Lower Upper

43 100

58 29.7 0.0 59.8

