


Data File : VW004224.D
Acq On : 26 Jul 2018 11:56
Operator : SY/AP
Sample : VSTD2.585
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 13:50:44 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 26 13:44:32 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
VSTD2.585

Manual Integrations
APPROVED

MMDadoda
7/30/2018 11:42:31 AM

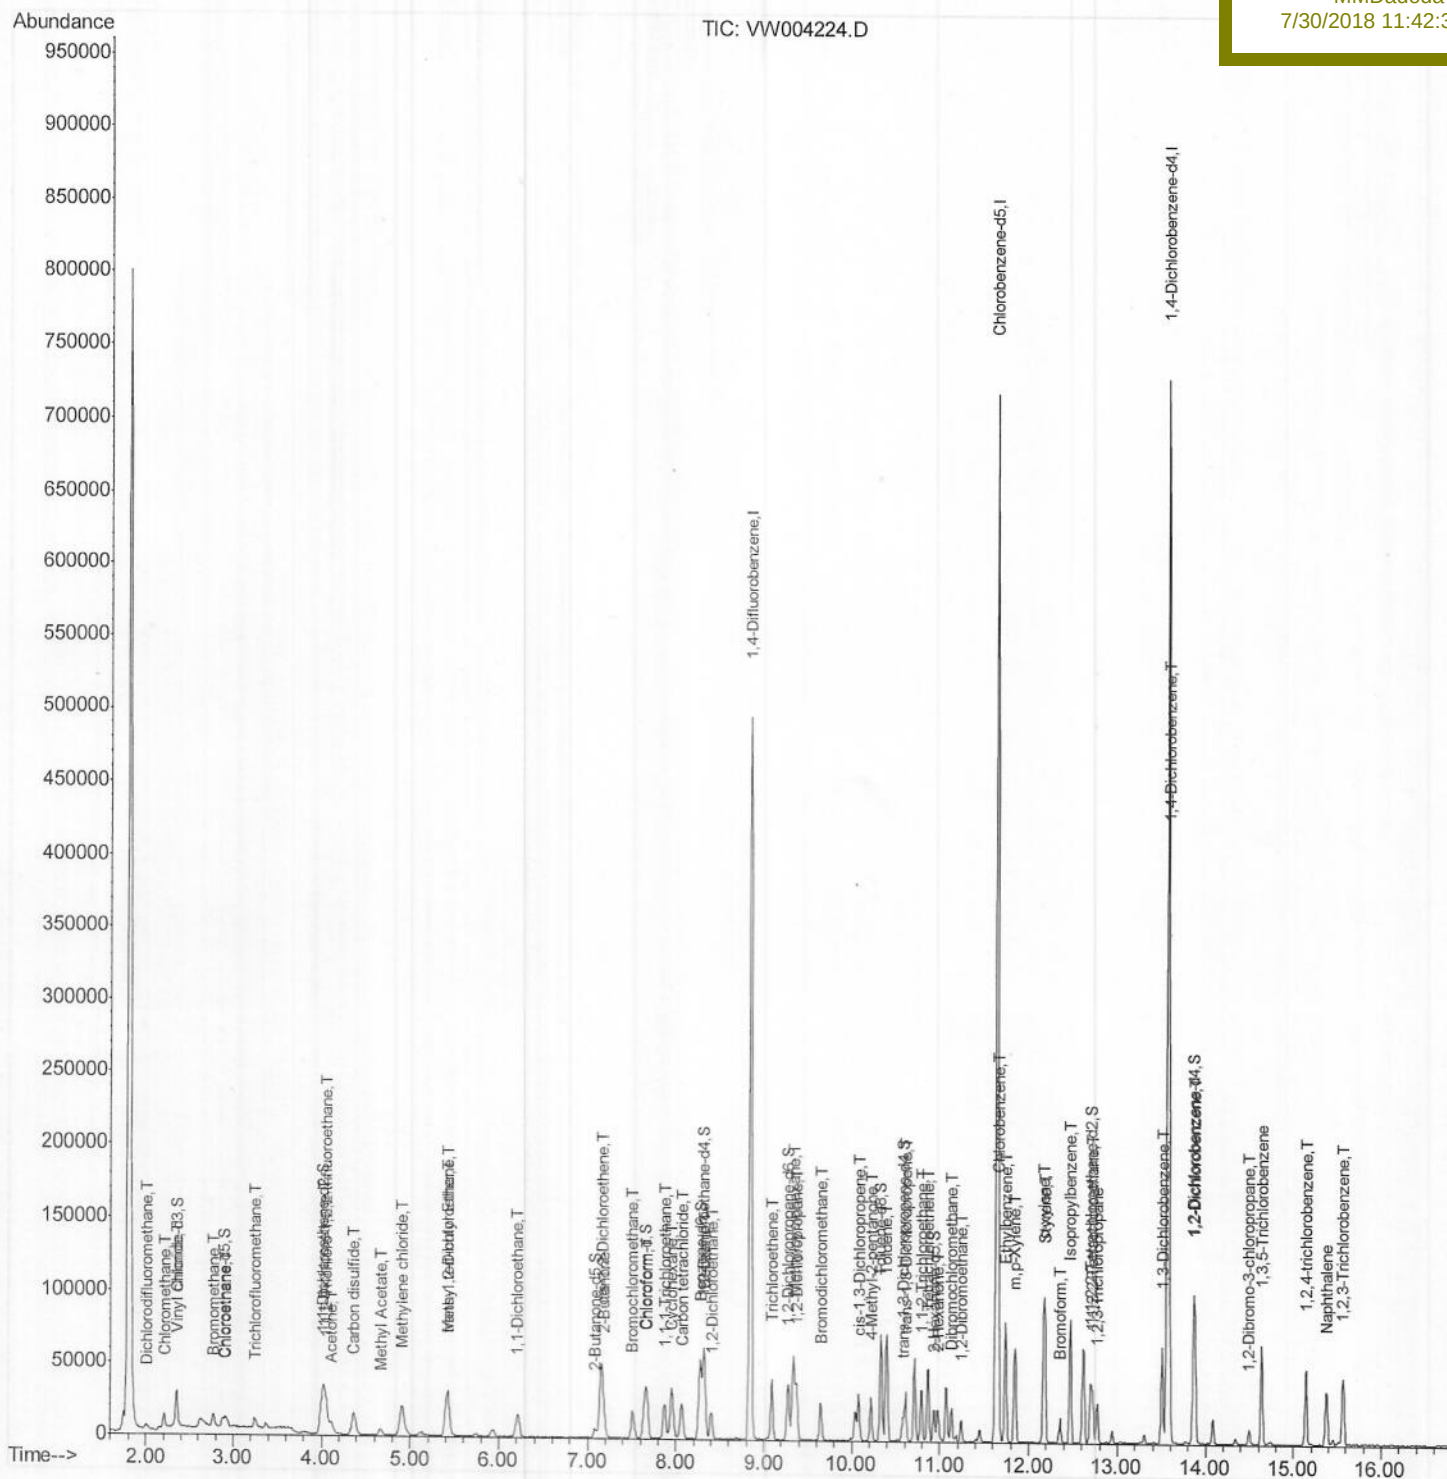

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072718\
Quantitation Report (Qedit)


Data File : VW004224.D
Acq On : 26 Jul 2018 11:56
Operator : SY/AP
Sample : VSTD2.585
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 13:44:34 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 26 13:44:32 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.585

Manual Integrations
APPROVED

MMDadoda
7/30/2018 11:42:31 AM

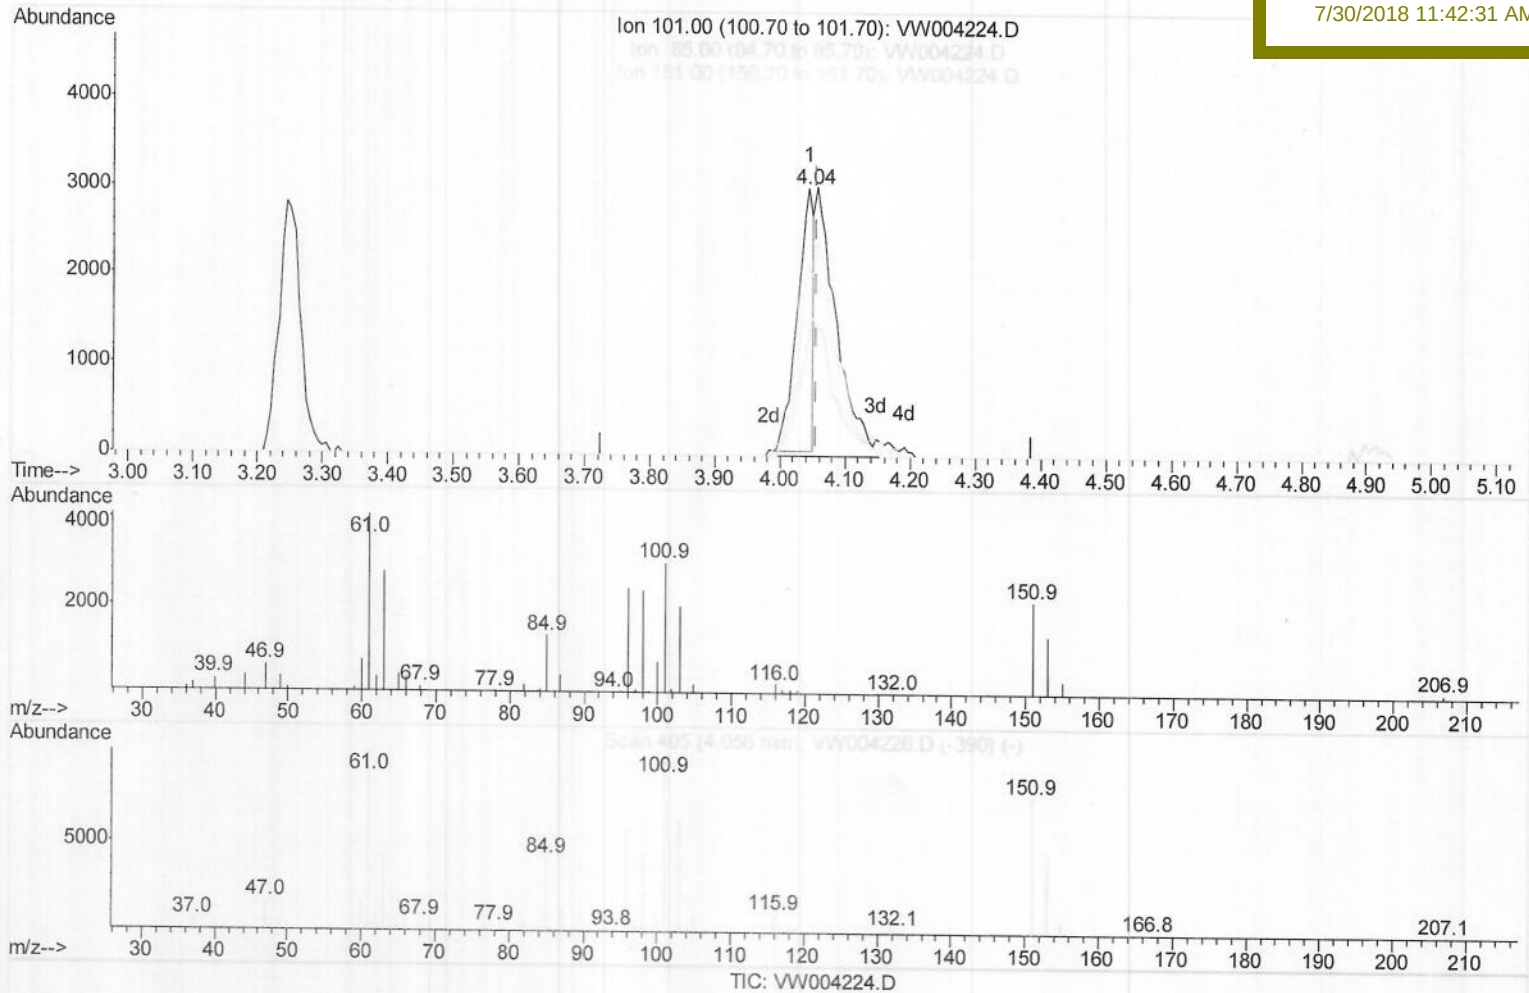

(11) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

4.044min (-0.012) 0.93ug/L

response 5157

Ion	Exp%	Act%
101.00	100	100
85.00	44.80	107.95#
151.00	79.30	71.96
0.00	0.00	0.00


Data File : VW004224.D
Acq On : 26 Jul 2018 11:56
Operator : SY/AP
Sample : VSTD2.585
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 13:44:34 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 26 13:44:32 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sample Id :
VSTD2.585

Manual Integrations
APPROVED

MMDadoda
7/30/2018 11:42:31 AM

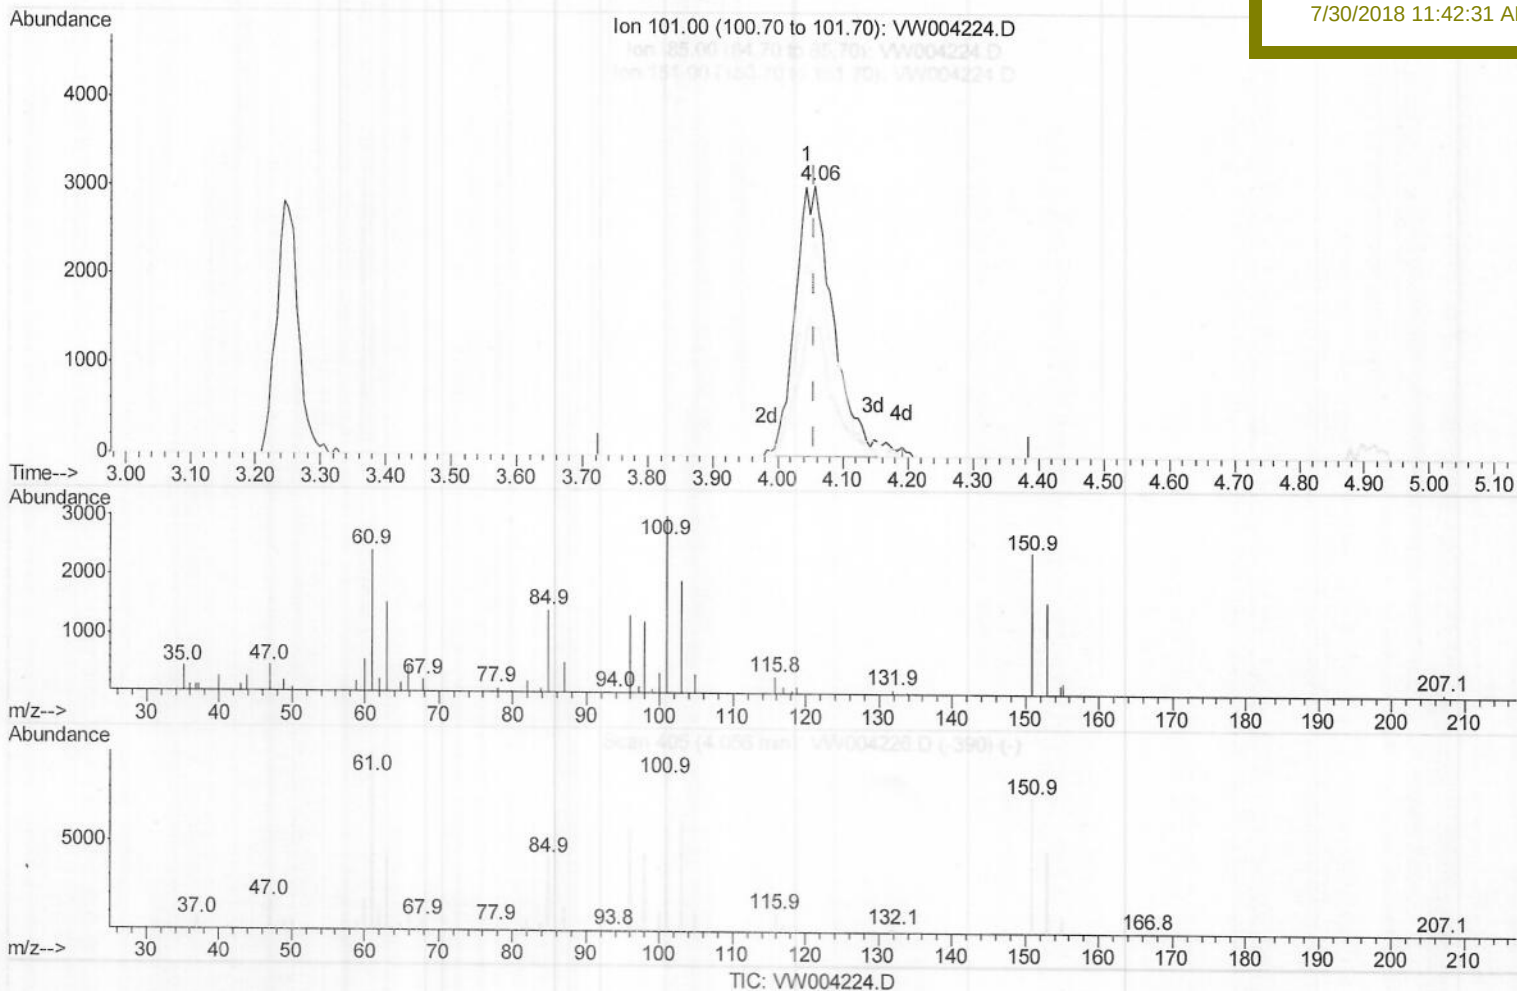

(11) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

4.056min (+0.000) 2.25ug/L m *MD 07/31/18*

response 12405

Ion	Exp%	Act%
101.00	100	100
85.00	44.80	44.88
151.00	79.30	29.92#
0.00	0.00	0.00




Data File : VW004224.D
Acq On : 26 Jul 2018 11:56
Operator : SY/AP
Sample : VSTD2.585
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 13:44:34 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 26 13:44:32 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.585

Manual Integrations
APPROVED

MMDadoda
7/30/2018 11:42:31 AM

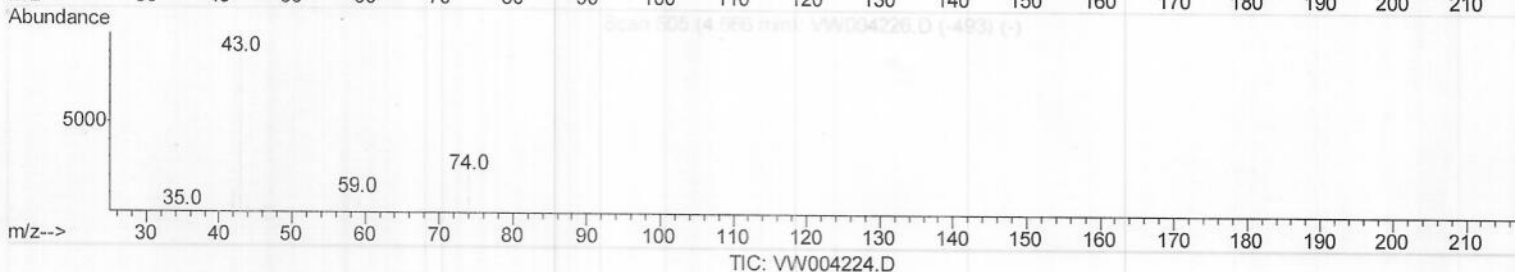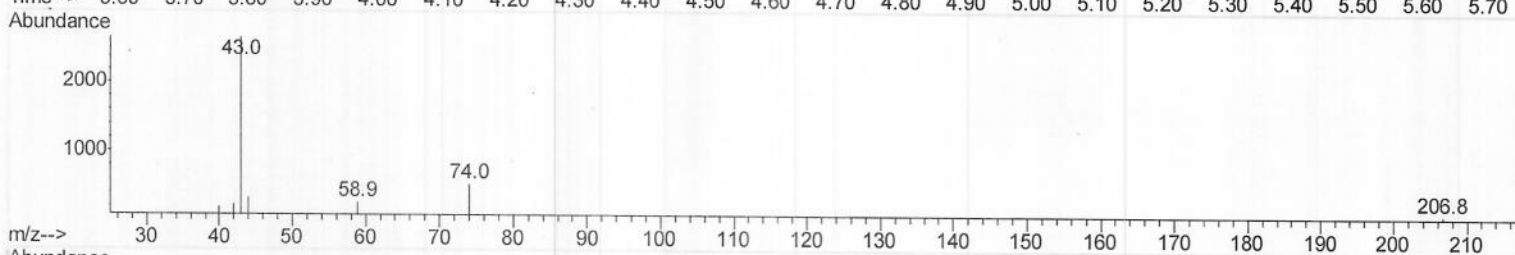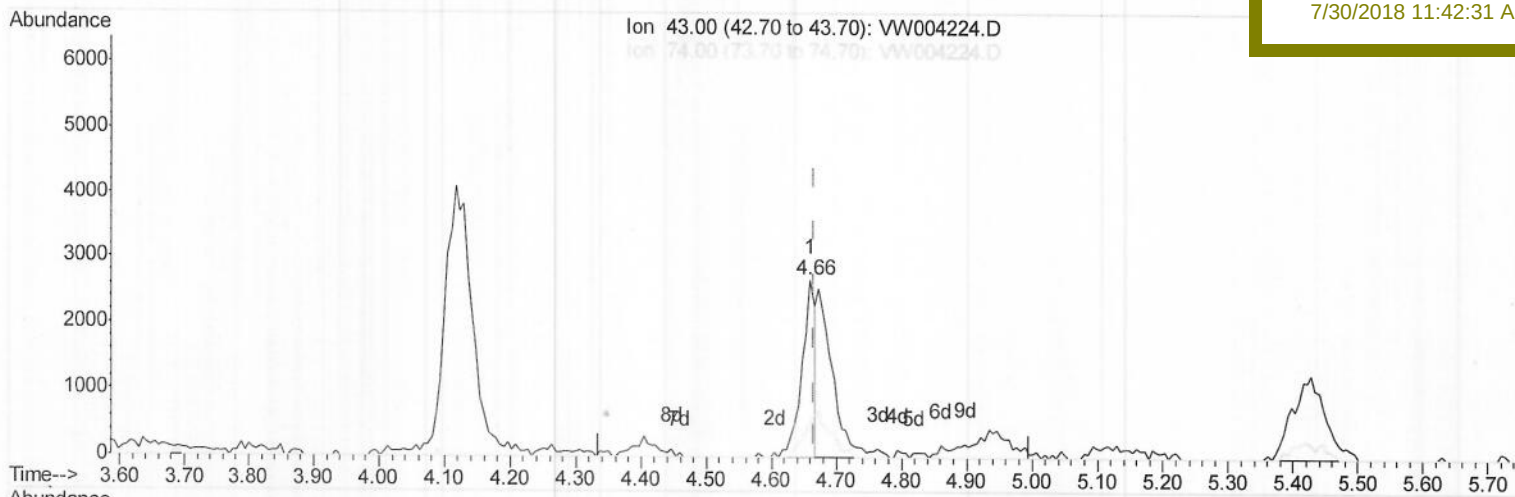

(15) Methyl Acetate (T)

4.660min (-0.006) 0.84ug/L

response 3668

Ion	Exp%	Act%
43.00	100	100
74.00	21.30	49.05#
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VW004224.D
Acq On : 26 Jul 2018 11:56
Operator : SY/AP
Sample : VSTD2.585
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 13:44:34 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 26 13:44:32 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
VSTD2.585

Manual Integrations
APPROVED

MMDadoda
7/30/2018 11:42:31 AM

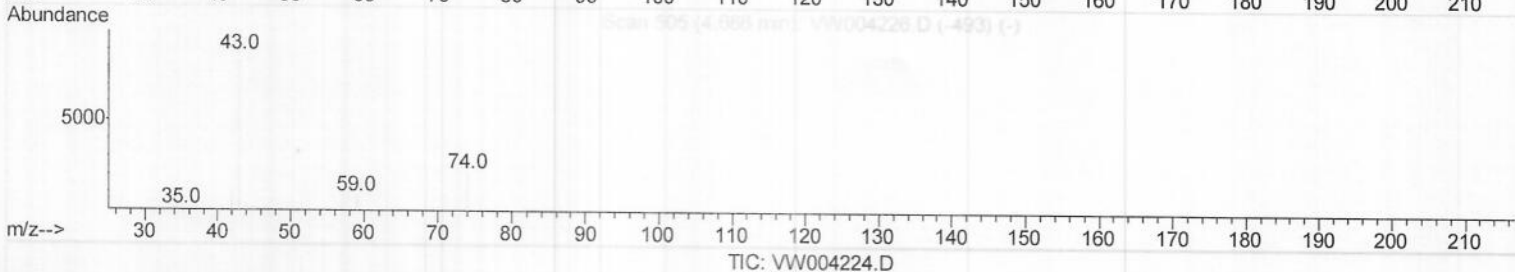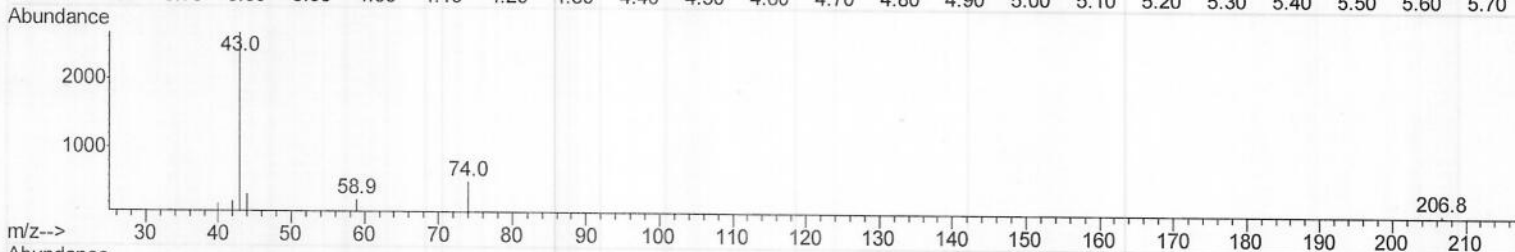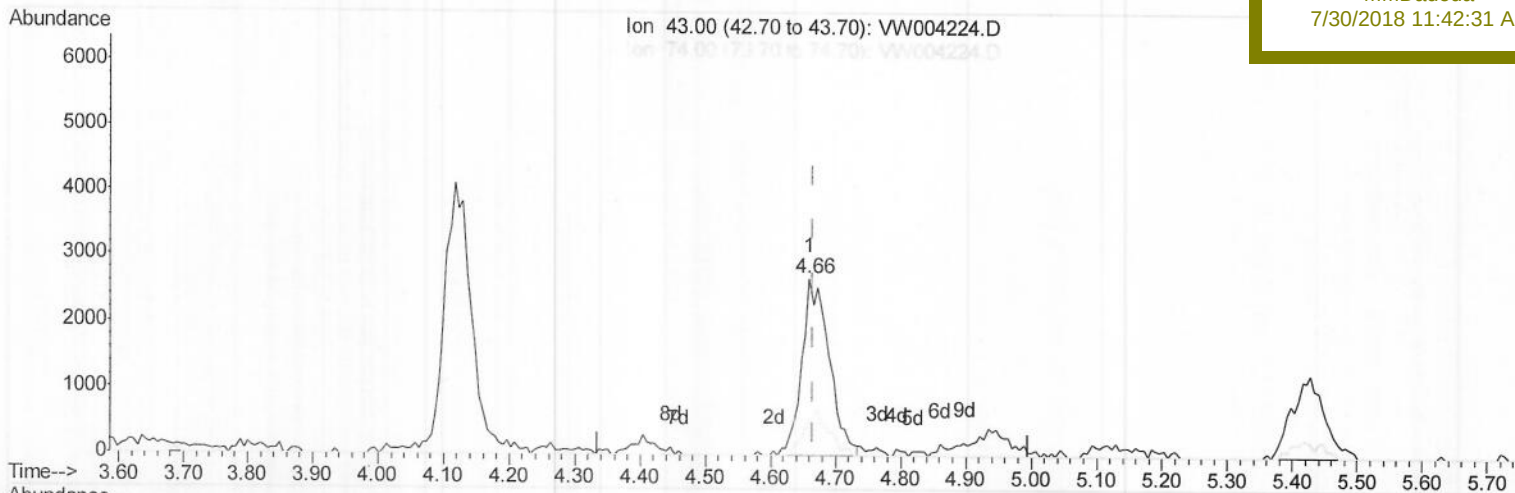

(15) Methyl Acetate (T)

4.660min (-0.006) 1.81ug/L m) MD 07/31/18

response 7861

Ion	Exp%	Act%
43.00	100	100
74.00	21.30	22.89
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VW004224.D

Acq On : 26 Jul 2018 11:56

Operator : SY/AP

Sample : VSTD2.585

Misc : 5.00G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 13:50:44 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M

Quant Title : VOC Analysis

QLast Update : Thu Jul 26 13:44:32 2018

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :

VSTD2.585

Manual Integrations

APPROVED

MMDadoda

7/30/2018 11:42:31 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	403976	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	387066	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	184524	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	12721	3.18	ug/L	0.00
7) Chloroethane-d5	2.89	69	8158	2.83	ug/L	0.00
10) 1,1-Dichloroethene-d2	4.00	63	26408	2.75	ug/L	-0.01
20) 2-Butanone-d5	7.08	46	9636	4.11	ug/L	0.00
24) Chloroform-d	7.65	84	27882	2.91	ug/L	0.00
26) 1,2-Dichloroethane-d4	8.31	65	16450	2.85	ug/L	0.00
29) Benzene-d6	8.27	84	51223	2.85	ug/L	0.00
33) 1,2-Dichloropropane-d6	9.27	67	18359	3.07	ug/L	0.00
37) Toluene-d8	10.32	98	47888	2.97	ug/L	0.00
38) trans-1,3-Dichloropropene-	10.58	79	7492	2.85	ug/L	0.00
39) 2-Hexanone-d5	10.93	63	6409	3.98	ug/L	0.00
48) 1,1,2,2-Tetrachloroethane-	12.70	84	17356	2.65	ug/L	0.00
61) 1,2-Dichlorobenzene-d4	13.86	152	19046	3.21	ug/L	0.00

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	2.00	85	5637	2.179	ug/L	89
3) Chloromethane	2.21	50	9635	2.330	ug/L	91
5) Vinyl chloride	2.36	62	13750	2.208	ug/L	91
6) Bromomethane	2.78	94	6748	2.041	ug/L	96
8) Chloroethane	2.92	64	6416	1.966	ug/L	88
9) Trichlorofluoromethane	3.25	101	6440	2.076	ug/L	95
11) 1,1,2-Trichloro-1,2,2-trif	4.06	101	12405m	2.249	ug/L	85
12) 1,1-Dichloroethene	4.02	96	11328	2.107	ug/L	99
13) Acetone	4.12	43	11162	4.382	ug/L	100
14) Carbon disulfide	4.37	76	36280	2.085	ug/L	98
15) Methyl Acetate	4.66	43	7861m	1.809	ug/L	94
16) Methylene chloride	4.90	84	17570	2.267	ug/L	97
17) Methyl tert-butyl Ether	5.42	73	18744	1.802	ug/L	94
18) trans-1,2-Dichloroethene	5.42	96	11328	2.046	ug/L	97
19) 1,1-Dichloroethane	6.21	63	22349	2.122	ug/L	94
21) 2-Butanone	7.18	43	12118	3.834	ug/L	80
22) cis-1,2-Dichloroethene	7.17	96	12018	2.031	ug/L	95
23) Bromochloromethane	7.51	128	5980	2.149	ug/L	97
25) Chloroform	7.67	83	23056	2.144	ug/L	99
27) 1,2-Dichloroethane	8.40	62	17090	2.156	ug/L	97
30) Cyclohexane	7.95	56	15819	1.676	ug/L	96
31) 1,1,1-Trichloroethane	7.87	97	17965	2.041	ug/L	98
32) Carbon tetrachloride	8.07	117	17097	2.013	ug/L	97
34) Benzene	8.32	78	49107	2.070	ug/L	100
35) Trichloroethene	9.09	95	14120	2.224	ug/L	98
36) Methylcyclohexane	9.34	83	20074	1.913	ug/L	92
40) 1,2-Dichloropropane	9.37	63	13867	2.156	ug/L	97
41) Bromodichloromethane	9.65	83	17367	2.193	ug/L	96
42) cis-1,3-Dichloropropene	10.07	75	18012	1.987	ug/L	92
43) 4-Methyl-2-pentanone	10.21	43	19430	3.436	ug/L	96

MMD07/31/18

Data File : VW004224.D
 Acq On : 26 Jul 2018 11:56
 Operator : SY/AP
 Sample : VSTD2.585
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 13:50:44 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 26 13:44:32 2018
 Response via : Initial Calibration

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.585

Manual Integrations
 APPROVED

MMDadoda
 7/30/2018 11:42:31 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) Toluene	10.39	91	52518	2.112	ug/L	99
45) trans-1,3-Dichloropropene	10.61	75	17350	2.075	ug/L	100
46) 1,1,2-Trichloroethane	10.79	97	10933	2.187	ug/L	98
47) Tetrachloroethene	10.87	164	11085	2.165	ug/L	96
49) 2-Hexanone	10.97	43	14962	3.418	ug/L	95
50) Dibromochloromethane	11.13	129	12036	2.149	ug/L	94
51) 1,2-Dibromoethane	11.24	107	10118	2.072	ug/L #	98
52) Chlorobenzene	11.66	112	35856	2.249	ug/L	97
53) Ethylbenzene	11.74	91	55133	2.049	ug/L	98
54) m,p-Xylene	11.85	106	20357	2.052	ug/L	98
55) o-xylene	12.17	106	18277	1.926	ug/L	98
56) Styrene	12.19	104	29027	1.771	ug/L	95
57) Isopropylbenzene	12.47	105	48068	1.848	ug/L	99
58) 1,1,2,2-Tetrachloroethane	12.72	83	14731	2.062	ug/L	97
59) 1,2,3-Trichloropropane	12.77	75	11208	2.026	ug/L	95
62) Bromoform	12.35	173	7301	2.097	ug/L #	96
63) 1,3-Dichlorobenzene	13.51	146	26131	2.299	ug/L	99
64) 1,4-Dichlorobenzene	13.58	146	28457	2.335	ug/L	96
65) 1,2-Dichlorobenzene	13.88	146	25266	2.281	ug/L	95
66) 1,2-Dibromo-3-chloropropan	14.49	75	2563	1.985	ug/L #	79
67) 1,3,5-Trichlorobenzene	14.64	180	20980	2.334	ug/L	97
68) 1,2,4-trichlorobenzene	15.15	180	15936	2.211	ug/L	98
69) Naphthalene	15.38	128	30144	1.858	ug/L	99
70) 1,2,3-Trichlorobenzene	15.57	180	15122	2.205	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed