


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW072718\
Data File : VW004222.D
Acq On : 26 Jul 2018 09:21
Operator : SY/AP
Sample : BFB87
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB87

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
Title : VOC Analysis
Last Update : Sat Jul 28 02:53:40 2018

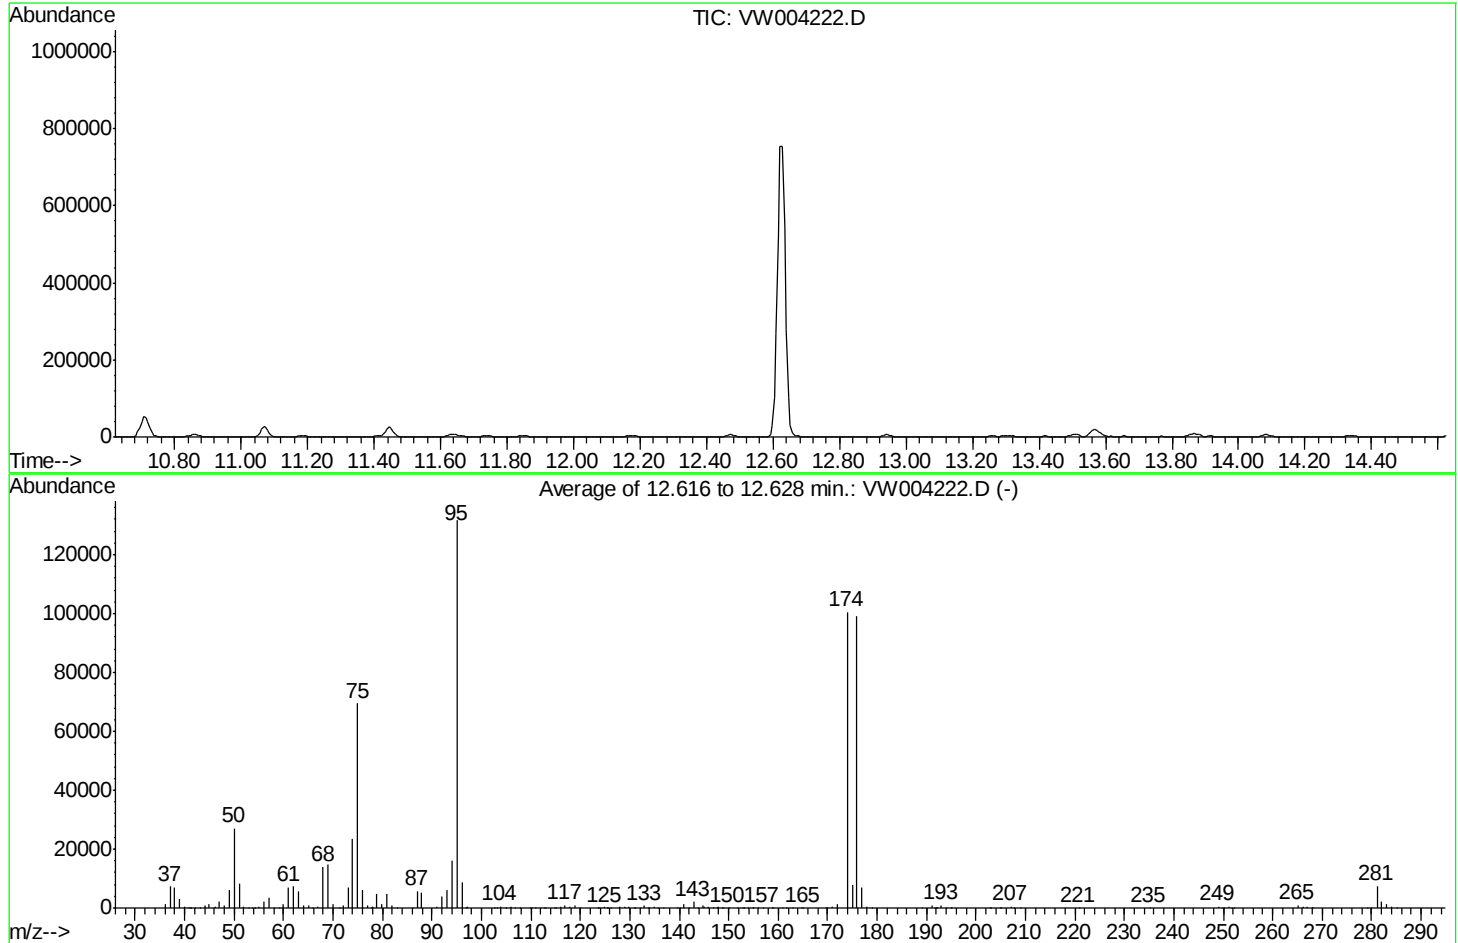

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	27152	PASS
75	95	30	80	52.8	69506	PASS
95	95	100	100	100.0	131637	PASS
96	95	5	9	6.6	8722	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.4	100632	PASS
175	174	5	9	7.6	7656	PASS
176	174	95	101	98.4	98994	PASS
177	176	5	9	6.8	6761	PASS

Scan 1802 (12.573 min): VW004222.D
BFB87

m/z	Abundance
39.80	177.0
43.80	254.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

m/z	Abundance
36.00	1036.0
37.00	5898.0
38.00	5532.0
39.10	2264.0
40.00	273.0
41.10	127.0
42.20	65.0
43.00	168.0
44.10	819.0
45.00	1298.0
46.00	291.0
47.00	1604.0
47.90	785.0
49.00	4737.0
50.00	22392.0
51.00	6850.0
52.00	313.0
52.90	193.0
54.10	60.0
55.00	349.0
56.00	1747.0
57.00	2825.0
58.00	82.0
59.20	188.0
60.00	1084.0
61.00	5405.0
62.00	5999.0
63.00	4886.0
63.90	1106.0
65.00	948.0
66.00	102.0
67.10	255.0
68.00	10830.0
69.00	11822.0
70.00	959.0
71.90	491.0
73.00	5650.0
74.00	18136.0
75.00	54184.0
76.00	5247.0
77.00	618.0
77.80	411.0
78.90	3780.0
79.90	998.0
80.90	3997.0
81.90	769.0
83.00	119.0
86.00	204.0
87.00	4143.0
87.90	4104.0
90.90	482.0
92.00	3074.0
93.00	4596.0
94.00	11930.0
95.00	101984.0
96.00	7260.0
96.90	217.0
102.70	151.0
103.90	539.0
104.80	281.0
105.90	472.0
106.80	115.0
109.80	61.0
110.20	109.0
111.00	91.0
112.70	91.0
114.80	195.0
116.00	301.0
116.90	906.0
117.80	448.0
118.90	903.0
120.00	57.0
123.90	80.0
124.90	452.0
125.20	467.0
126.10	136.0
127.90	309.0
128.90	218.0
129.90	347.0
130.70	174.0
131.00	178.0
132.90	748.0
133.60	219.0
135.00	313.0
136.90	92.0
140.00	93.0
140.90	864.0
141.90	188.0
142.90	1595.0
143.80	167.0
144.90	905.0
145.80	220.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

146.90	236.0
147.70	159.0
147.90	160.0
148.90	162.0
150.00	136.0
153.10	74.0
153.80	101.0
154.80	337.0
155.80	68.0
156.90	158.0
158.80	81.0
161.00	228.0
161.70	74.0
162.90	169.0
165.10	59.0
170.90	378.0
171.90	887.0
173.90	69376.0
175.00	5205.0
175.90	69200.0
177.00	4662.0
177.90	225.0
178.80	231.0
189.00	114.0
191.00	789.0
192.00	212.0
192.90	1115.0
193.90	182.0
194.90	141.0
202.80	119.0
205.00	163.0
207.00	719.0
207.80	183.0
209.00	119.0
220.80	72.0
235.10	135.0
249.00	552.0
249.80	176.0
251.00	462.0
252.10	53.0
265.10	1428.0
266.10	281.0
267.10	351.0
267.90	85.0
268.10	87.0
279.10	145.0
281.10	7796.0
282.00	2155.0
283.00	1568.0
284.00	313.0
285.10	93.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

m/z	Abundance
36.00	1275.0
37.00	8377.0
38.00	7631.0
39.00	3412.0
40.10	339.0
41.00	113.0
42.10	55.0
42.90	164.0
44.00	874.0
45.00	1559.0
46.10	241.0
47.00	2152.0
48.00	1133.0
49.00	6695.0
50.00	30120.0
51.00	9286.0
52.00	415.0
53.00	233.0
54.10	75.0
54.90	446.0
56.00	2064.0
57.00	3917.0
58.00	201.0
59.00	226.0
60.00	1518.0
61.00	7962.0
62.00	8357.0
63.00	6419.0
63.90	1139.0
65.00	1017.0
65.90	150.0
67.00	403.0
68.00	15426.0
69.00	16146.0
70.00	1302.0
72.00	906.0
73.00	7911.0
74.00	25848.0
75.00	79000.0
76.00	6787.0
76.90	952.0
78.00	631.0
78.90	5304.0
79.90	1484.0
80.90	5321.0
81.90	1186.0
83.00	130.0
85.90	263.0
86.90	6586.0
87.90	5745.0
90.90	456.0
92.00	4349.0
93.00	6488.0
94.00	17928.0
95.00	151616.0
96.00	9597.0
97.10	397.0
103.00	273.0
103.90	744.0
104.80	193.0
105.80	578.0
106.90	208.0
110.00	186.0
110.80	162.0
111.80	176.0
112.80	111.0
115.00	235.0
115.90	456.0
116.90	1164.0
117.80	502.0
118.90	1220.0
119.90	88.0
123.90	92.0
124.80	297.0
125.30	183.0
125.60	196.0
128.00	638.0
128.90	271.0
129.80	697.0
130.90	278.0
132.00	86.0
132.90	756.0
133.90	234.0
134.80	312.0
135.80	54.0
136.70	257.0
140.00	116.0
140.90	1353.0
141.80	178.0
142.90	2484.0
143.90	243.0
144.90	1128.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

145.90	254.0
147.00	208.0
147.90	457.0
149.00	163.0
149.90	131.0
152.00	77.0
152.80	109.0
153.80	98.0
154.80	326.0
155.80	90.0
157.00	209.0
159.00	124.0
160.80	172.0
162.80	229.0
165.10	104.0
169.70	92.0
171.00	420.0
172.00	1326.0
173.90	112720.0
174.90	8330.0
175.90	106616.0
176.90	7368.0
178.00	299.0
178.90	235.0
189.10	59.0
191.10	729.0
191.90	199.0
193.00	912.0
194.00	198.0
194.90	66.0
195.10	69.0
203.00	202.0
205.10	157.0
207.00	598.0
207.80	105.0
209.00	139.0
235.00	144.0
249.00	756.0
249.80	157.0
251.00	389.0
252.20	67.0
265.00	955.0
266.00	340.0
267.00	350.0
267.90	113.0
279.20	91.0
281.00	8295.0
282.10	2311.0
283.00	1512.0
284.10	308.0
284.90	95.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

m/z	Abundance
36.00	1599.0
37.00	7356.0
38.00	7579.0
39.00	2861.0
39.80	227.0
40.10	179.0
40.70	92.0
41.30	79.0
42.10	81.0
43.00	138.0
44.00	986.0
45.00	1367.0
46.10	245.0
47.00	2391.0
47.90	980.0
49.00	6501.0
50.00	28944.0
51.10	8584.0
52.00	428.0
53.00	163.0
53.80	65.0
55.00	510.0
56.00	2378.0
57.00	3965.0
58.10	187.0
58.90	124.0
60.00	1391.0
61.00	7985.0
62.00	7471.0
63.00	5912.0
64.00	890.0
65.00	1033.0
65.90	145.0
66.90	367.0
68.00	15736.0
69.00	15893.0
70.00	1104.0
71.20	55.0
71.90	959.0
73.00	7003.0
74.00	26208.0
75.00	75336.0
76.00	6389.0
76.90	954.0
77.90	554.0
78.90	4984.0
79.90	1204.0
80.90	4868.0
81.90	959.0
82.80	104.0
86.00	208.0
86.90	6376.0
88.00	5822.0
90.90	627.0
91.90	4470.0
93.00	6962.0
94.00	17824.0
95.00	141312.0
96.00	9310.0
97.00	304.0
103.10	161.0
103.90	587.0
105.00	246.0
105.90	694.0
106.80	223.0
107.80	66.0
109.80	90.0
110.10	107.0
110.70	112.0
111.00	90.0
111.90	89.0
113.00	94.0
115.00	240.0
115.90	560.0
116.90	1104.0
117.90	697.0
118.90	1053.0
123.60	54.0
125.00	219.0
125.70	125.0
127.90	598.0
128.90	238.0
129.80	702.0
131.10	167.0
133.00	697.0
133.90	93.0
134.90	461.0
135.80	82.0
136.80	229.0
139.70	74.0
140.10	79.0
140.90	1299.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

141.80	128.0
142.90	2015.0
143.80	175.0
145.10	751.0
145.80	280.0
147.00	147.0
147.90	308.0
148.70	194.0
149.90	136.0
151.80	79.0
152.80	119.0
153.10	117.0
153.90	148.0
155.00	380.0
155.80	68.0
157.00	299.0
158.90	145.0
160.90	203.0
162.90	178.0
164.70	63.0
170.00	127.0
170.80	490.0
171.90	1450.0
173.90	119800.0
175.00	9433.0
175.90	121168.0
176.90	8253.0
177.80	231.0
179.00	138.0
189.00	60.0
190.90	534.0
191.70	180.0
192.20	117.0
193.00	766.0
193.90	101.0
203.00	67.0
204.80	119.0
207.10	577.0
207.80	125.0
208.90	64.0
234.90	148.0
249.00	595.0
250.10	109.0
251.10	289.0
251.80	92.0
265.00	798.0
266.10	293.0
267.10	287.0
267.90	69.0
279.10	86.0
280.00	160.0
281.10	6667.0
282.10	2087.0
283.10	935.0
284.10	294.0
284.90	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87