

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW072719\
 Data File : VW011546.D
 Acq On : 27 Jul 2019 05:11
 Operator : SY/VA
 Sample : K4021-01
 Misc : 8.37G/5.0ML/MSVOA W/SOIL
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 TP-10

Quant Time: Jul 27 06:57:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 27 00:23:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	227260	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	378411	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	312990	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	127460	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	154572	59.23	ug/l	0.00
Spiked Amount	50.000		Recovery	=	118.46%	
35) Dibromofluoromethane	7.88	113	116065	54.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	109.34%	
50) Toluene-d8	10.32	98	461342	53.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.16%	
62) 4-Bromofluorobenzene	12.62	95	148438	47.90	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.80%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW072719\
Data File : VW011546.D
Acq On : 27 Jul 2019 05:11
Operator : SY/VA
Sample : K4021-01
Misc : 8.37G/5.0ML/MSVOA W/SOIL
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
TP-10

Quant Time: Jul 27 06:57:01 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W072719S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 27 00:23:30 2019
Response via : Initial Calibration

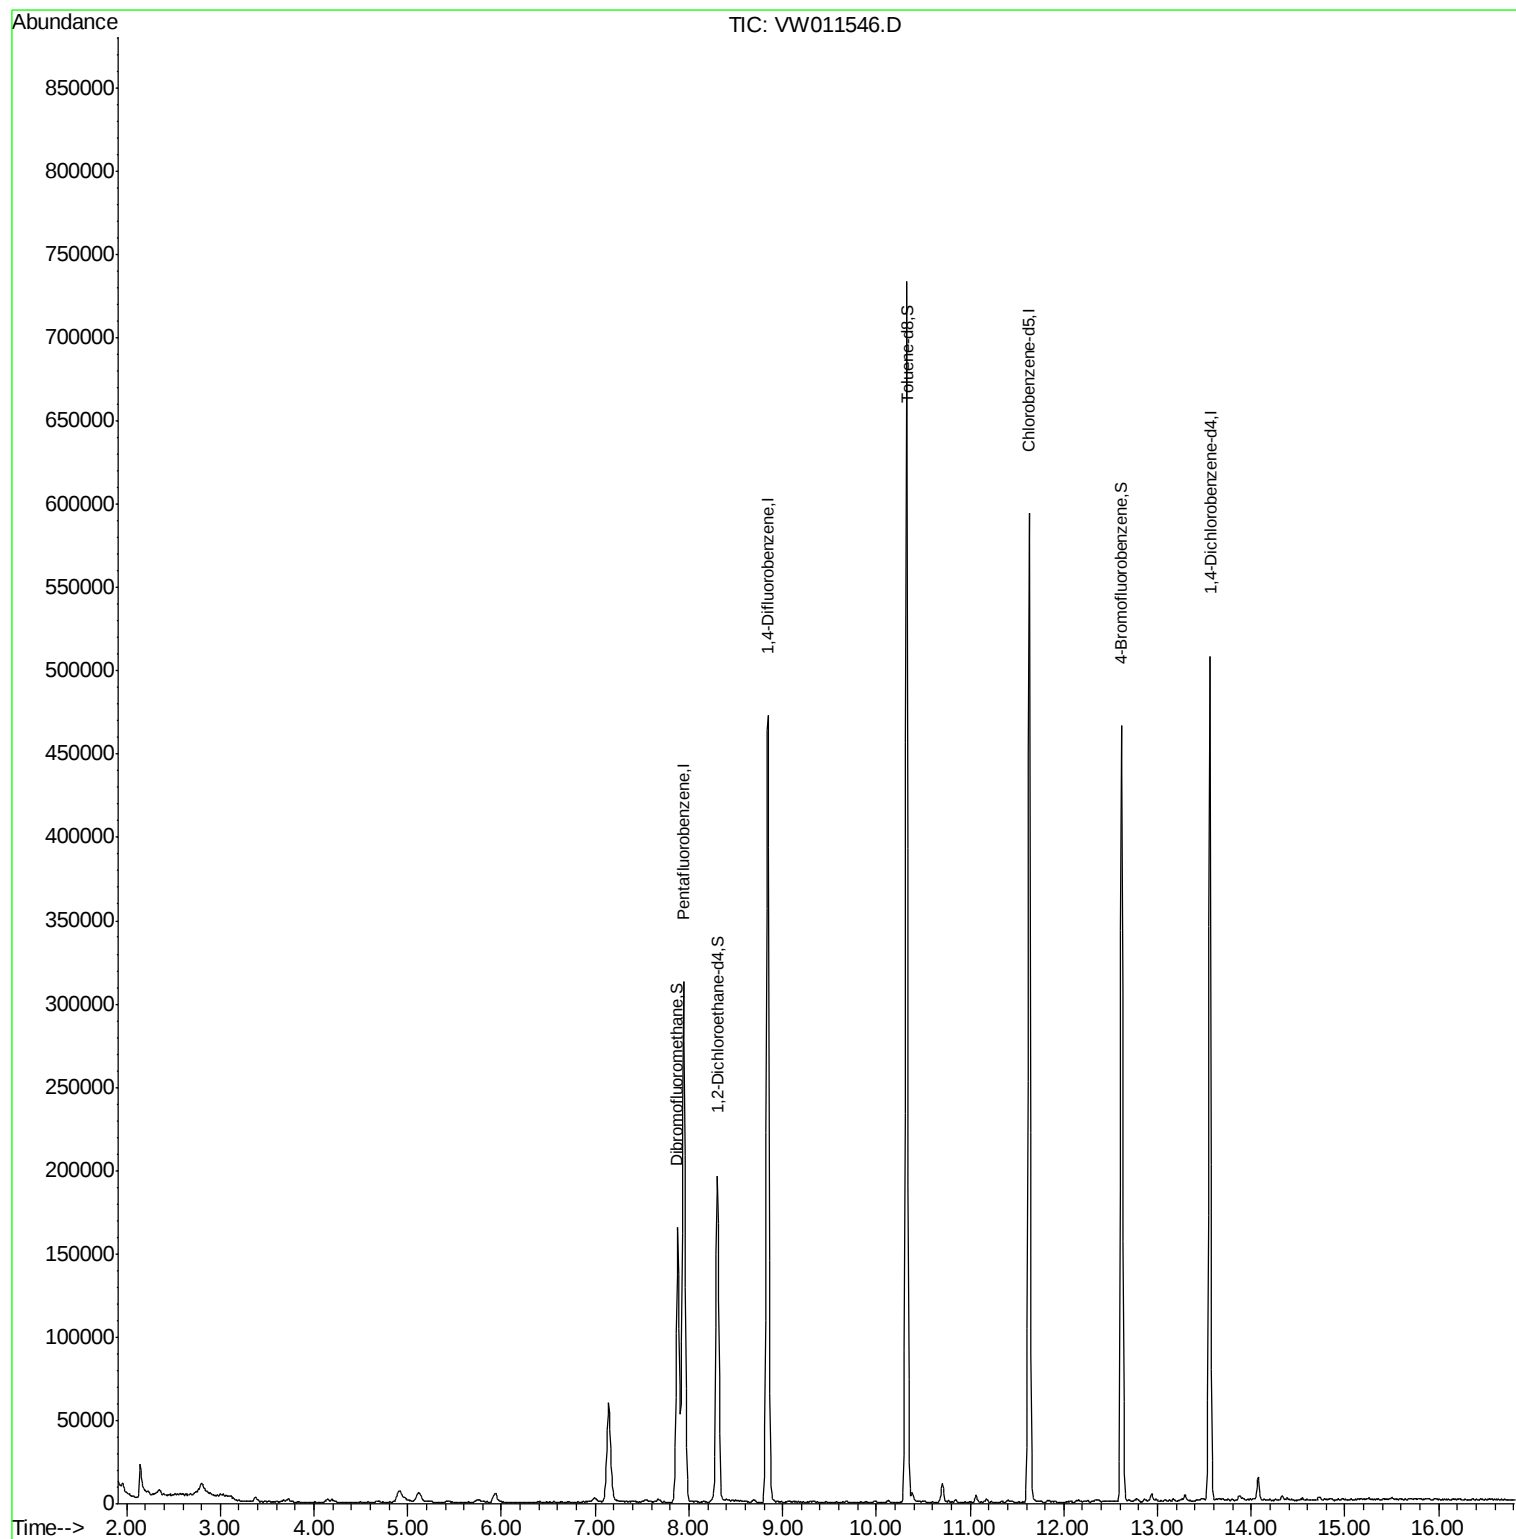

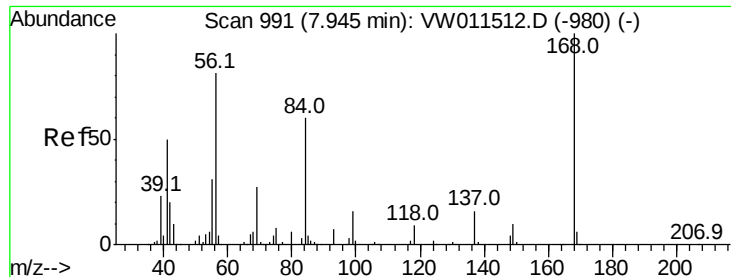

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW011546.D

Acq: 27 Jul 2019 05:11

Instrument :

MSVOA_W

ClientSampleId :


TP-10

Tot Ion:168 Resp: 227260

Ion Ratio Lower Upper

168 100

99 61.3 48.2 72.4

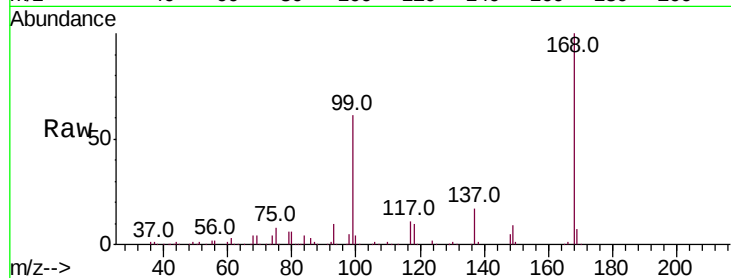

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

120000

100000

80000



60000

40000

20000

0

Time-->

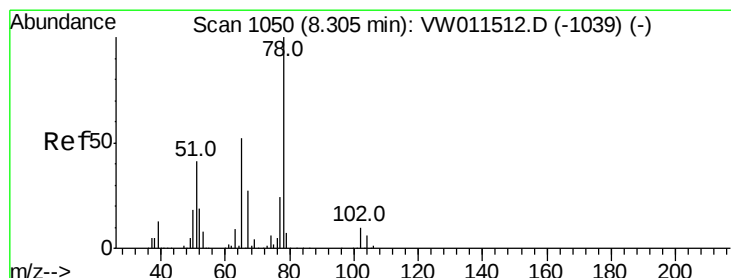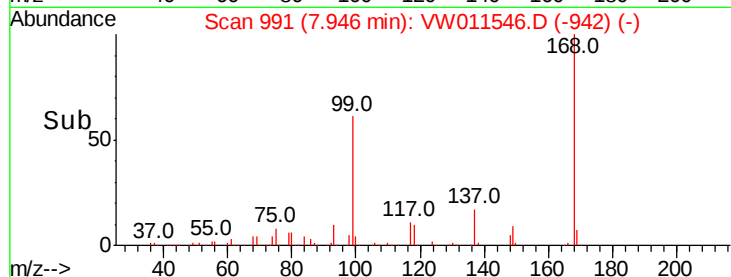

#33

1,2-Dichloroethane-d4

Concen: 59.233 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. 0.00 min

Lab File: VW011546.D


Acq: 27 Jul 2019 05:11

Tgt Ion: 65 Resp: 154572

Ion Ratio Lower Upper

65 100

67 52.1 0.0 105.2

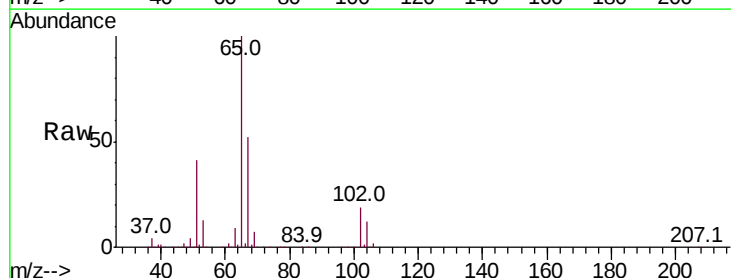

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31

80000


60000


40000

20000

0

Time-->

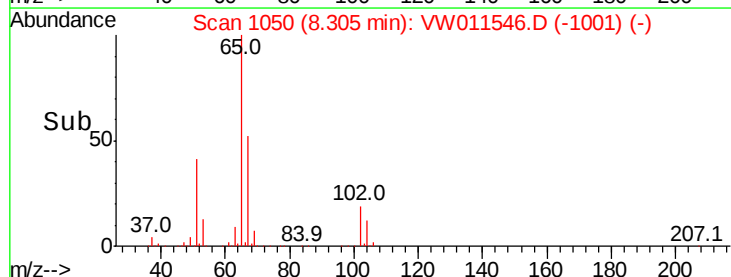


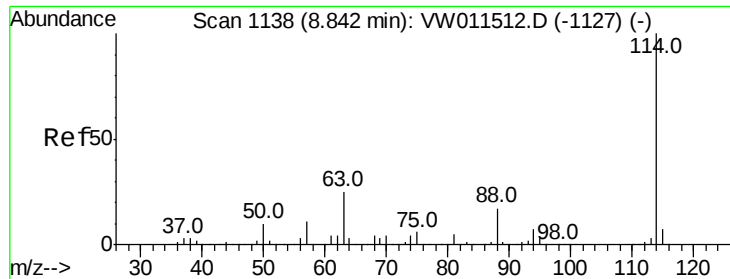




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW011546.D
 Acq: 27 Jul 2019 05:11

Instrument :
 MSVOA_W
 ClientSampleId :
 TP-10

Tot Ion:114 Resp: 378411
 Ion Ratio Lower Upper
 114 100
 63 24.0 0.0 49.2
 88 17.3 0.0 33.8

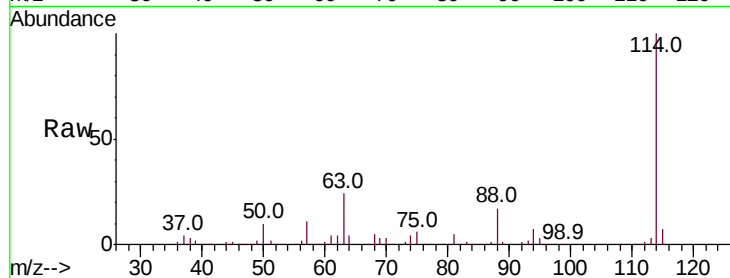


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

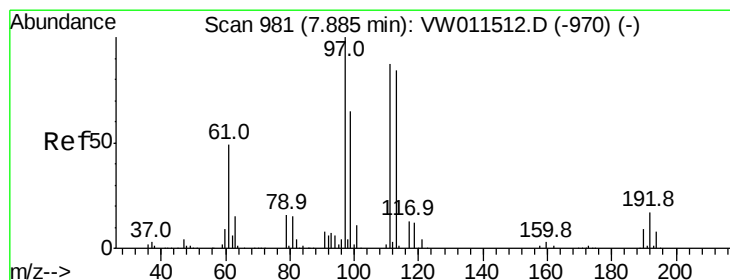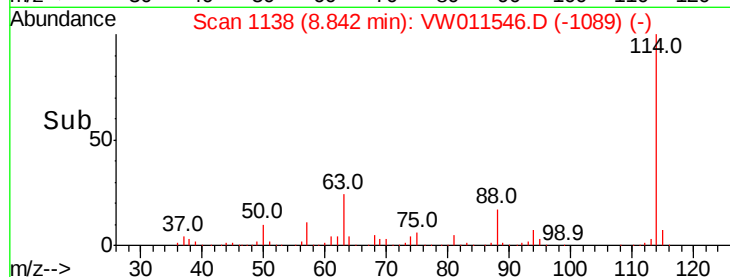
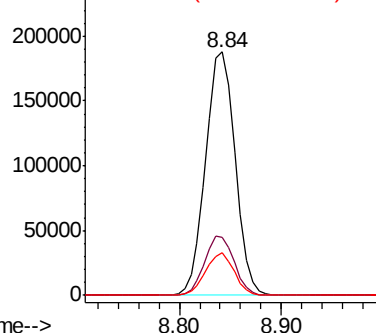



#35
 Dibromofluoromethane
 Concen: 54.671 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. 0.00 min
 Lab File: VW011546.D
 Acq: 27 Jul 2019 05:11

Tgt Ion:113 Resp: 116065
 Ion Ratio Lower Upper
 113 100
 111 102.6 82.7 124.1
 192 20.2 16.1 24.1

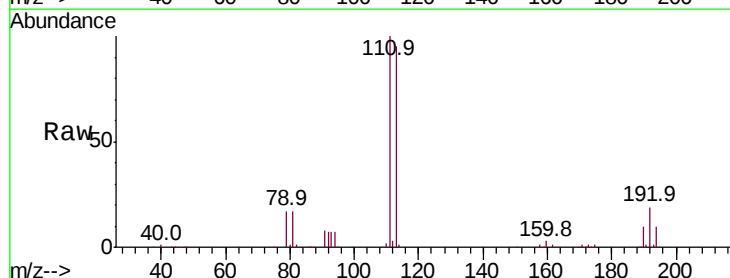

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



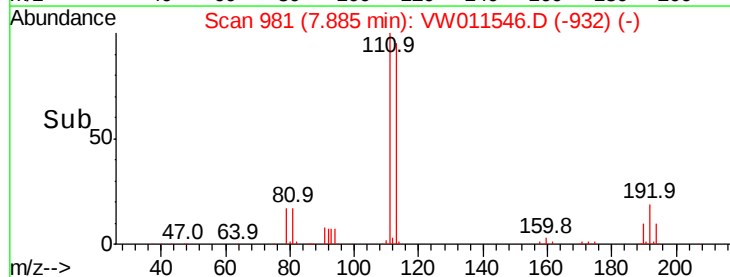
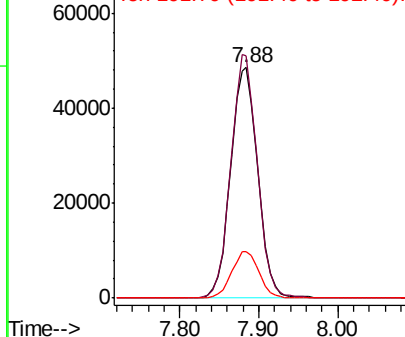


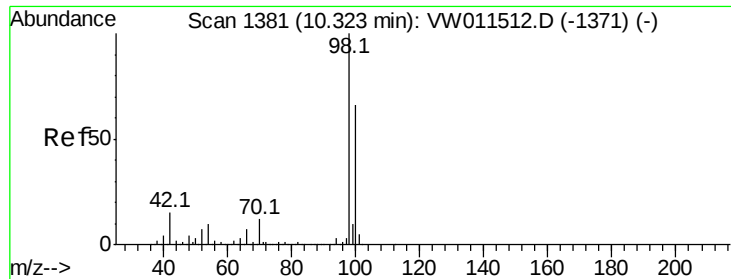

#50
Toluene-d8
Concen: 53.077 ug/l
RT: 10.32 min Scan# 1381
Delta R.T. 0.00 min
Lab File: VW011546.D
Acq: 27 Jul 2019 05:11




Instrument :
MSVOA_W
ClientSampleId :
TP-10


Tot Ion: 98 Resp: 461342
Ion Ratio Lower Upper
98 100
100 65.4 52.7 79.1

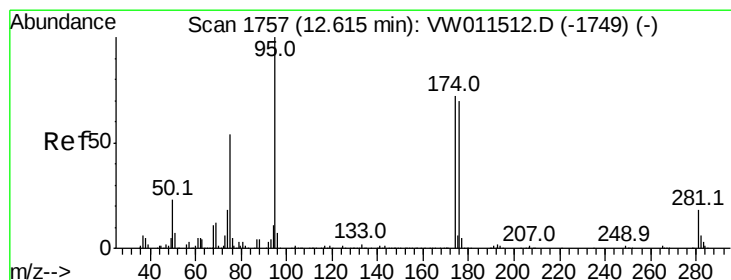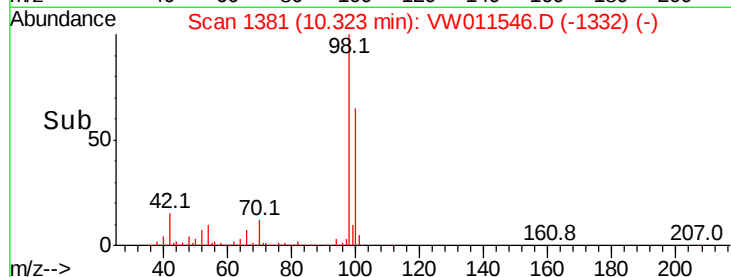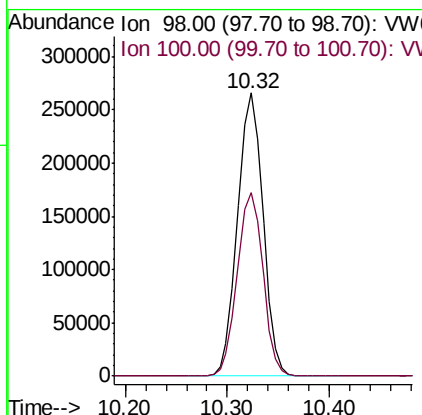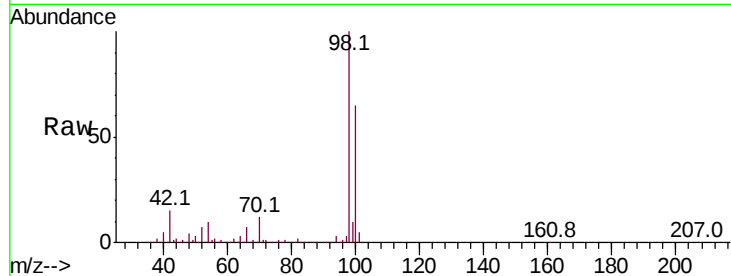

#62
4-Bromofluorobenzene
Concen: 47.901 ug/l
RT: 12.62 min Scan# 1757
Delta R.T. 0.00 min
Lab File: VW011546.D
Acq: 27 Jul 2019 05:11

Tgt Ion: 95 Resp: 148438
Ion Ratio Lower Upper
95 100
174 76.1 0.0 150.2
176 72.6 0.0 144.4

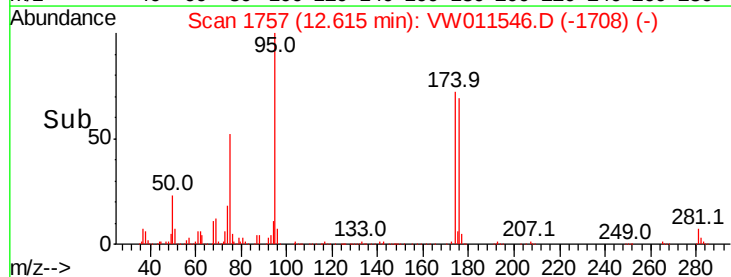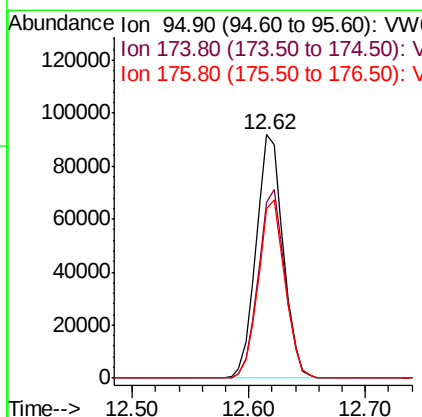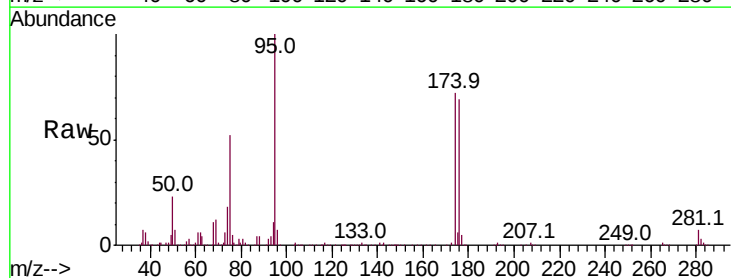


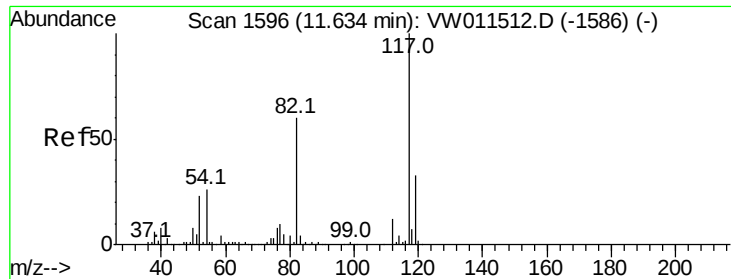




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1595
Delta R.T. -0.01 min
Lab File: VW011546.D
Acq: 27 Jul 2019 05:11

Instrument :
MSVOA_W
ClientSampleId :
TP-10

Tot Ion:117 Resp: 312990
Ion Ratio Lower Upper
117 100
82 61.0 47.9 71.9
119 31.1 26.2 39.2

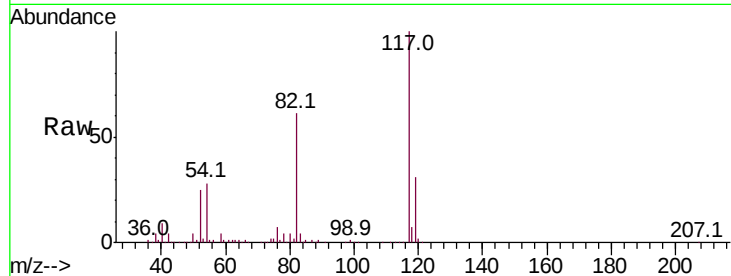


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

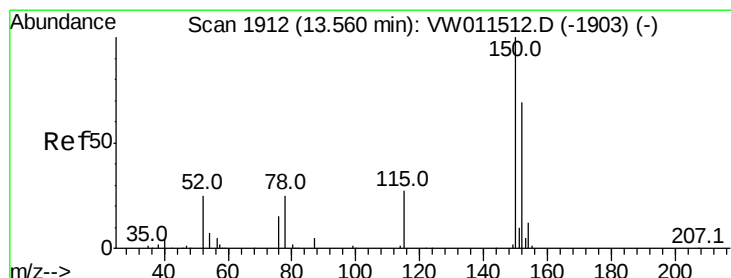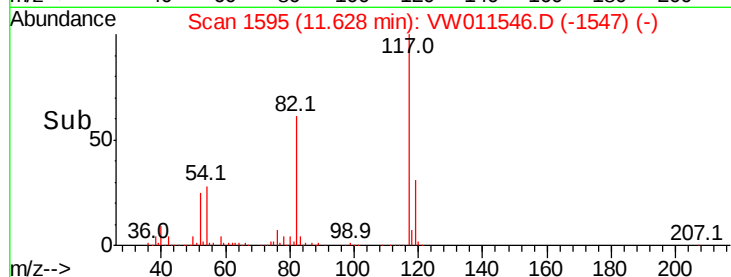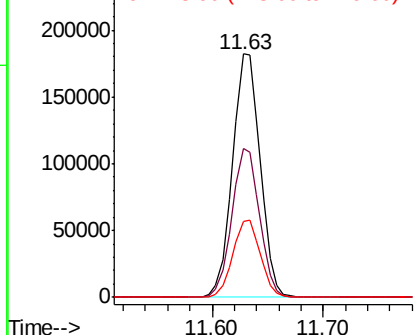

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. 0.00 min
Lab File: VW011546.D
Acq: 27 Jul 2019 05:11

Tgt Ion:152 Resp: 127460
Ion Ratio Lower Upper
152 100
115 60.1 30.5 91.5
150 155.8 0.0 352.6

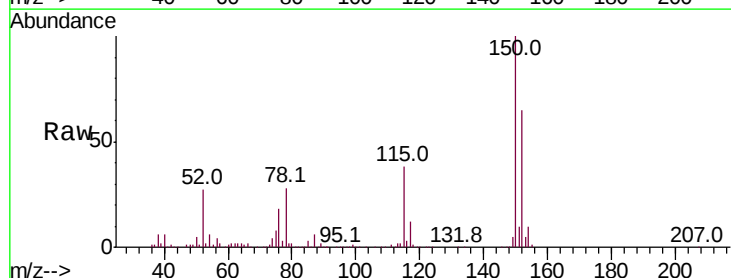

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

