
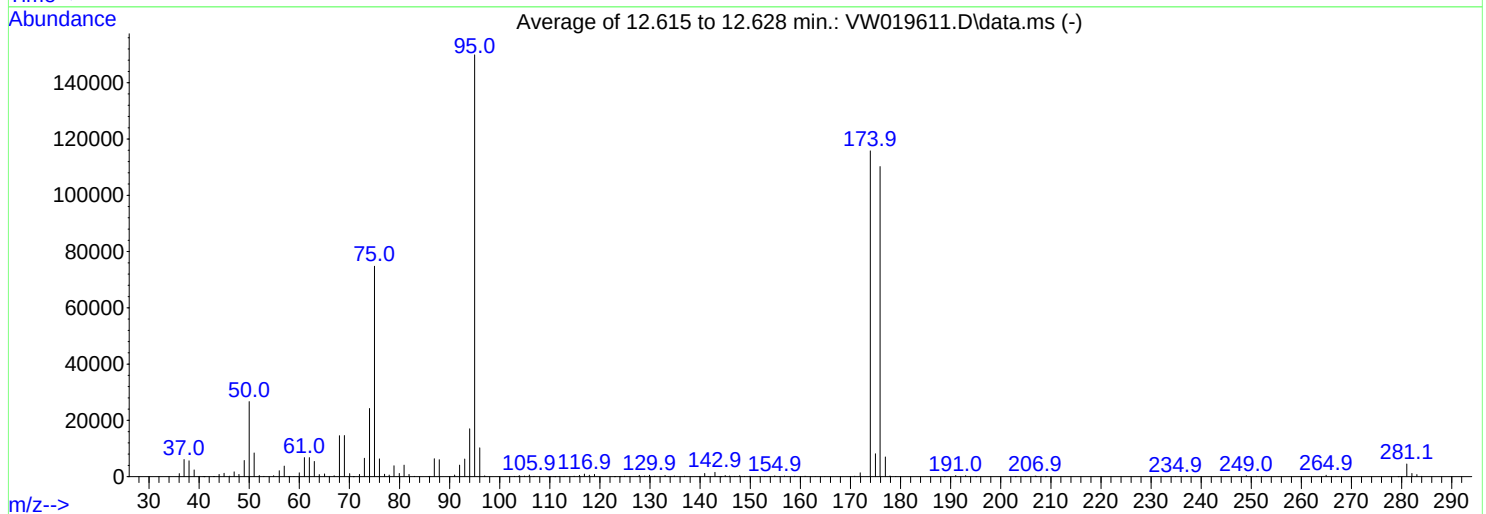


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072721\
 Data File : VW019611.D
 Acq On : 27 Jul 2021 09:39
 Operator : SY/VA
 Sample : BFB410
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB410

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Title : SFAM01.0
 Last Update : Wed Jul 28 00:48:17 2021

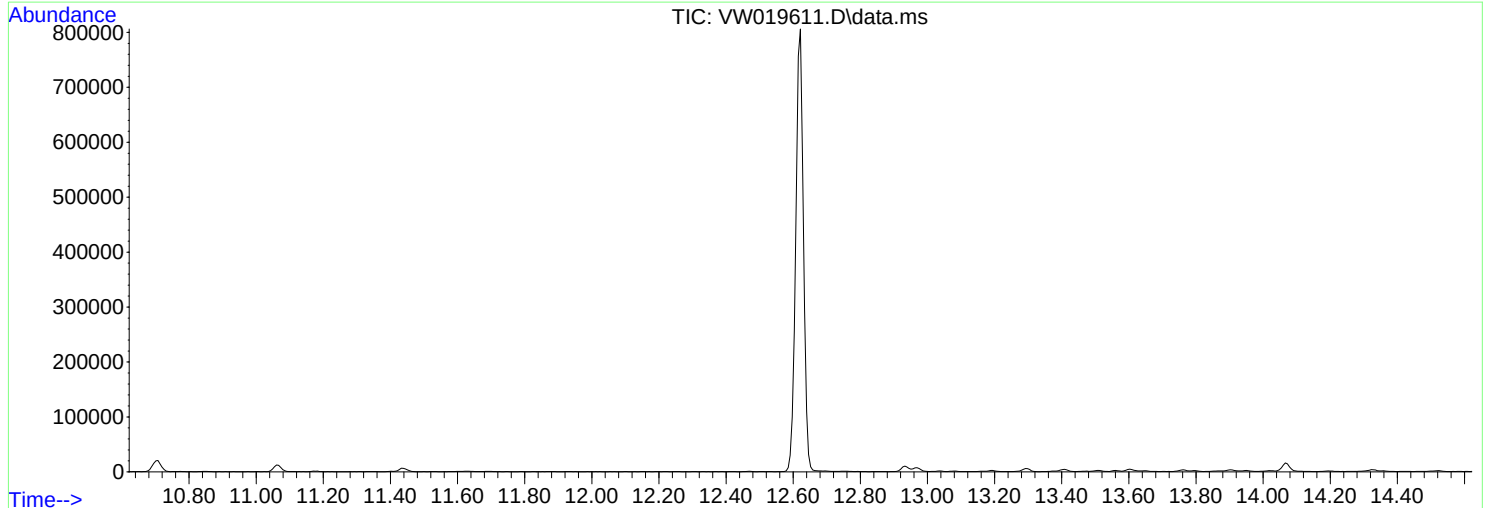

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	26683	PASS
75	95	30	80	49.9	74765	PASS
95	95	100	100	100.0	149912	PASS
96	95	5	9	6.8	10247	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.2	115760	PASS
175	174	5	9	7.0	8129	PASS
176	174	95	105	95.2	110213	PASS
177	176	5	10	6.3	6971	PASS

Scan 1749 (12.567 min): VW019611.D\data.ms
BFB410

m/z	Abundance
40.00	180.0
44.00	199.0
54.90	56.0
57.30	82.0

Instrument :
MSVOA_W
ClientSampleId :
BFB410

m/z	Abundance
36.00	1086.0
37.00	7150.0
38.00	6959.0
39.00	2742.0
40.00	306.0
40.80	66.0
42.90	108.0
44.00	935.0
45.00	1469.0
46.00	235.0
47.00	2075.0
47.90	994.0
49.00	6436.0
50.00	30048.0
51.00	9657.0
52.00	378.0
52.90	161.0
54.90	459.0
56.00	2486.0
57.00	4018.0
57.90	110.0
58.90	109.0
60.00	1494.0
61.00	7707.0
62.00	7764.0
63.00	6075.0
64.00	874.0
65.00	1217.0
66.10	164.0
67.00	415.0
68.00	16125.0
69.00	16600.0
70.10	1234.0
72.00	837.0
73.00	7226.0
74.00	26352.0
75.00	82352.0
76.00	7074.0
77.00	764.0
78.10	602.0
78.90	4207.0
79.90	1287.0
80.90	4615.0
81.90	808.0
83.00	91.0
85.90	238.0
86.90	7048.0
88.00	6373.0
91.00	625.0
92.00	4339.0
93.00	7009.0
94.00	17880.0
95.00	162880.0
96.00	11056.0
97.00	348.0
103.00	194.0
103.80	575.0
104.90	260.0
105.90	621.0
106.80	159.0
110.00	90.0
110.80	139.0
111.90	124.0
112.90	98.0
114.80	183.0
115.90	527.0
116.90	1067.0
117.90	655.0
118.90	790.0
122.90	53.0
124.90	265.0
127.80	430.0
128.90	254.0
129.90	548.0
131.00	169.0
133.00	694.0
133.70	136.0
134.20	121.0
134.80	273.0
136.90	179.0
139.90	129.0
140.90	1202.0
141.70	117.0
143.00	1690.0
143.80	123.0
145.00	563.0
145.80	198.0
146.80	109.0
147.90	314.0
148.90	154.0
150.00	147.0
151.90	56.0

Instrument :
MSVOA_W
ClientSampleId :
BFB410

153.00	99.0
153.90	83.0
154.90	383.0
156.80	238.0
158.80	224.0
160.90	240.0
163.00	102.0
164.90	61.0
170.90	209.0
172.00	1453.0
173.90	114808.0
175.00	8157.0
175.90	101984.0
176.90	7060.0
177.90	342.0
179.10	121.0
188.70	79.0
191.00	747.0
191.90	130.0
193.00	526.0
193.90	180.0
195.00	94.0
202.90	55.0
205.00	130.0
206.90	487.0
208.00	144.0
234.90	135.0
249.00	597.0
249.80	145.0
250.90	148.0
252.10	127.0
265.00	762.0
266.10	231.0
266.90	147.0
279.30	66.0
281.10	7784.0
282.00	1672.0
283.10	1248.0
284.00	193.0

Instrument :
MSVOA_W
ClientSampleId :
BFB410

m/z	Abundance
36.00	1339.0
37.00	6749.0
38.00	6096.0
39.00	2620.0
40.00	269.0
40.80	51.0
43.10	69.0
44.00	1222.0
45.00	1257.0
46.10	146.0
47.00	1759.0
48.00	889.0
49.00	6453.0
50.00	30400.0
51.00	9326.0
52.00	527.0
53.00	153.0
55.00	453.0
56.00	2442.0
57.00	4530.0
58.10	262.0
59.00	113.0
60.00	1590.0
61.00	7524.0
62.00	7515.0
63.00	6006.0
64.00	904.0
65.10	1134.0
66.00	107.0
66.90	381.0
68.00	16544.0
69.00	16089.0
70.00	1051.0
72.00	979.0
73.00	7343.0
74.00	28072.0
75.00	84776.0
76.00	7026.0
77.00	1069.0
77.90	668.0
78.90	4458.0
80.00	1217.0
80.90	4484.0
81.90	880.0
82.90	117.0
86.10	268.0
87.00	7026.0
87.90	7067.0
90.90	647.0
92.00	4768.0
93.00	6742.0
94.00	19656.0
95.00	167872.0
96.00	11593.0
97.00	342.0
102.90	128.0
104.00	594.0
104.90	224.0
105.90	574.0
106.90	137.0
109.70	57.0
110.80	92.0
111.80	104.0
112.80	134.0
114.90	218.0
115.90	431.0
116.90	1004.0
117.90	602.0
118.90	1111.0
124.00	78.0
124.90	186.0
126.00	101.0
127.90	541.0
129.00	288.0
129.90	598.0
130.90	197.0
133.00	331.0
134.00	71.0
134.90	221.0
137.00	248.0
140.00	135.0
140.90	1275.0
142.10	128.0
142.90	1679.0
143.80	123.0
145.00	419.0
145.90	256.0
146.90	107.0
147.90	350.0
148.80	76.0
149.90	239.0
151.90	69.0

Instrument :
MSVOA_W
ClientSampleId :
BFB410

152.90	116.0
153.80	68.0
154.90	295.0
155.80	88.0
156.90	274.0
158.90	146.0
161.00	189.0
162.90	137.0
164.90	62.0
170.80	256.0
171.90	1558.0
173.90	133504.0
175.00	8959.0
175.90	127640.0
176.90	7775.0
177.90	223.0
179.00	86.0
191.00	347.0
191.90	72.0
193.00	402.0
207.10	286.0
208.10	88.0
208.90	64.0
249.00	284.0
251.00	124.0
264.90	513.0
265.90	128.0
266.90	95.0
279.90	88.0
281.00	3891.0
282.10	1227.0
283.00	773.0
284.00	109.0

Instrument :
MSVOA_W
ClientSampleId :
BFB410

m/z	Abundance
36.10	830.0
37.00	4453.0
38.00	3891.0
39.00	1829.0
40.10	238.0
41.00	73.0
43.10	79.0
44.00	821.0
45.10	872.0
46.20	99.0
47.00	1294.0
48.00	559.0
49.00	4348.0
50.00	19600.0
51.00	6313.0
52.10	293.0
53.00	70.0
55.00	242.0
56.00	1467.0
57.00	2666.0
58.10	129.0
60.00	1020.0
61.00	5084.0
62.00	5004.0
63.00	4143.0
63.90	498.0
65.00	608.0
65.90	56.0
67.00	283.0
68.00	11044.0
69.00	11190.0
70.00	957.0
70.80	61.0
72.00	575.0
73.00	5095.0
74.00	18232.0
75.00	57168.0
76.00	4896.0
77.00	752.0
77.80	510.0
78.90	3013.0
79.90	952.0
80.90	3163.0
81.90	660.0
83.00	129.0
86.00	141.0
87.00	5083.0
88.00	4584.0
91.10	382.0
92.00	3197.0
93.00	5040.0
94.00	13455.0
95.00	118984.0
96.00	8091.0
97.00	253.0
103.00	107.0
103.90	401.0
105.00	188.0
105.90	520.0
106.90	121.0
111.00	85.0
111.70	84.0
112.00	75.0
112.80	91.0
114.90	99.0
115.90	422.0
116.90	701.0
117.90	288.0
118.90	572.0
124.90	93.0
126.00	65.0
127.90	392.0
128.90	210.0
129.90	436.0
130.90	144.0
132.90	158.0
134.90	256.0
136.80	145.0
140.00	81.0
140.90	1013.0
142.10	111.0
142.90	1307.0
144.10	51.0
145.00	244.0
145.80	170.0
147.00	157.0
147.90	302.0
148.90	88.0
149.90	145.0
152.80	57.0
154.00	86.0
154.90	231.0

Instrument :
MSVOA_W
ClientSampleId :
BFB410

155.90	62.0
156.80	173.0
159.00	129.0
161.00	144.0
172.00	1063.0
174.00	98968.0
175.00	7270.0
175.90	101016.0
177.00	6078.0
177.90	128.0
191.00	189.0
192.00	59.0
192.90	164.0
206.90	174.0
208.20	57.0
249.10	104.0
251.10	102.0
264.90	204.0
266.10	58.0
266.90	61.0
281.00	1851.0
282.00	518.0
283.20	289.0
284.00	62.0

Instrument :
MSVOA_W
ClientSampleId :
BFB410