


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW072818\
 Data File : VW004242.D
 Acq On : 26 Jul 2018 23:19
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W071618S.M
 Title : SW846 8260
 Last Update : Mon Jul 16 15:06:12 2018

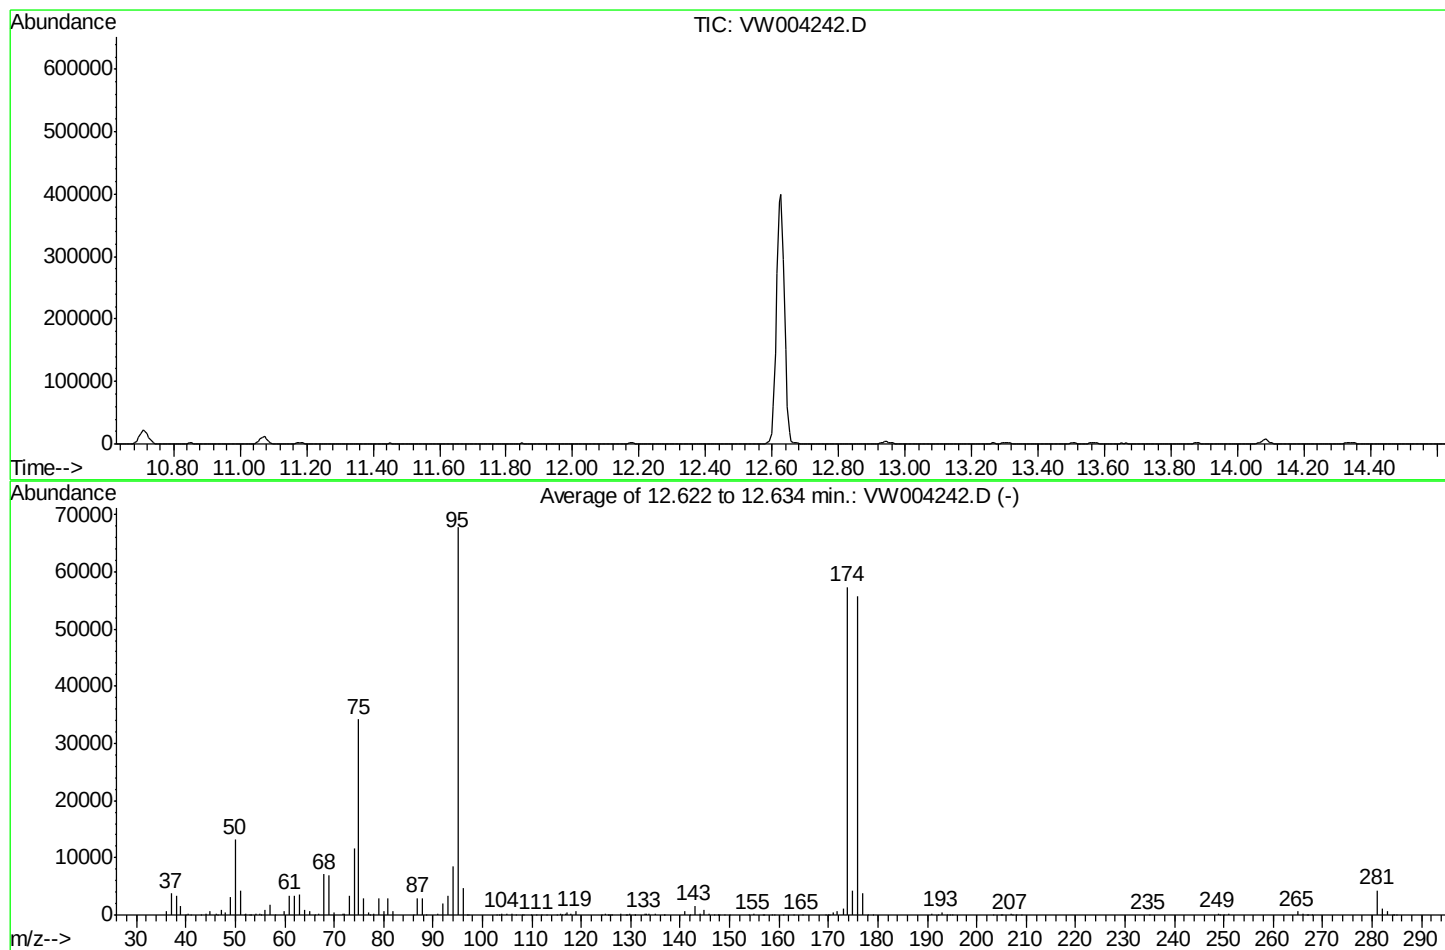

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	13183	PASS
75	95	30	60	50.5	34202	PASS
95	95	100	100	100.0	67768	PASS
96	95	5	9	6.8	4624	PASS
173	174	0.00	2	1.8	1057	PASS
174	95	50	100	84.7	57378	PASS
175	174	5	9	7.4	4257	PASS
176	174	95	101	97.3	55818	PASS
177	176	5	9	6.7	3764	PASS