

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072821\
 Data File : VW019639.D
 Acq On : 28 Jul 2021 14:09
 Operator : SY/VA
 Sample : M3181-07
 Misc : 5.01g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual Integrations
 APPROVED

MMDadoda
 7/30/2021 12:53:54 PM

Quant Time: Jul 29 01:14:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 29 01:12:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	388290	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	371587	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	177725	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	103758	18.860	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.440%		
7) Chloroethane-d5	2.898	69	81096m	20.671	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.680%		
11) 1,1-Dichloroethene-d2	4.025	63	150515	14.179	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.720%		
21) 2-Butanone-d5	7.086	46	73933	46.301	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.600%		
24) Chloroform-d	7.653	84	225364	21.005	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.040%		
26) 1,2-Dichloroethane-d4	8.311	65	126628	21.507	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	86.040%		
32) Benzene-d6	8.275	84	440345	19.908	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	79.640%		
36) 1,2-Dichloropropane-d6	9.274	67	140487	20.378	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	81.520%		
41) Toluene-d8	10.323	98	387131	19.412	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	77.640%		
43) trans-1,3-Dichloroprop...	10.579	79	58184	19.707	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	78.840%		
47) 2-Hexanone-d5	10.927	63	56927	44.508	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	89.020%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	127934	22.966	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	91.880%		
66) 1,2-Dichlorobenzene-d4	13.853	152	146512	23.365	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	93.440%		
Target Compounds						Qvalue
16) Methylene chloride	4.928	84	24297	3.139	ug/L	93
42) Toluene	10.390	91	7328	0.302	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072821\
Data File : VW019639.D
Acq On : 28 Jul 2021 14:09
Operator : SY/VA
Sample : M3181-07
Misc : 5.01g/10.0mL/MSVOA_W/SOIL
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual Integrations
APPROVED

MMDadoda
7/30/2021 12:53:54 PM


Quant Time: Jul 29 01:14:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 29 01:12:37 2021
Response via : Initial Calibration

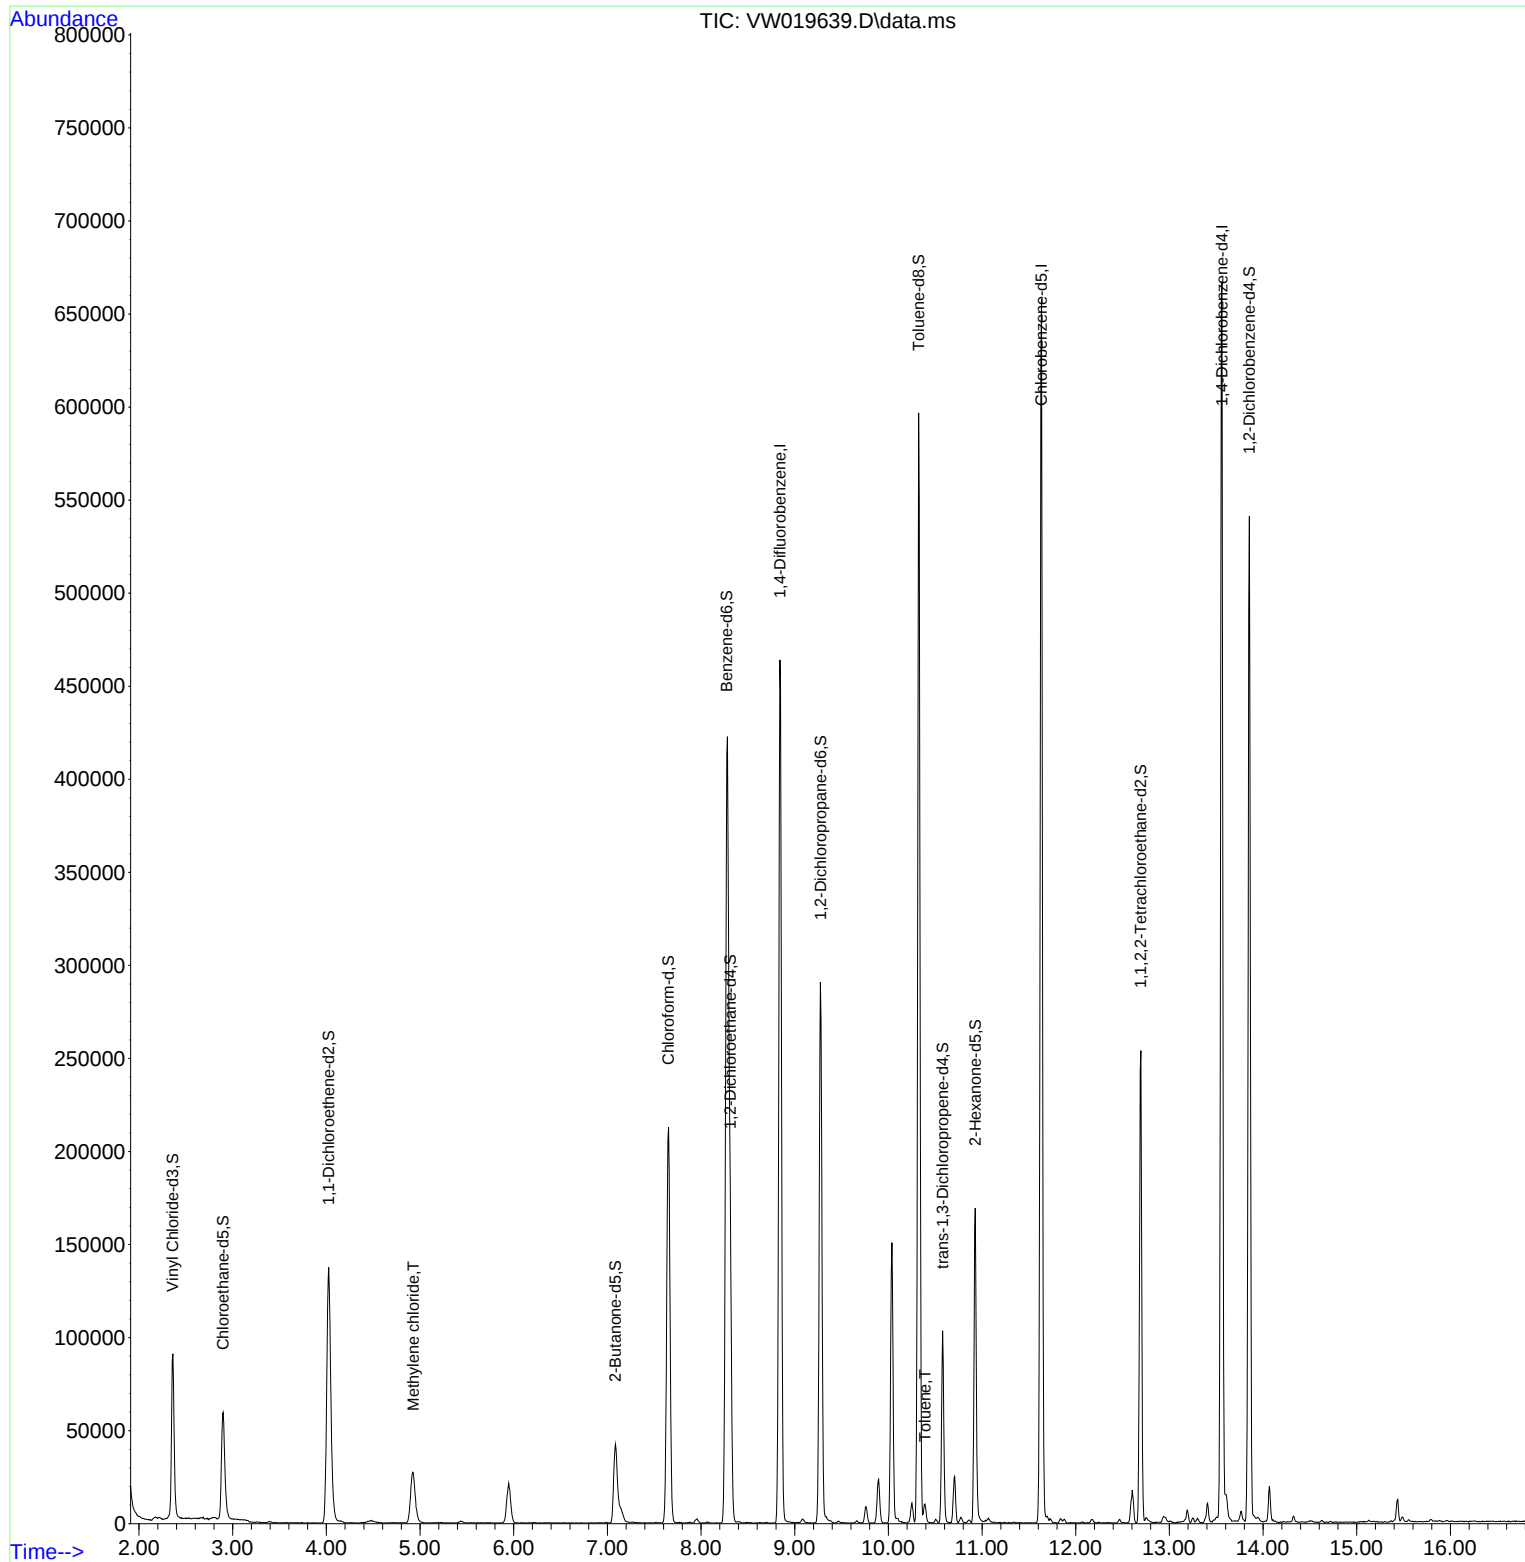

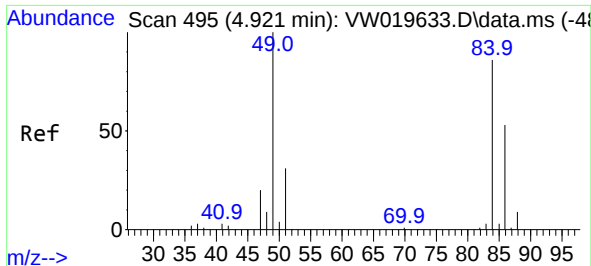

#16
Methylene chloride
Concen: 3.139 ug/L
RT: 4.928 min Scan# 496
Delta R.T. 0.006 min
Lab File: VW019639.D
Acq: 28 Jul 2021 14:09



Instrument :
MSVOA_W
ClientSampled :
VHBLK001

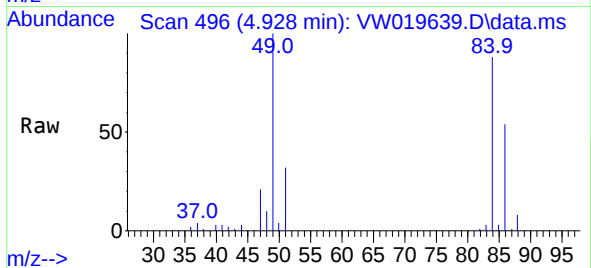


Tgt Ion: 84 Resp: 24297
Ion Ratio Lower Upper
84 100
86 61.0 45.3 84.1
49 113.6 86.6 160.8

Manual Integrations
APPROVED

MMDadoda
7/30/2021 12:53:54 PM

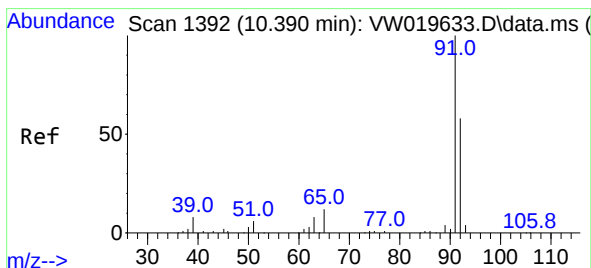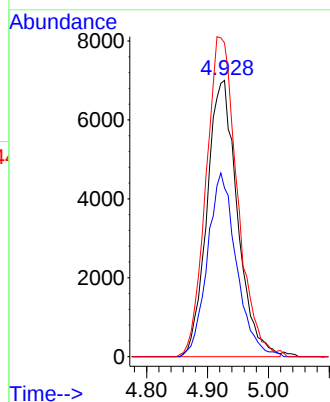

#42
Toluene
Concen: 0.302 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. 0.000 min
Lab File: VW019639.D
Acq: 28 Jul 2021 14:09

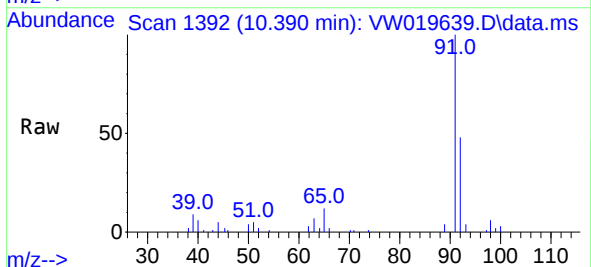

Tgt Ion: 91 Resp: 7328
Ion Ratio Lower Upper
91 100
92 48.3 39.5 73.3

