
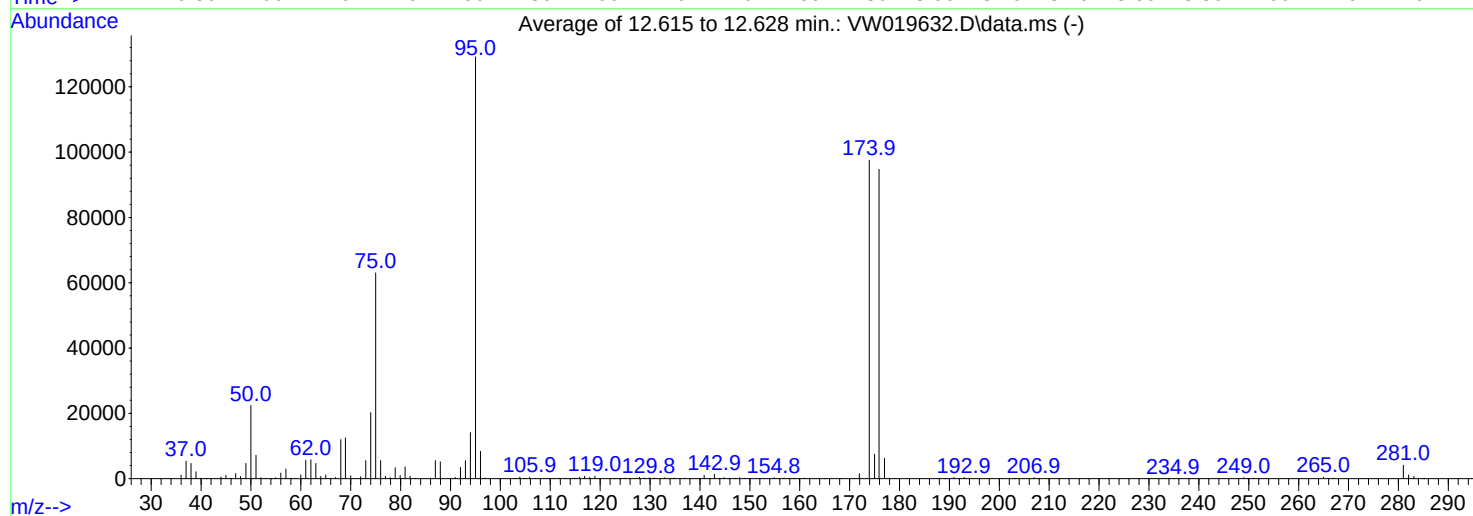


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072821\
 Data File : VW019632.D
 Acq On : 28 Jul 2021 08:49
 Operator : SY/VA
 Sample : BFB411
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB411

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Title : SFAM01.0
 Last Update : Thu Jul 29 01:12:37 2021

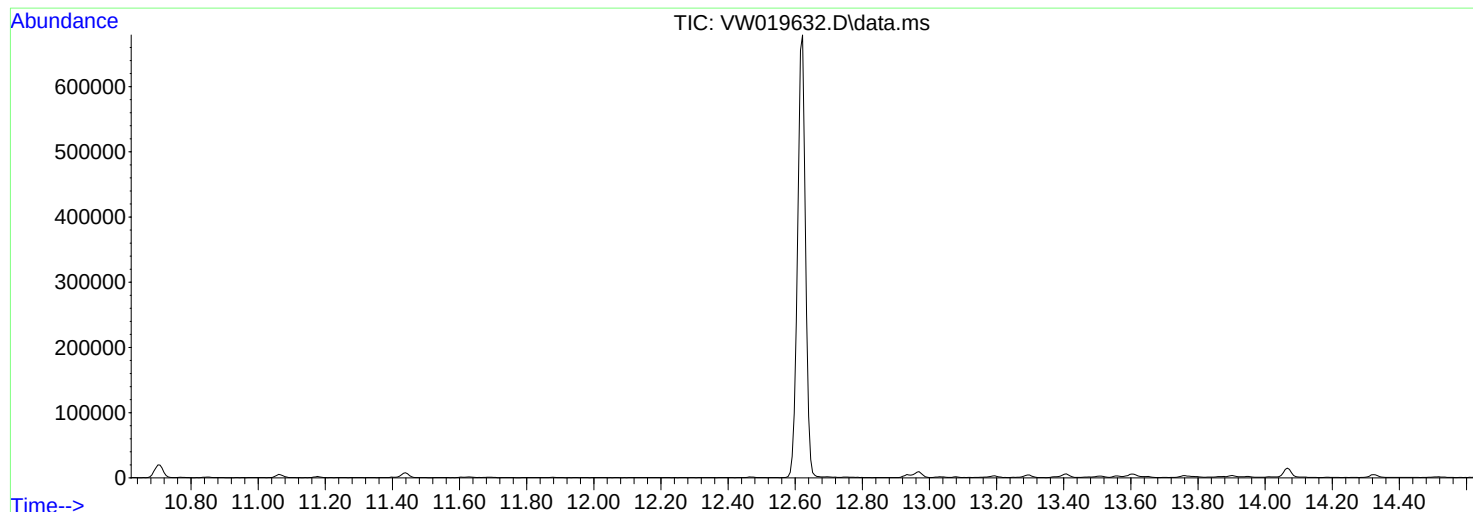

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	22401	PASS
75	95	30	80	48.8	63032	PASS
95	95	100	100	100.0	129192	PASS
96	95	5	9	6.5	8398	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.5	97525	PASS
175	174	5	9	7.6	7445	PASS
176	174	95	105	97.1	94725	PASS
177	176	5	10	6.6	6208	PASS

m/z	Abundance
36.00	1236.0
37.00	5987.0
38.00	5225.0
39.00	2401.0
40.00	275.0
42.90	101.0
44.00	776.0
45.00	1256.0
46.00	131.0
46.90	1663.0
47.90	764.0
49.00	5345.0
50.00	25120.0
51.00	8157.0
52.00	383.0
53.10	137.0
55.00	408.0
56.00	1837.0
57.00	3659.0
58.00	122.0
58.90	85.0
60.00	1316.0
61.00	6577.0
62.00	6682.0
63.00	5028.0
64.00	691.0
65.00	1299.0
65.90	111.0
67.00	308.0
68.00	13301.0
69.00	14314.0
70.00	985.0
72.00	721.0
73.00	6157.0
74.00	22720.0
75.00	69848.0
76.00	6181.0
77.00	794.0
78.90	3705.0
79.90	1070.0
80.90	3877.0
81.90	862.0
83.00	88.0
86.00	258.0
87.00	6254.0
88.00	5811.0
91.00	394.0
92.00	3805.0
93.00	6225.0
94.00	15616.0
95.00	146240.0
96.00	9694.0
97.00	221.0
102.90	76.0
103.90	531.0
104.70	117.0
105.80	540.0
107.00	81.0
109.70	74.0
110.80	65.0
111.80	121.0
113.00	119.0
114.80	174.0
115.80	440.0
116.90	930.0
117.90	445.0
119.00	914.0
124.00	81.0
125.00	209.0
125.80	80.0
127.90	447.0
128.90	241.0
130.00	484.0
130.90	254.0
133.00	224.0
134.80	186.0
136.90	170.0
140.80	1076.0
141.90	117.0
142.90	1357.0
143.80	90.0
144.90	264.0
145.70	210.0
147.10	119.0
147.90	296.0
148.90	79.0
149.90	95.0
152.00	64.0
152.80	90.0
153.80	75.0
154.90	333.0
155.80	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB411

156.90	281.0
158.90	194.0
160.90	151.0
163.00	61.0
170.90	194.0
172.00	1579.0
173.90	112096.0
175.00	7856.0
175.90	103800.0
177.00	6713.0
177.90	190.0
179.00	66.0
191.00	292.0
191.90	108.0
192.90	321.0
204.90	63.0
207.00	261.0
208.00	101.0
234.90	54.0
249.00	215.0
249.70	88.0
251.00	132.0
265.00	518.0
266.00	77.0
266.90	113.0
281.00	4229.0
282.00	1099.0
283.10	630.0
284.00	189.0

Instrument :
MSVOA_W
ClientSampleId :
BFB411

m/z	Abundance
36.00	662.0
37.00	3798.0
38.00	3530.0
39.00	1527.0
39.90	285.0
44.00	650.0
45.00	737.0
46.10	94.0
47.00	1203.0
48.00	500.0
49.00	3507.0
50.00	15955.0
51.00	5323.0
52.00	175.0
53.10	69.0
54.90	235.0
56.00	1290.0
57.00	2328.0
58.10	97.0
60.00	735.0
61.00	3961.0
62.00	4144.0
63.00	3564.0
64.00	578.0
65.00	872.0
65.80	57.0
67.00	322.0
68.00	9674.0
69.00	9839.0
70.00	685.0
71.90	456.0
73.00	4551.0
74.00	15328.0
75.00	48376.0
76.00	4139.0
77.00	583.0
77.90	369.0
78.90	2424.0
79.80	737.0
80.90	2840.0
81.90	612.0
82.90	103.0
85.90	122.0
86.90	4384.0
87.90	3864.0
90.90	306.0
92.00	2778.0
93.00	4353.0
94.00	11300.0
95.00	102520.0
96.00	6481.0
96.90	186.0
104.00	368.0
105.10	157.0
105.90	356.0
111.90	104.0
112.90	61.0
114.80	102.0
115.90	344.0
116.90	562.0
117.90	371.0
119.00	639.0
128.00	296.0
128.80	113.0
129.80	305.0
130.80	108.0
132.80	116.0
134.00	62.0
134.70	134.0
136.90	119.0
140.00	65.0
140.90	856.0
141.90	117.0
142.90	1094.0
143.80	87.0
144.90	212.0
145.90	237.0
147.00	129.0
148.00	246.0
148.90	142.0
149.90	60.0
152.90	123.0
153.80	64.0
154.80	242.0
155.80	56.0
156.80	156.0
159.00	80.0
160.90	108.0
170.70	53.0
172.00	1244.0
174.00	84200.0
175.00	6627.0

Instrument :
MSVOA_W
ClientSampleId :
BFB411

175.90	84416.0
177.00	5203.0
177.80	137.0
191.00	159.0
192.90	186.0
207.00	169.0
248.90	142.0
251.00	87.0
265.00	180.0
266.90	76.0
281.10	1582.0
282.10	500.0
283.00	228.0

Instrument :
MSVOA_W
ClientSampleId :
BFB411

Scan 1749 (12.567 min): VW019632.D\data.ms
BFB411

m/z	Abundance
40.00	170.0
44.10	241.0
57.00	116.0
68.90	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB411

m/z	Abundance
36.00	1192.0
37.00	6218.0
38.00	5249.0
39.00	2454.0
40.00	335.0
41.00	69.0
43.10	112.0
44.00	758.0
45.00	1163.0
46.00	228.0
47.00	1806.0
47.90	845.0
49.00	5209.0
50.00	26128.0
51.00	7927.0
52.00	332.0
53.00	88.0
54.00	74.0
55.00	292.0
56.00	2102.0
57.00	3247.0
58.00	161.0
58.90	88.0
60.00	1365.0
61.00	6585.0
62.00	6520.0
63.00	5392.0
64.00	728.0
65.00	1166.0
65.90	158.0
66.90	392.0
68.00	12871.0
69.00	13383.0
70.00	930.0
72.00	654.0
73.00	5941.0
74.00	22648.0
75.00	70872.0
76.00	6359.0
76.90	832.0
77.90	665.0
78.90	3912.0
80.00	1112.0
80.90	3971.0
81.90	899.0
82.90	84.0
86.00	247.0
87.00	5972.0
87.90	5773.0
90.90	512.0
92.00	3770.0
93.00	5838.0
94.00	15423.0
95.00	138816.0
96.00	9019.0
97.00	209.0
103.00	146.0
103.80	524.0
104.90	260.0
106.00	441.0
107.00	97.0
109.90	138.0
110.90	79.0
112.00	163.0
113.00	167.0
114.90	171.0
115.90	368.0
116.90	794.0
117.90	493.0
118.90	830.0
122.80	66.0
123.80	86.0
125.00	274.0
125.90	146.0
127.90	502.0
128.90	238.0
129.80	446.0
130.80	175.0
133.00	575.0
133.90	101.0
134.90	224.0
137.00	204.0
139.90	122.0
140.90	976.0
141.90	126.0
142.90	1526.0
144.00	107.0
144.80	485.0
146.00	193.0
146.90	148.0
147.90	292.0
148.90	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB411

149.90	99.0
152.00	54.0
152.90	60.0
153.90	57.0
154.90	296.0
155.80	52.0
156.80	178.0
158.70	100.0
161.00	151.0
163.00	96.0
165.00	88.0
170.90	175.0
171.90	1703.0
173.90	96280.0
175.00	7852.0
175.90	95960.0
177.00	6708.0
178.00	186.0
178.90	136.0
189.10	85.0
190.90	551.0
191.80	100.0
193.00	629.0
193.90	122.0
203.00	85.0
204.90	142.0
206.90	400.0
208.10	102.0
234.90	81.0
249.00	509.0
249.80	93.0
250.90	278.0
252.00	56.0
265.00	664.0
266.00	142.0
267.10	219.0
281.00	6587.0
282.10	1736.0
283.10	1311.0
284.10	233.0
285.10	94.0

Instrument :
MSVOA_W
ClientSampleId :
BFB411