
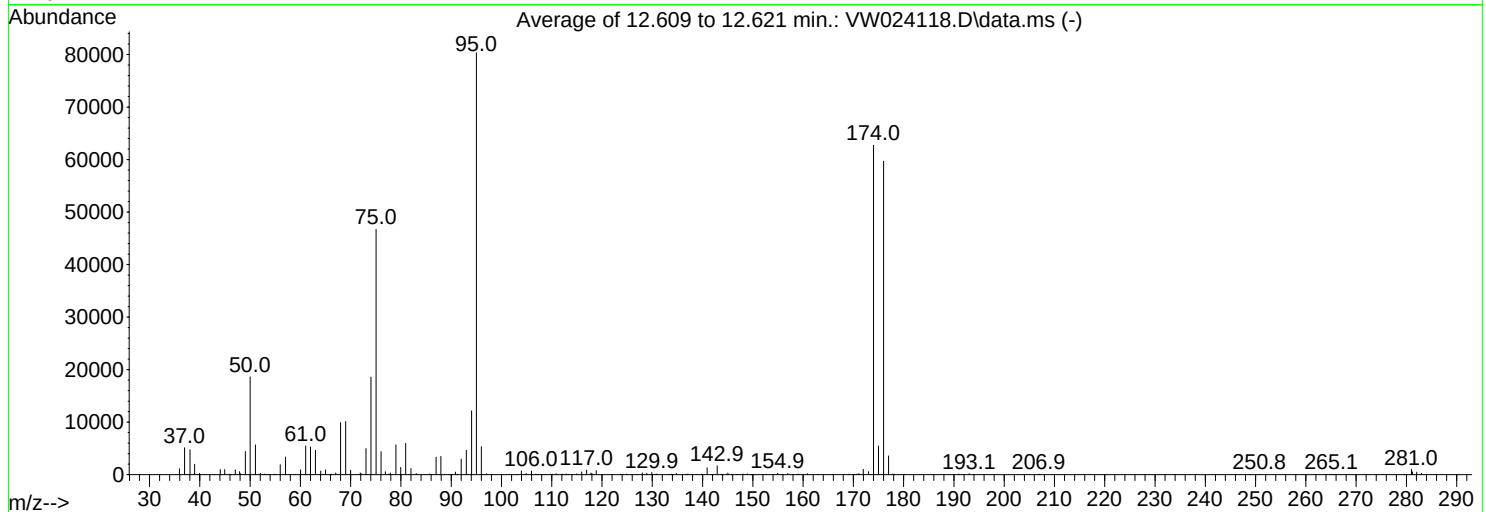


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072822\
Data File : VW024118.D
Acq On : 28 Jul 2022 07:52
Operator : SY/VA
Sample : BFB595
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB595

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Title : SFAM01.0
Last Update : Fri Jul 29 01:16:23 2022

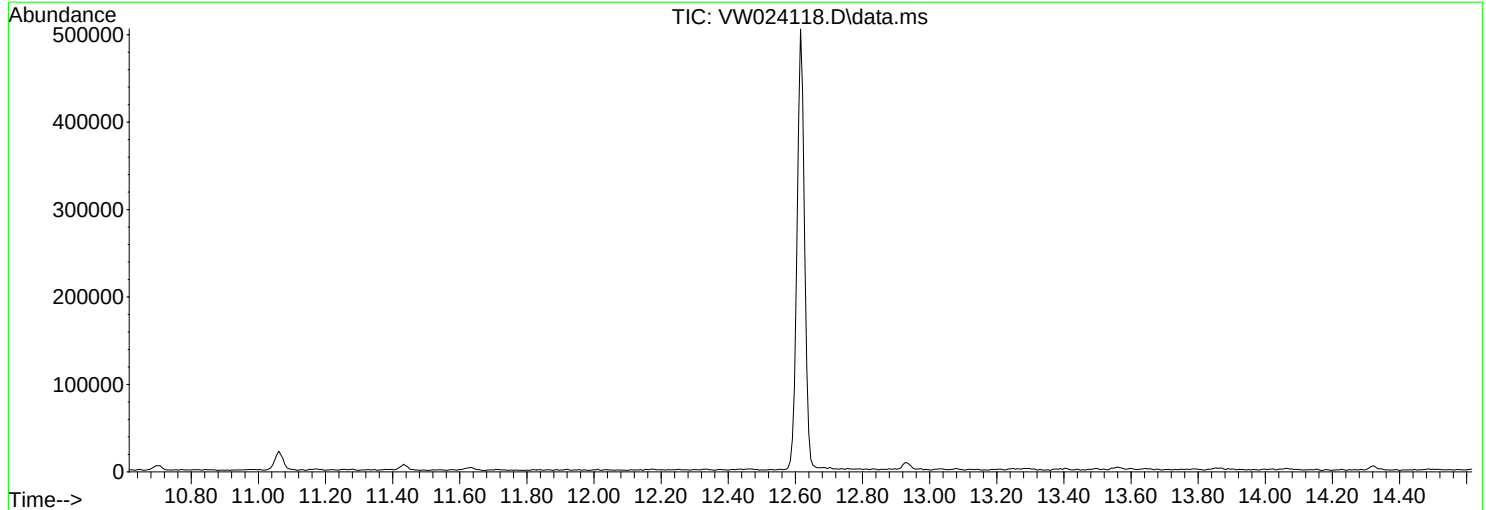

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.2	18608	PASS
75	95	30	80	58.2	46715	PASS
95	95	100	100	100.0	80320	PASS
96	95	5	9	6.6	5335	PASS
173	174	0.00	2	0.9	577	PASS
174	95	50	120	78.1	62749	PASS
175	174	5	9	8.7	5458	PASS
176	174	95	105	95.1	59699	PASS
177	176	5	10	6.0	3581	PASS

m/z	Abundance
35.20	73.0
35.80	146.0
36.90	73.0
38.00	150.0
38.90	59.0
39.70	217.0
40.30	135.0
41.80	84.0
42.90	117.0
44.10	97.0
44.90	109.0
49.10	71.0
49.40	60.0
50.50	100.0
55.00	148.0
56.10	53.0
57.20	80.0
57.90	119.0
58.70	65.0
59.80	67.0
60.60	89.0
61.60	64.0
71.60	79.0
122.10	51.0
194.30	74.0
295.50	73.0
296.50	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

m/z	Abundance
36.00	1052.0
37.00	5505.0
38.10	4935.0
39.00	1974.0
40.10	305.0
41.00	71.0
41.90	50.0
43.00	231.0
44.00	1055.0
45.00	948.0
45.90	94.0
46.30	102.0
47.00	823.0
47.90	975.0
49.00	4717.0
50.00	18512.0
51.10	5446.0
52.10	191.0
52.90	211.0
53.70	89.0
55.10	385.0
56.00	1763.0
57.10	3407.0
58.10	168.0
60.00	968.0
61.10	4784.0
62.00	5076.0
63.00	4344.0
64.00	806.0
65.00	1033.0
66.10	153.0
67.10	291.0
68.00	8718.0
69.00	8956.0
70.00	1021.0
71.90	480.0
73.10	4793.0
74.00	17840.0
75.00	42288.0
76.10	3810.0
77.00	608.0
78.00	440.0
79.00	5216.0
79.90	1291.0
80.90	5407.0
82.00	1215.0
83.10	204.0
84.80	61.0
85.70	220.0
87.00	3377.0
88.00	3060.0
88.70	273.0
90.80	403.0
91.20	288.0
92.00	2452.0
93.00	4360.0
94.10	9833.0
95.00	72048.0
96.00	5503.0
97.10	197.0
103.10	69.0
103.90	621.0
104.90	210.0
105.90	563.0
106.90	149.0
110.00	199.0
110.90	190.0
112.10	110.0
112.70	71.0
113.30	86.0
115.10	175.0
116.00	413.0
116.90	1078.0
117.80	310.0
118.90	893.0
122.00	84.0
124.90	169.0
126.90	190.0
128.00	278.0
128.90	94.0
129.90	492.0
130.70	188.0
133.10	91.0
133.40	98.0
133.90	65.0
134.70	214.0
136.80	122.0
138.70	86.0
139.80	57.0
140.80	863.0
142.20	193.0
142.90	1528.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

145.10	467.0
145.80	93.0
146.70	105.0
147.50	174.0
147.90	188.0
148.90	155.0
149.60	58.0
152.70	72.0
154.90	248.0
155.80	73.0
156.90	207.0
158.80	94.0
160.90	212.0
163.00	60.0
169.00	92.0
170.70	275.0
171.20	352.0
172.00	1159.0
174.00	50728.0
175.00	4746.0
176.00	48672.0
177.00	2580.0
177.90	221.0
180.10	89.0
185.80	50.0
190.90	193.0
193.00	327.0
194.00	72.0
206.90	124.0
248.90	160.0
250.80	233.0
252.10	126.0
265.10	207.0
266.90	111.0
275.30	81.0
281.00	2474.0
282.10	487.0
283.10	301.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

m/z	Abundance
36.00	1446.0
37.00	5365.0
38.10	4971.0
39.00	2348.0
39.90	209.0
43.00	137.0
44.10	1181.0
45.10	1328.0
45.90	142.0
47.10	1249.0
47.90	807.0
49.10	4928.0
50.00	19872.0
51.10	6478.0
52.00	297.0
52.90	190.0
55.00	287.0
56.00	2101.0
57.00	3826.0
58.10	189.0
59.00	86.0
60.00	932.0
61.00	6566.0
62.00	6258.0
63.00	5172.0
64.10	644.0
65.00	1116.0
66.10	109.0
67.00	267.0
68.00	11925.0
69.00	10769.0
70.00	743.0
70.90	101.0
72.10	532.0
73.00	5506.0
74.00	20752.0
75.00	54704.0
76.00	4914.0
76.90	610.0
77.60	334.0
79.00	6473.0
80.00	1638.0
80.90	7313.0
82.00	1255.0
82.90	239.0
87.00	3683.0
87.90	3603.0
89.70	88.0
90.80	525.0
92.00	3444.0
93.00	4542.0
94.10	14444.0
95.00	91976.0
96.00	5612.0
97.00	226.0
103.00	166.0
103.90	813.0
104.80	215.0
105.90	573.0
106.80	191.0
108.40	76.0
109.70	173.0
110.10	114.0
110.90	211.0
111.90	124.0
112.90	203.0
114.90	117.0
115.90	557.0
117.00	852.0
118.00	705.0
118.90	694.0
121.90	61.0
123.70	134.0
124.20	80.0
125.00	91.0
125.90	51.0
128.00	351.0
129.00	394.0
129.80	305.0
131.00	246.0
133.10	80.0
133.80	135.0
134.80	235.0
136.60	143.0
137.10	110.0
139.70	87.0
140.90	1582.0
141.90	176.0
142.80	1725.0
143.80	123.0
145.00	439.0
145.80	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

147.00	145.0
148.10	247.0
148.90	156.0
150.10	88.0
152.70	55.0
155.00	279.0
156.00	64.0
156.90	227.0
159.00	199.0
160.70	116.0
162.90	54.0
165.80	89.0
169.10	74.0
170.20	145.0
170.90	340.0
172.00	1031.0
173.00	1730.0
174.00	73008.0
175.00	6319.0
176.00	67192.0
177.00	4601.0
178.10	102.0
191.00	223.0
193.10	120.0
193.80	83.0
194.20	77.0
207.10	162.0
249.10	107.0
264.80	94.0
265.40	57.0
281.20	1569.0
282.00	606.0
282.90	248.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

m/z	Abundance
35.20	121.0
36.00	1351.0
37.00	4674.0
38.10	4778.0
39.00	1765.0
39.80	208.0
40.40	95.0
41.10	113.0
43.10	221.0
44.00	998.0
44.90	945.0
45.90	82.0
47.00	650.0
48.10	588.0
49.00	3870.0
50.00	17440.0
51.00	5108.0
52.10	222.0
53.10	207.0
53.90	66.0
54.80	320.0
56.00	1958.0
57.10	3074.0
58.00	128.0
58.50	67.0
60.10	837.0
61.00	5132.0
62.00	4503.0
63.00	4395.0
64.00	625.0
65.00	621.0
67.00	419.0
68.00	9026.0
69.00	10630.0
70.00	819.0
71.90	558.0
73.00	4625.0
74.10	17176.0
75.10	43152.0
76.00	4419.0
76.80	480.0
77.80	464.0
79.00	5328.0
79.90	1189.0
81.00	5162.0
82.00	1035.0
83.10	202.0
85.70	149.0
87.00	2880.0
87.90	3726.0
89.80	65.0
90.90	522.0
92.00	2939.0
93.00	5006.0
94.00	12206.0
95.00	76936.0
96.00	4890.0
97.10	104.0
104.00	665.0
105.00	303.0
106.00	876.0
107.20	55.0
108.90	80.0
109.70	145.0
110.90	171.0
112.10	125.0
113.00	163.0
114.90	149.0
115.90	587.0
117.00	624.0
117.80	632.0
118.80	717.0
123.70	114.0
124.20	106.0
124.80	140.0
128.00	350.0
128.80	301.0
130.00	431.0
130.90	199.0
133.70	86.0
134.90	211.0
137.10	216.0
139.90	140.0
141.00	1444.0
143.00	1807.0
143.80	175.0
144.80	260.0
145.80	115.0
146.80	77.0
147.90	198.0
148.90	172.0
150.10	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

152.70	82.0
154.90	266.0
156.10	109.0
157.00	201.0
158.00	63.0
159.00	174.0
160.90	189.0
165.90	106.0
169.20	79.0
171.00	255.0
171.90	865.0
174.00	64512.0
175.00	5310.0
176.00	63232.0
177.00	3563.0
177.90	121.0
191.60	115.0
193.00	83.0
194.30	118.0
206.90	133.0
264.80	96.0
279.50	57.0
281.00	533.0
282.10	376.0
283.00	169.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595