

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW072918\
 Data File : VW004289.D
 Acq On : 28 Jul 2018 00:05
 Operator : SY/AP
 Sample : J4204-05
 Misc : 5.67G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JJ1J2

Quant Time: Jul 28 02:54:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 28 02:53:40 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	252517	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	177775	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	38432	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	67570	26.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.32%
7) Chloroethane-d5	2.89	69	67250	36.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	145.48%
10) 1,1-Dichloroethene-d2	4.01	63	136460	22.49	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	89.96%
20) 2-Butanone-d5	7.08	46	71427	49.63	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.26%
24) Chloroform-d	7.65	84	181227	28.03	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	112.12%
26) 1,2-Dichloroethane-d4	8.31	65	108179	27.82	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.28%
29) Benzene-d6	8.27	84	337560	35.83	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	143.32%#
33) 1,2-Dichloropropane-d6	9.27	67	119781	38.22	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	152.88%#
37) Toluene-d8	10.33	98	265215	29.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	119.12%
38) trans-1,3-Dichloropropene-	10.59	79	33631	23.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.56%
39) 2-Hexanone-d5	10.93	63	38547	46.81	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.62%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	85740	26.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.16%
61) 1,2-Dichlorobenzene-d4	13.87	152	39048	27.18	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.72%


Target Compounds					Qvalue
13) Acetone	4.12	43	100288	69.013 ug/L	98
21) 2-Butanone	7.18	43	26768	14.614 ug/L	97
59) 1,2,3-Trichloropropane	13.57	75	4768	2.019 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW072918\
Data File : VW004289.D
Acq On : 28 Jul 2018 00:05
Operator : SY/AP
Sample : J4204-05
Misc : 5.67G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JJ1J2

Quant Time: Jul 28 02:54:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072618S.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 28 02:53:40 2018
Response via : Initial Calibration

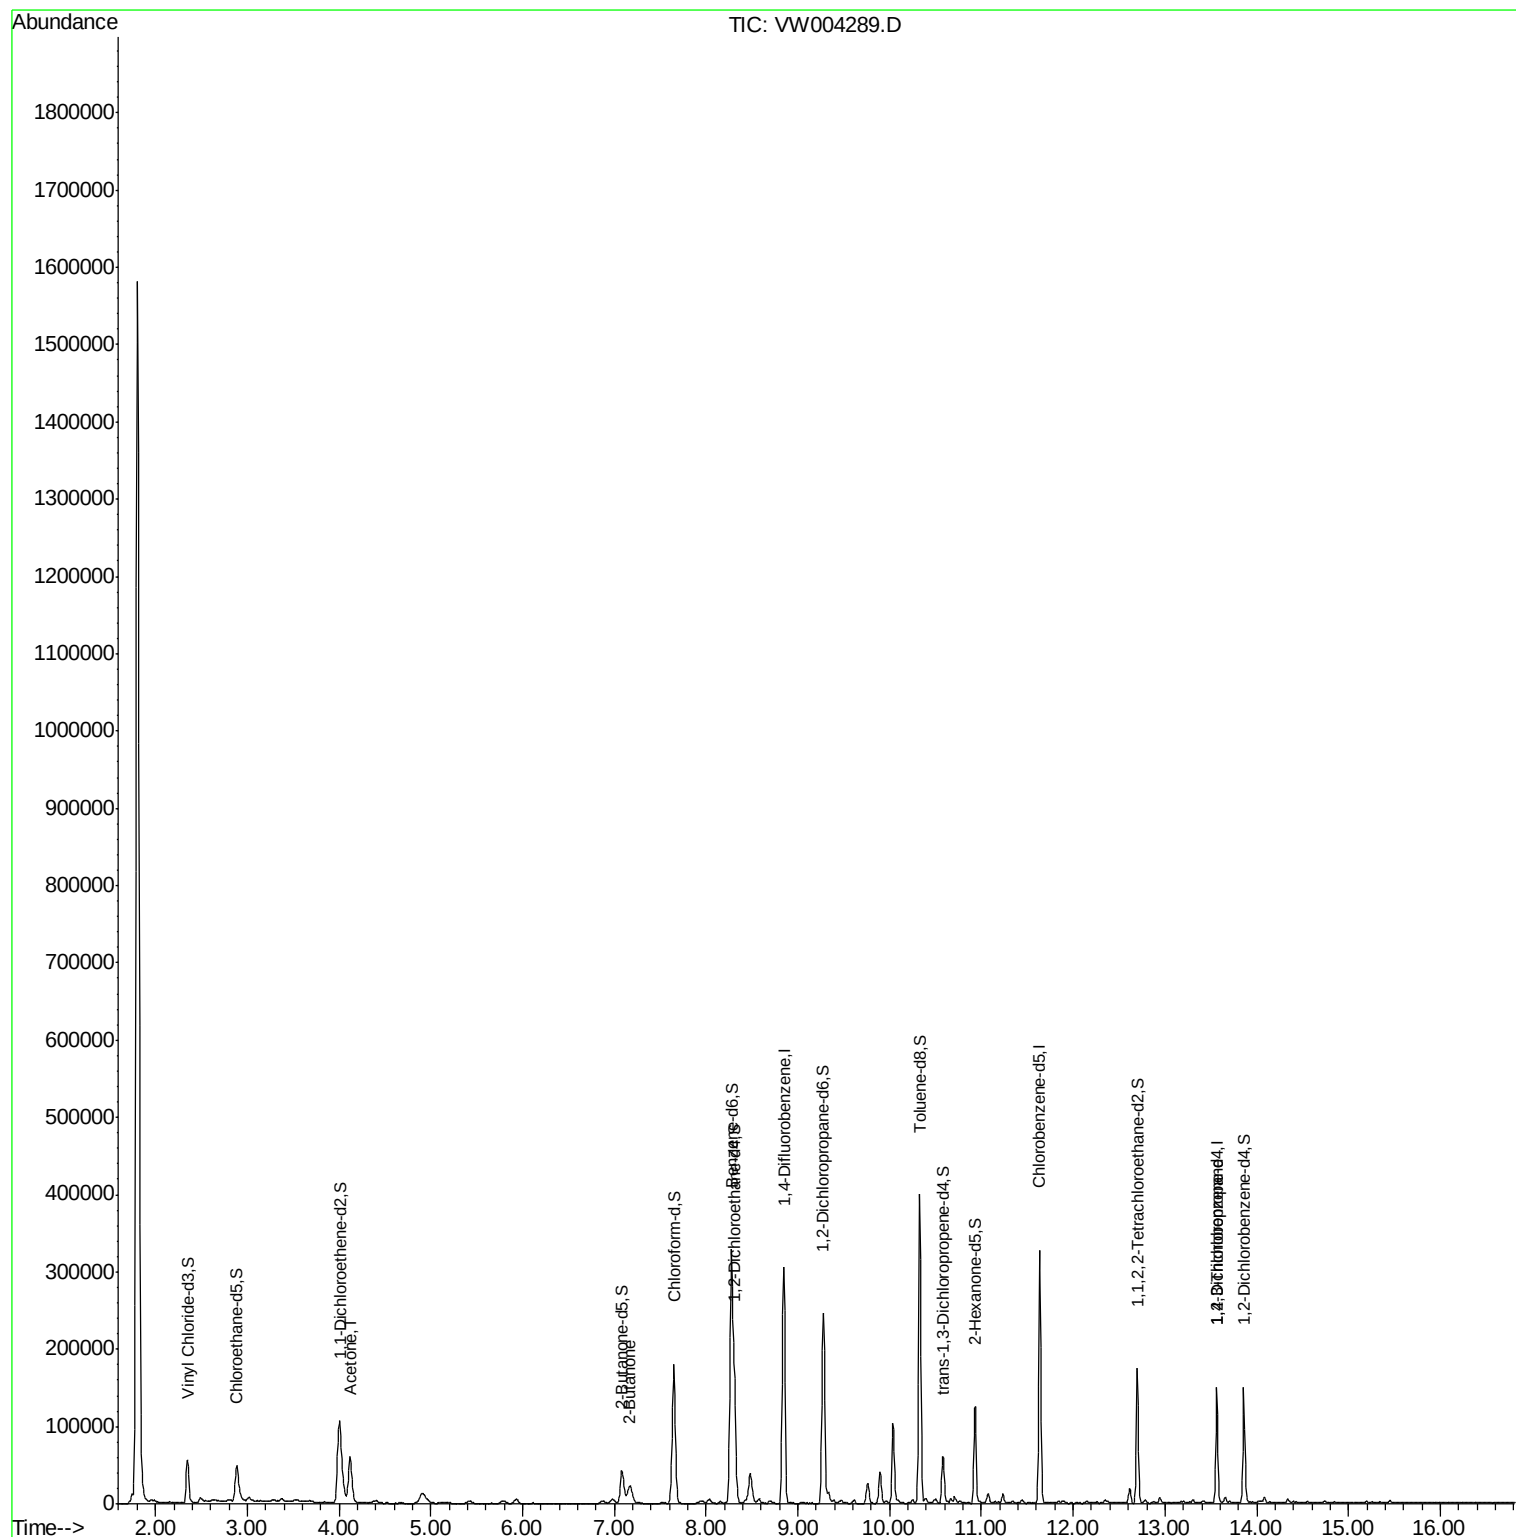

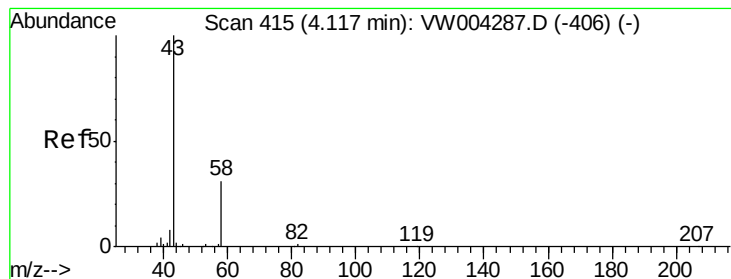

#13

Acetone

Concen: 69.013 ug/L

RT: 4.12 min Scan# 415

Delta R.T. -0.00 min

Lab File: VW004289.D

Acq: 28 Jul 2018 00:05

Instrument :

MSVOA_W

ClientSampled :





JJ1J2

Tgt Ion: 43 Resp: 100288

Ion Ratio Lower Upper

43 100

58 31.1 0.0 59.8

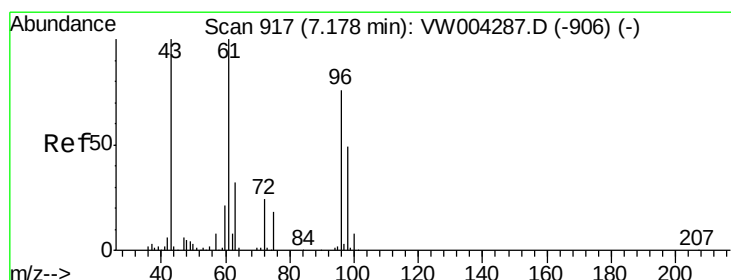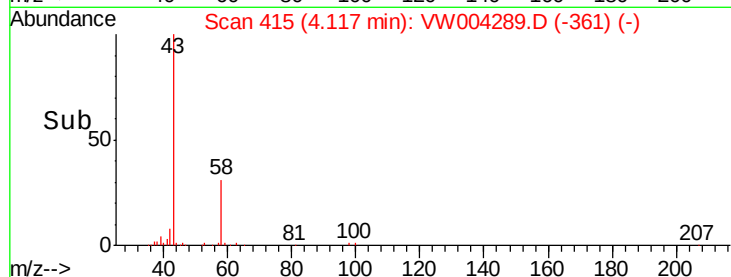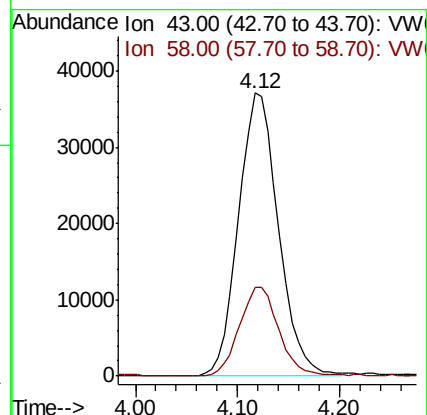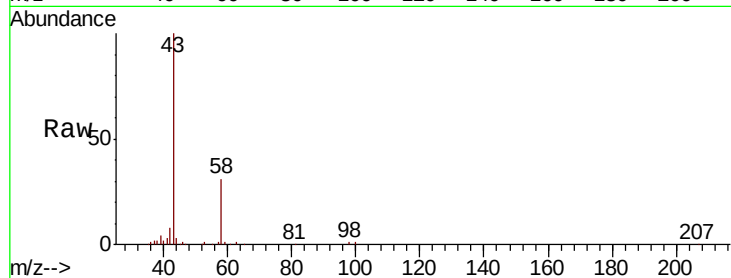

#21

2-Butanone

Concen: 14.614 ug/L

RT: 7.18 min Scan# 917

Delta R.T. -0.00 min

Lab File: VW004289.D




Acq: 28 Jul 2018 00:05


Tgt Ion: 43 Resp: 26768

Ion Ratio Lower Upper

43 100

72 23.3 12.3 36.9

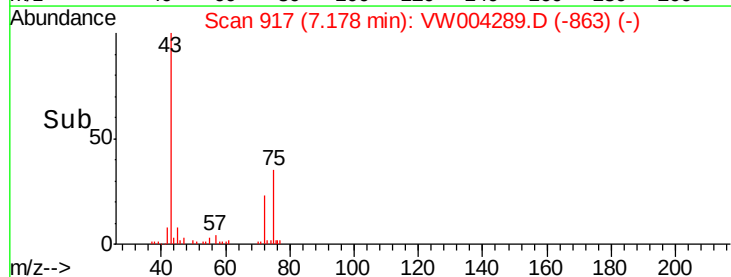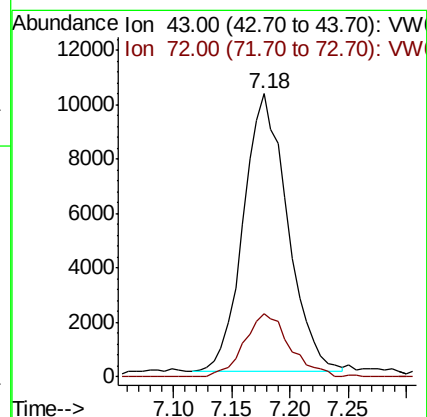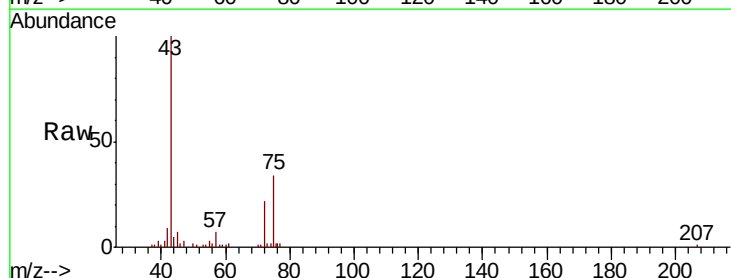

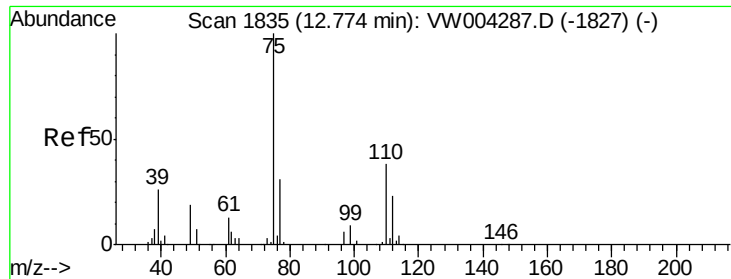

#59

1,2,3-Trichloropropane

Concen: 2.019 ug/L

RT: 13.57 min Scan# 1965

Delta R.T. 0.79 min

Lab File: VW004289.D

Acq: 28 Jul 2018 00:05

Instrument :

MSVOA_W

ClientSampleId :

JJ1J2

Tgt Ion: 75 Resp: 4768

Ion Ratio Lower Upper

75 100

77 35.4 25.2 37.8

