

Data File : VW011553.D
Acq On : 29 Jul 2019 11:30
Operator : SY/VA
Sample : VW0729SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK13

Quant Time: Jul 30 05:59:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 30 05:56:36 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	402408	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	354544	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	160838	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	112143	20.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.52%
7) Chloroethane-d5	2.89	69	84890	21.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.76%
10) 1,1-Dichloroethene-d2	4.01	63	192529	15.82	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.28%
20) 2-Butanone-d5	7.07	46	137447	60.08	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.16%
24) Chloroform-d	7.65	84	230930	22.41	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.64%
26) 1,2-Dichloroethane-d4	8.31	65	146545	23.92	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.68%
29) Benzene-d6	8.27	84	478845	22.58	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.32%
33) 1,2-Dichloropropane-d6	9.27	67	159448	23.21	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.84%
37) Toluene-d8	10.32	98	417843	21.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.96%
38) trans-1,3-Dichloropropene-	10.58	79	68268	23.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.00%
39) 2-Hexanone-d5	10.92	63	88188	59.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.40%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	141530	25.78	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.12%
61) 1,2-Dichlorobenzene-d4	13.85	152	140223	23.22	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.88%


Target Compounds						Qvalue
59) 1,2,3-Trichloropropane	13.56	75	21336	5.194	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011553.D
Acq On : 29 Jul 2019 11:30
Operator : SY/VA
Sample : VW0729SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK13

Quant Time: Jul 30 05:59:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 30 05:56:36 2019
Response via : Initial Calibration

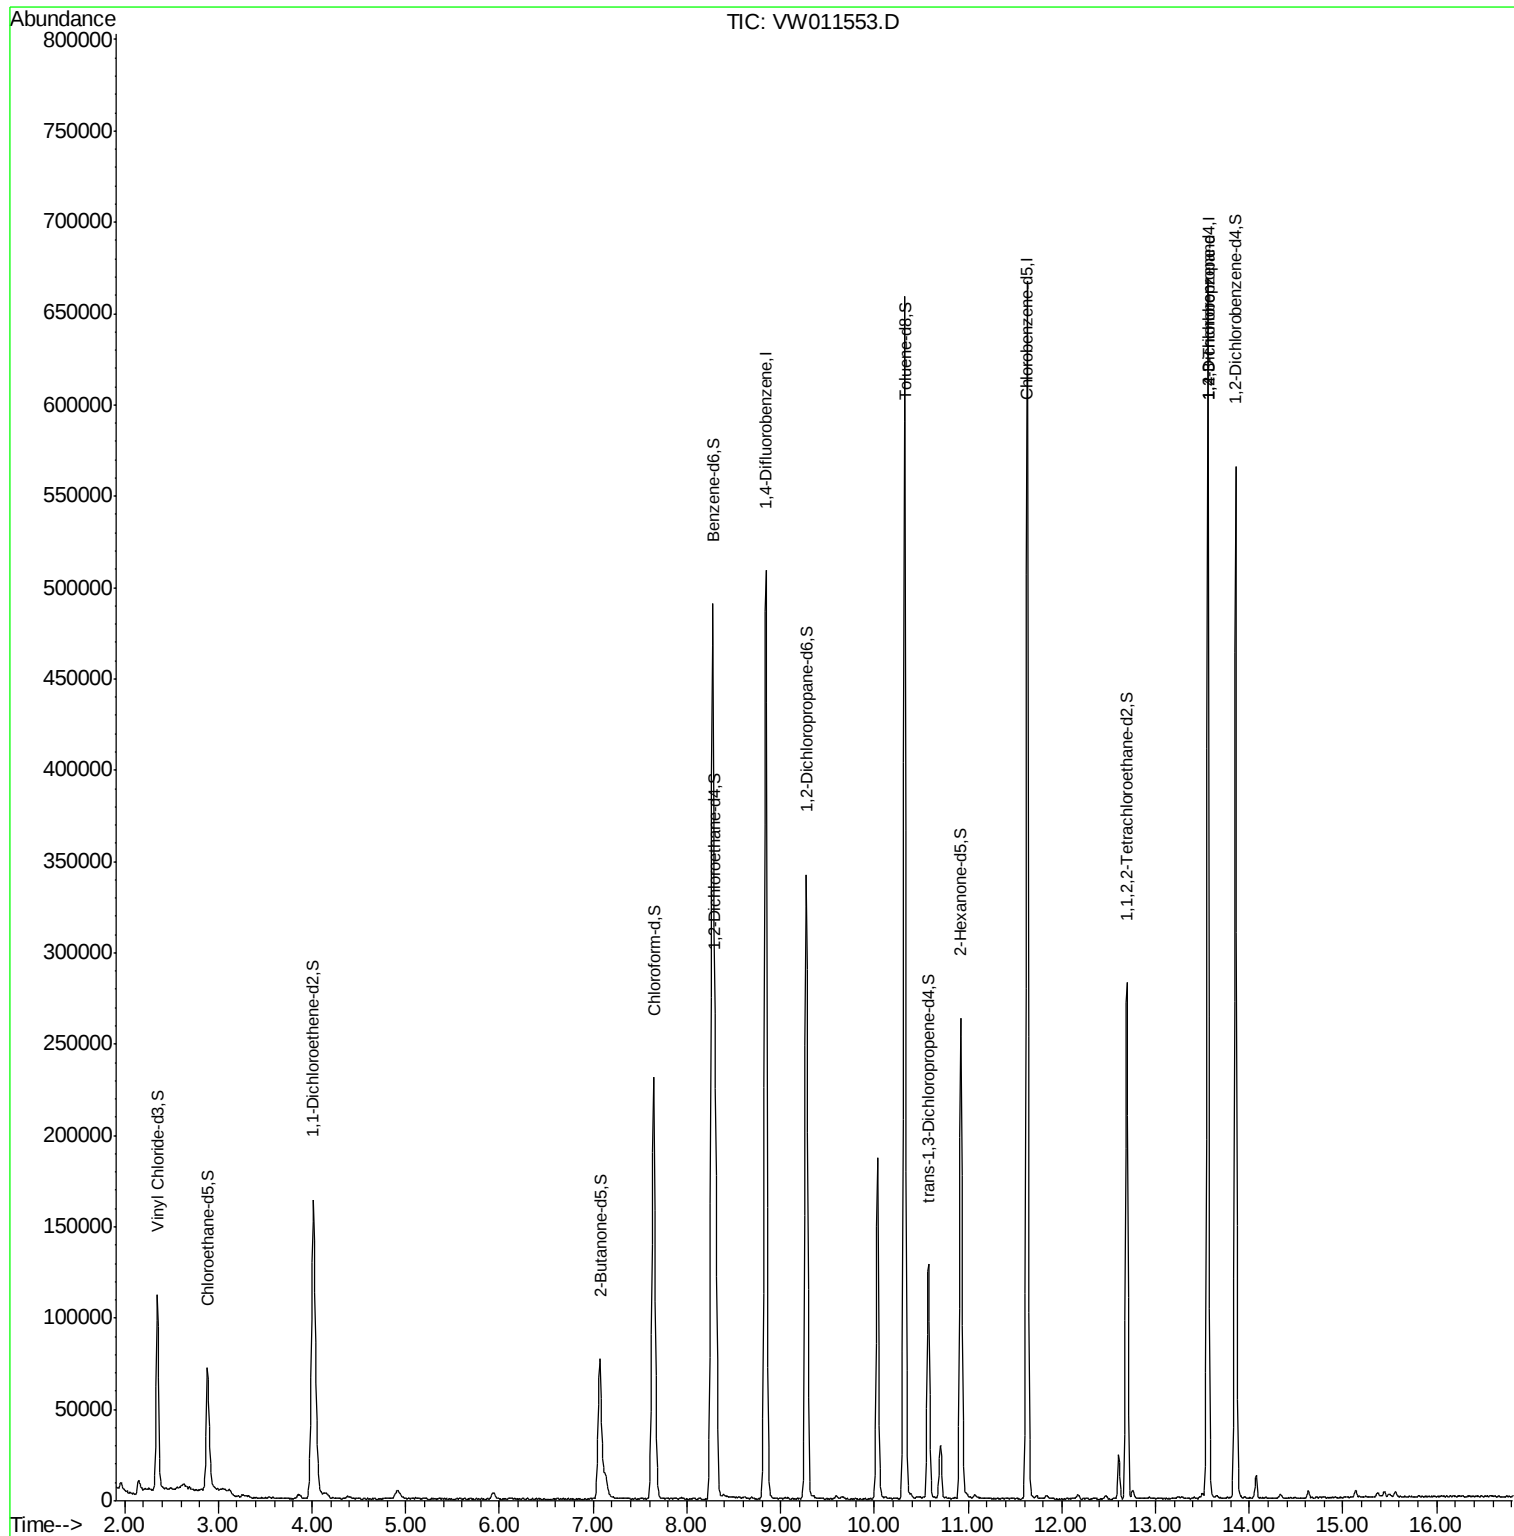

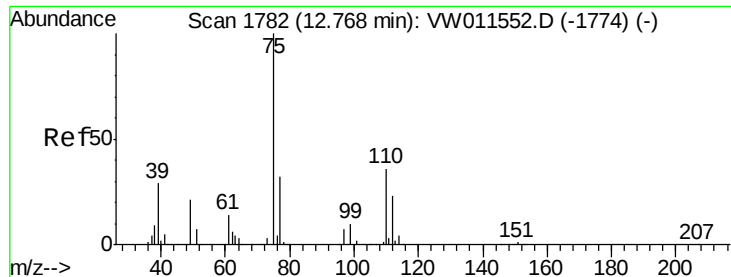

#59

1,2,3-Trichloropropane

Concen: 5.194 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW011553.D

Acq: 29 Jul 2019 11:30

Instrument :

MSVOA_W

ClientSampleId :

VBLK13

Tgt Ion: 75 Resp: 21336

Ion Ratio Lower Upper

75 100

77 36.8 25.8 38.8

