


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW072920\
 Data File : VW015987.D
 Acq On : 29 Jul 2020 08:47
 Operator : SY/VA
 Sample : BFB29
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB29

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM072020S.M
 Title : VOC Analysis
 Last Update : Fri Jul 31 06:34:21 2020

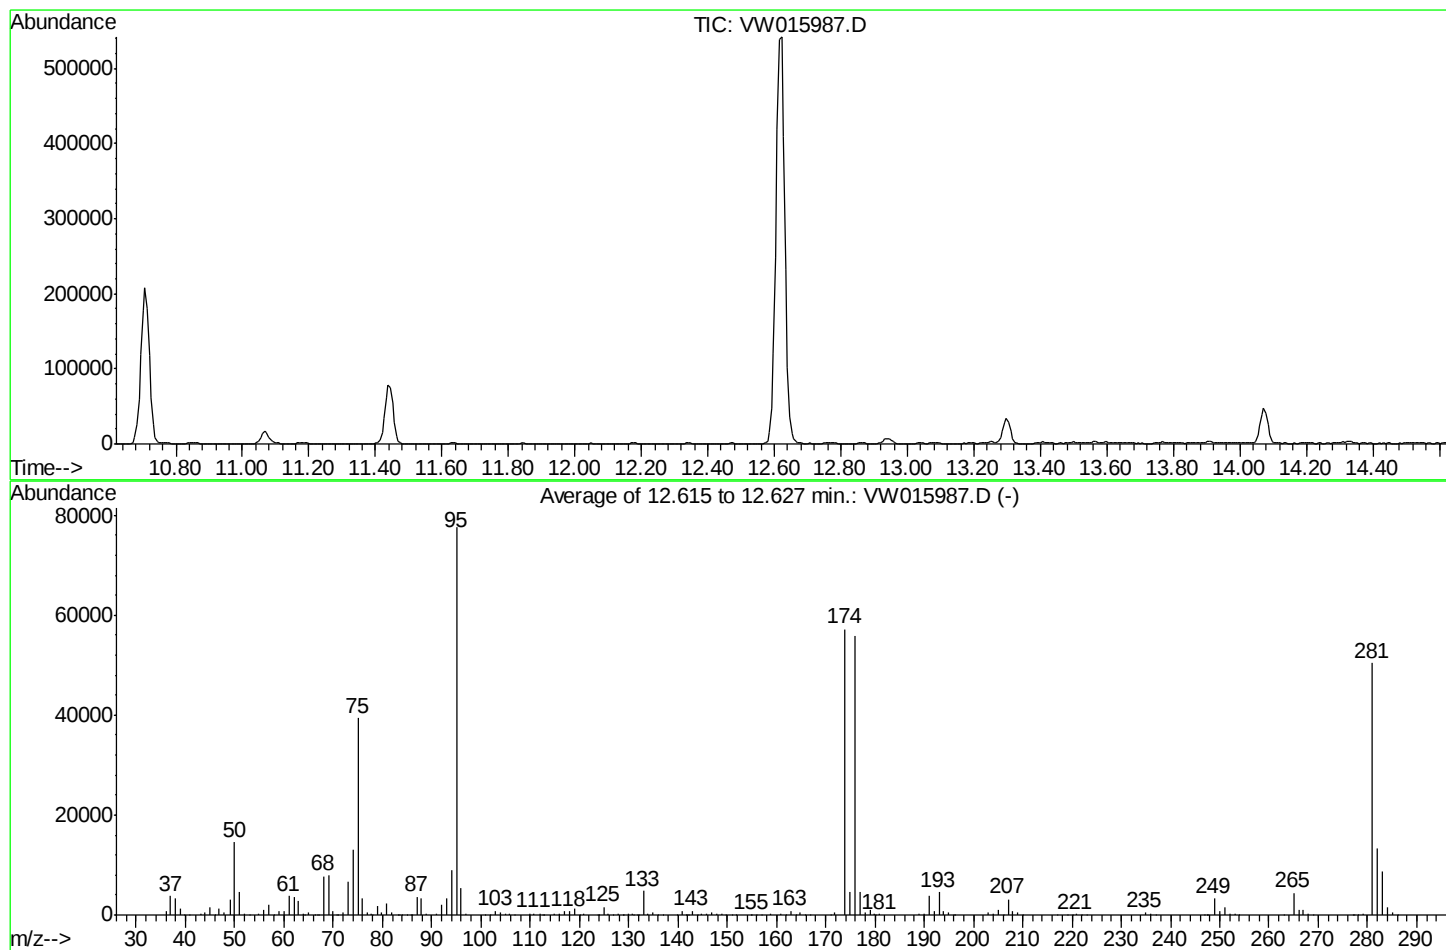

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	14546	PASS
75	95	30	80	50.8	39434	PASS
95	95	100	100	100.0	77578	PASS
96	95	5	9	6.9	5387	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.7	57200	PASS
175	174	5	9	8.1	4616	PASS
176	174	95	101	97.8	55941	PASS
177	176	5	9	8.5	4733	PASS

m/z	Abundance
36.00	736.0
37.00	4016.0
38.00	3465.0
39.00	1338.0
40.00	242.0
40.90	68.0
43.00	291.0
44.00	763.0
45.00	1720.0
45.90	117.0
46.90	1331.0
47.90	539.0
49.00	3294.0
50.00	14592.0
51.00	4579.0
52.00	197.0
53.00	73.0
54.90	272.0
56.00	1123.0
57.00	2373.0
58.00	207.0
59.00	1340.0
60.00	768.0
61.00	4051.0
62.00	3780.0
63.00	2743.0
63.90	330.0
64.90	503.0
66.20	72.0
66.90	206.0
68.00	7569.0
69.00	7701.0
70.00	646.0
71.00	89.0
72.00	564.0
73.00	8914.0
74.00	12337.0
75.00	38272.0
76.00	3478.0
76.90	388.0
77.80	396.0
78.90	1902.0
79.90	514.0
80.90	2293.0
82.00	558.0
83.50	246.0
85.00	174.0
85.80	168.0
86.90	3736.0
87.90	3247.0
88.70	572.0
90.90	275.0
92.00	2065.0
93.00	3124.0
94.00	8540.0
95.00	72640.0
96.00	5346.0
96.90	273.0
100.80	83.0
101.90	115.0
103.00	1159.0
103.90	817.0
104.90	462.0
105.90	350.0
106.80	93.0
109.80	313.0
110.80	485.0
112.00	306.0
112.90	189.0
115.00	547.0
115.80	296.0
116.90	694.0
117.90	1056.0
118.90	1764.0
120.00	163.0
120.90	245.0
123.70	103.0
125.00	2723.0
125.70	854.0
126.70	99.0
127.90	241.0
128.80	191.0
129.90	242.0
130.80	295.0
131.80	263.0
133.00	7746.0
134.80	689.0
136.00	62.0
136.90	110.0
140.90	541.0
141.70	104.0
142.90	727.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

143.90	67.0
144.90	252.0
145.90	180.0
146.90	804.0
148.00	219.0
148.80	334.0
149.80	71.0
151.00	96.0
154.80	132.0
157.00	77.0
158.80	166.0
160.80	403.0
161.90	162.0
162.90	1313.0
163.90	170.0
164.90	830.0
165.90	155.0
166.90	81.0
171.00	118.0
171.90	703.0
173.90	50496.0
174.90	4387.0
175.90	48264.0
176.90	5321.0
178.00	454.0
179.00	1427.0
179.90	282.0
181.00	231.0
189.10	496.0
189.90	344.0
190.90	5904.0
192.00	1318.0
193.00	6969.0
193.90	1227.0
194.90	689.0
195.90	73.0
202.90	679.0
204.00	213.0
205.00	1538.0
207.00	4681.0
208.00	954.0
209.00	578.0
210.00	94.0
216.90	64.0
219.10	116.0
220.00	59.0
220.90	289.0
221.90	57.0
223.00	110.0
234.90	658.0
235.90	209.0
236.90	186.0
247.00	129.0
248.90	4514.0
249.90	1138.0
250.90	2472.0
251.90	556.0
253.00	323.0
253.80	115.0
263.00	141.0
265.00	6103.0
266.00	1791.0
267.00	1566.0
267.90	553.0
269.00	176.0
276.90	169.0
278.10	158.0
279.10	540.0
281.00	75128.0
282.10	17248.0
283.00	12288.0
284.00	2341.0
285.00	684.0
286.00	109.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

m/z	Abundance
36.00	876.0
37.00	4268.0
38.00	3698.0
39.00	1673.0
39.90	287.0
40.90	88.0
43.10	237.0
44.00	847.0
45.00	1650.0
45.90	158.0
46.90	1400.0
47.90	529.0
49.00	3497.0
50.00	16370.0
51.00	5183.0
52.00	252.0
53.00	113.0
55.00	310.0
56.00	1280.0
57.00	2271.0
57.90	100.0
59.00	523.0
59.90	749.0
61.00	4317.0
62.00	3948.0
63.00	3123.0
63.90	383.0
65.00	486.0
66.20	74.0
67.10	239.0
68.00	8614.0
69.00	9157.0
70.00	681.0
71.10	89.0
71.90	688.0
73.00	6834.0
74.00	14737.0
75.00	44576.0
76.00	3573.0
76.90	486.0
78.00	419.0
78.90	1961.0
79.90	733.0
80.90	2364.0
81.90	436.0
83.10	110.0
83.90	101.0
84.80	77.0
86.00	117.0
86.90	4135.0
87.90	3846.0
88.80	243.0
90.80	347.0
92.00	2449.0
92.90	3530.0
94.00	9840.0
95.00	86688.0
96.00	6255.0
96.90	163.0
102.90	1113.0
103.90	592.0
104.90	272.0
105.80	370.0
106.80	78.0
109.90	206.0
110.80	420.0
111.90	237.0
112.60	82.0
115.00	415.0
115.80	402.0
116.90	709.0
117.90	829.0
118.90	1192.0
119.90	78.0
120.80	209.0
125.00	1565.0
127.80	257.0
128.80	180.0
129.80	248.0
130.80	228.0
132.00	161.0
132.90	4589.0
134.90	491.0
135.90	53.0
136.80	115.0
140.90	765.0
141.90	132.0
142.90	902.0
143.80	77.0
144.90	238.0
145.90	152.0
146.80	445.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

147.90	329.0
148.90	313.0
151.80	64.0
155.00	191.0
157.00	113.0
158.90	178.0
160.80	391.0
161.70	148.0
162.90	798.0
164.00	184.0
164.80	452.0
165.80	112.0
170.90	92.0
171.90	659.0
173.90	61872.0
174.90	4738.0
175.90	64104.0
177.00	4860.0
178.00	502.0
178.90	1085.0
179.90	187.0
180.90	111.0
188.90	374.0
190.00	212.0
191.00	4196.0
191.90	892.0
193.00	4509.0
193.90	870.0
195.00	572.0
196.10	57.0
203.00	642.0
204.00	186.0
205.00	977.0
207.00	3087.0
208.00	670.0
208.90	394.0
210.00	78.0
218.90	117.0
220.90	224.0
234.80	465.0
236.00	225.0
236.90	117.0
246.90	94.0
247.30	55.0
247.70	66.0
248.90	3763.0
250.00	990.0
251.00	1470.0
252.00	391.0
253.00	249.0
262.80	51.0
265.00	4664.0
266.00	1019.0
267.00	1274.0
268.00	258.0
269.10	111.0
277.40	103.0
278.10	127.0
279.00	332.0
281.00	49728.0
282.00	15299.0
283.00	9671.0
283.90	1632.0
285.00	389.0
286.00	100.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

m/z	Abundance
36.00	638.0
37.00	3064.0
38.00	2954.0
39.00	1170.0
40.00	244.0
42.90	76.0
43.90	681.0
44.90	907.0
47.00	881.0
48.00	413.0
49.00	2637.0
50.00	12676.0
51.00	3943.0
52.00	149.0
52.80	60.0
54.90	133.0
56.00	1025.0
57.00	1935.0
58.10	75.0
58.90	230.0
60.00	553.0
61.00	3102.0
62.00	3148.0
62.90	2397.0
64.10	266.0
65.00	391.0
67.10	173.0
68.00	6905.0
69.00	6989.0
69.90	658.0
70.80	57.0
72.00	344.0
73.00	4137.0
74.00	11917.0
75.00	35456.0
76.00	2925.0
76.90	507.0
77.80	337.0
78.90	1833.0
79.90	509.0
80.90	2052.0
81.90	452.0
83.10	92.0
86.00	75.0
87.00	2914.0
87.90	2870.0
90.80	233.0
92.00	1993.0
93.00	3067.0
94.00	8196.0
95.00	73408.0
96.00	4562.0
97.00	151.0
102.80	323.0
103.80	401.0
104.80	163.0
106.00	250.0
106.80	53.0
109.80	178.0
110.70	144.0
111.90	131.0
112.50	67.0
114.80	153.0
115.80	196.0
116.80	603.0
117.90	421.0
119.00	754.0
120.00	74.0
120.80	82.0
124.00	77.0
125.00	610.0
125.70	224.0
127.80	304.0
129.00	130.0
129.80	261.0
131.00	146.0
133.00	2020.0
133.80	431.0
134.80	261.0
136.90	89.0
139.70	68.0
141.00	703.0
142.10	72.0
142.90	688.0
143.90	59.0
144.70	128.0
144.90	122.0
145.90	101.0
146.70	248.0
147.90	171.0
149.00	172.0
149.80	92.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

151.90	53.0
154.90	180.0
155.90	58.0
156.80	161.0
158.90	103.0
160.80	202.0
161.90	72.0
162.80	400.0
163.80	53.0
164.90	245.0
171.90	428.0
173.90	59232.0
175.00	4723.0
175.90	55456.0
176.90	4018.0
177.90	249.0
178.90	450.0
180.10	97.0
180.90	85.0
189.00	140.0
190.00	100.0
190.90	1816.0
191.90	391.0
192.90	2260.0
193.90	447.0
195.00	233.0
202.90	252.0
203.90	104.0
205.00	654.0
206.10	161.0
207.00	1548.0
208.00	374.0
208.90	216.0
219.10	72.0
220.70	104.0
234.90	248.0
235.90	64.0
236.80	54.0
248.90	1643.0
249.90	440.0
250.90	853.0
251.80	123.0
253.00	74.0
265.00	2483.0
266.00	514.0
267.00	636.0
268.10	128.0
269.00	57.0
278.10	62.0
278.90	137.0
281.00	26208.0
282.00	7651.0
283.00	4229.0
284.00	902.0
285.00	222.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29

Scan 1749 (12.566 min): VW015987.D
BFB29

m/z	Abundance
38.90	59.0
39.80	160.0
41.00	51.0
41.80	64.0
42.80	61.0
44.00	300.0
56.90	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB29