

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
 Data File : VW024132.D
 Acq On : 29 Jul 2022 16:42
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 30 00:13:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 30 00:12:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	197643	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	194743	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	87046	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.342	65	118715	28.022	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	112.080%
7) Chloroethane-d5	2.714	69	212	0.074	ug/L	-0.16
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.280%#
11) 1,1-Dichloroethene-d2	4.208	63	180	0.048	ug/L	0.20
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.200%#
21) 2-Butanone-d5	7.079	46	38899	51.664	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.320%
24) Chloroform-d	7.646	84	134079	24.676	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.720%
26) 1,2-Dichloroethane-d4	8.305	65	80565	25.808	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.240%
32) Benzene-d6	8.274	84	241289	26.672	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	106.680%
36) 1,2-Dichloropropane-d6	9.274	67	78354	27.460	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.840%
41) Toluene-d8	10.323	98	223932	24.752	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.000%
43) trans-1,3-Dichloroprop...	10.573	79	31488	24.889	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.560%
47) 2-Hexanone-d5	10.926	63	30965	51.909	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.820%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	80056	24.316	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.280%
66) 1,2-Dichlorobenzene-d4	13.852	152	80700	28.627	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	114.520%
Target Compounds						Qvalue
16) Methylene chloride	4.909	84	14839	4.933	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
Data File : VW024132.D
Acq On : 29 Jul 2022 16:42
Operator : SY/VA
Sample : VIBLK
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jul 30 00:13:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 30 00:12:08 2022
Response via : Initial Calibration

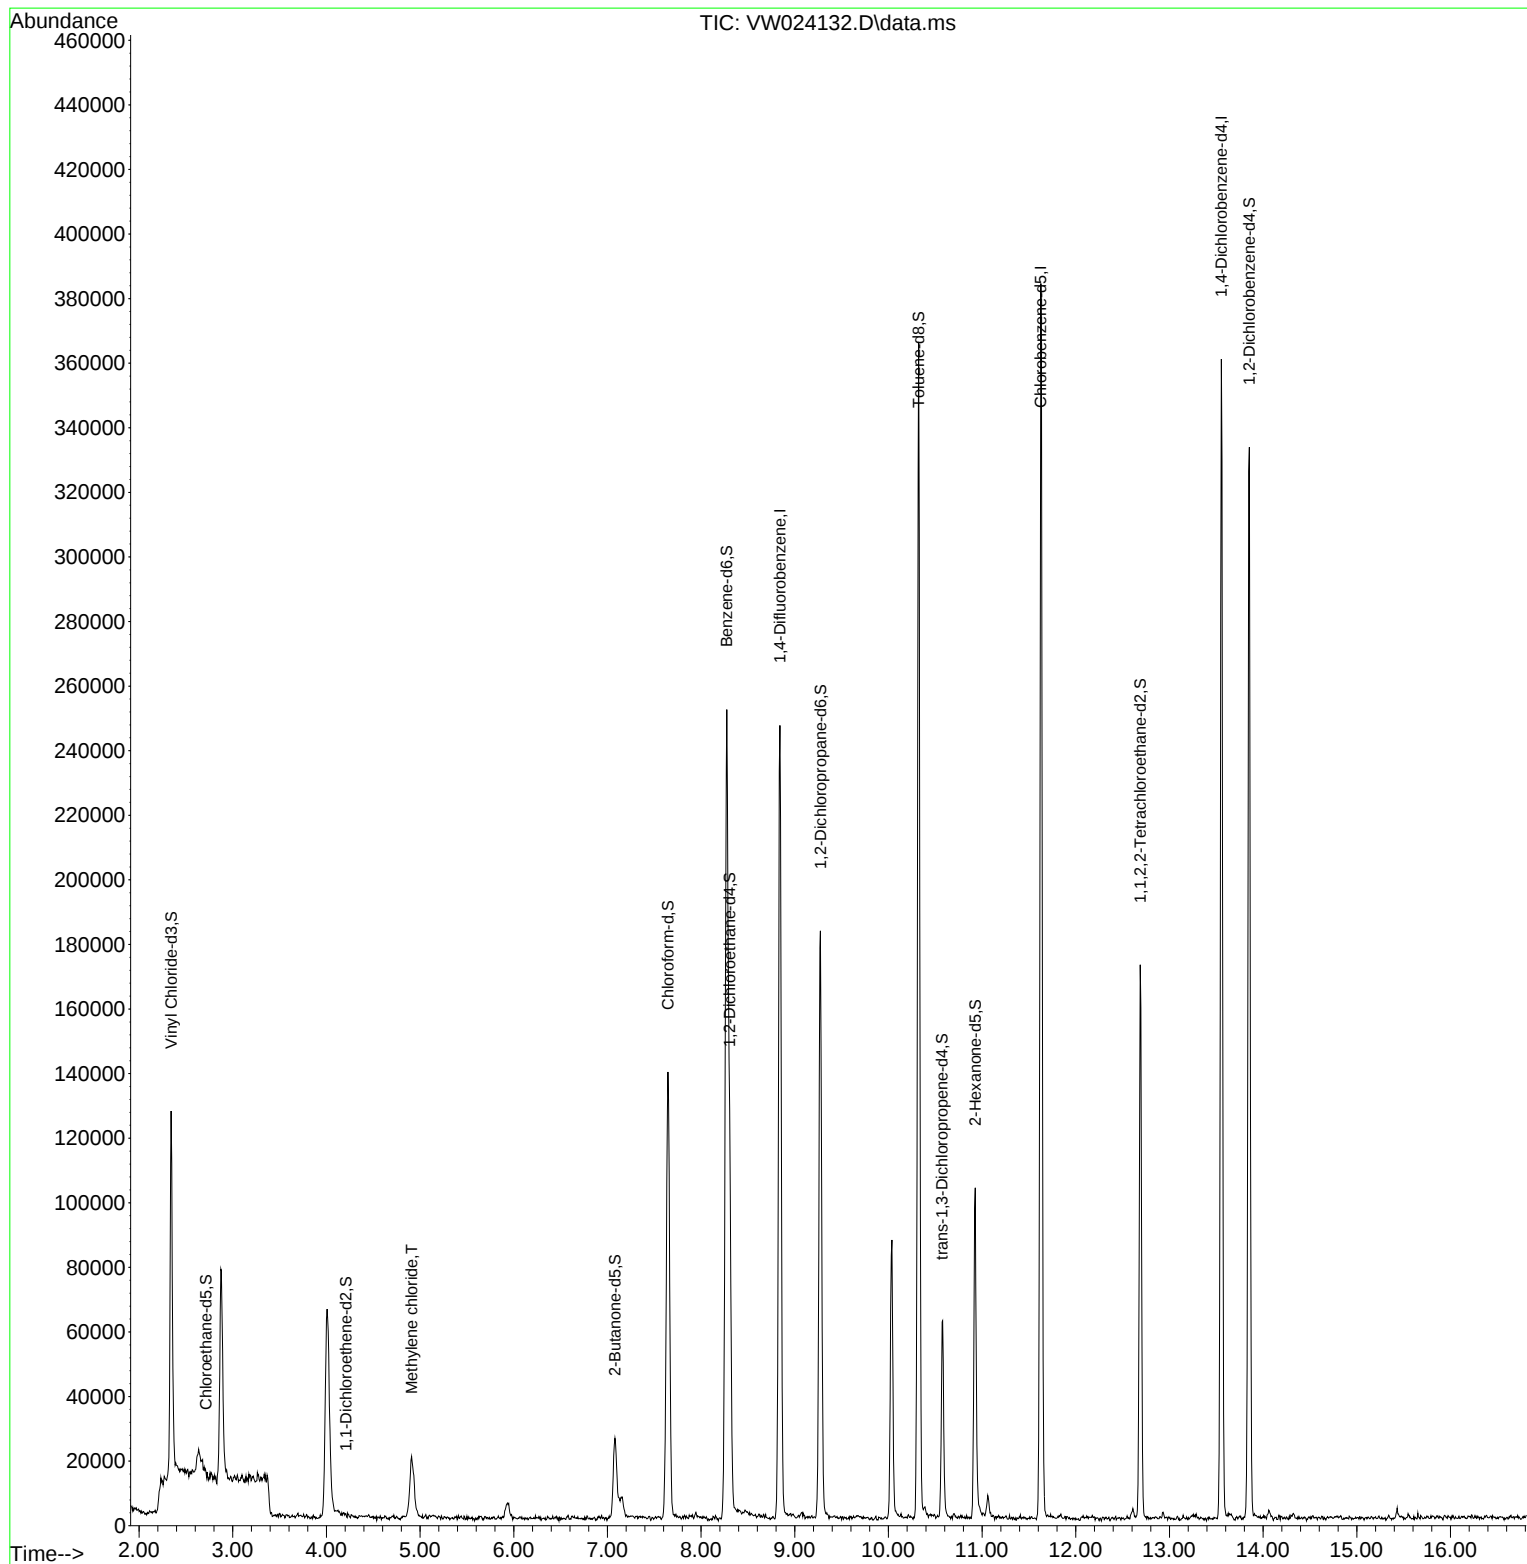

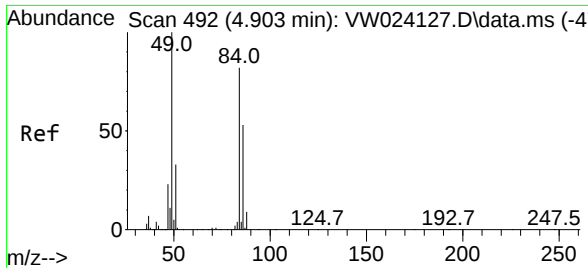

#16
Methylene chloride
Concen: 4.933 ug/L
RT: 4.909 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW024132.D
Acq: 29 Jul 2022 16:42

Instrument :
MSVOA_W
ClientSampleId :

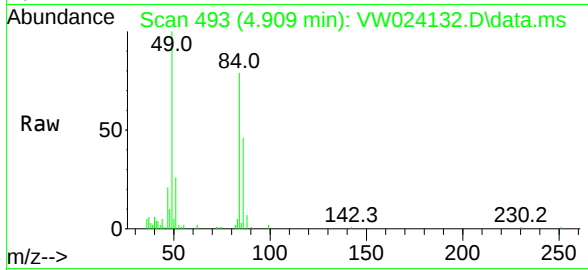

Tgt Ion: 84 Resp: 14839
Ion Ratio Lower Upper
84 100
86 58.4 44.7 83.1
49 127.2 83.7 155.4

