




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
Data File : VW024129.D
Acq On : 29 Jul 2022 15:28
Operator : SY/VA
Sample : VW0729SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK567

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 30 00:12:08 2022
Response via : Initial Calibration

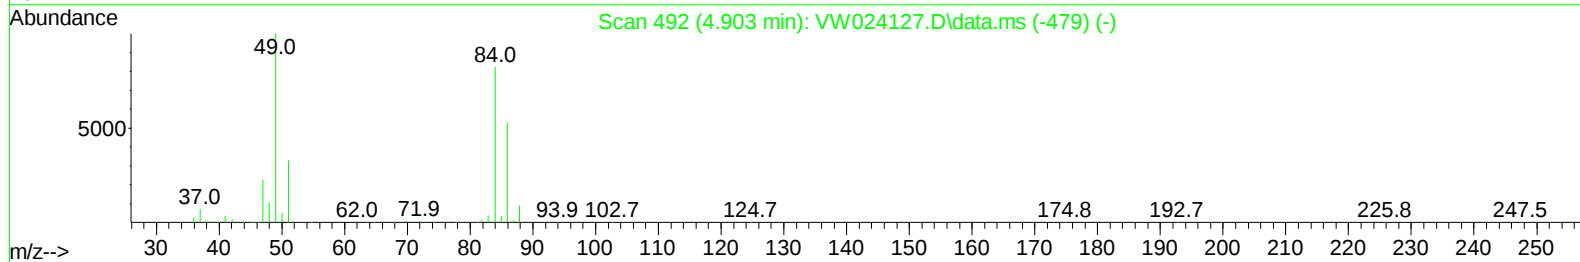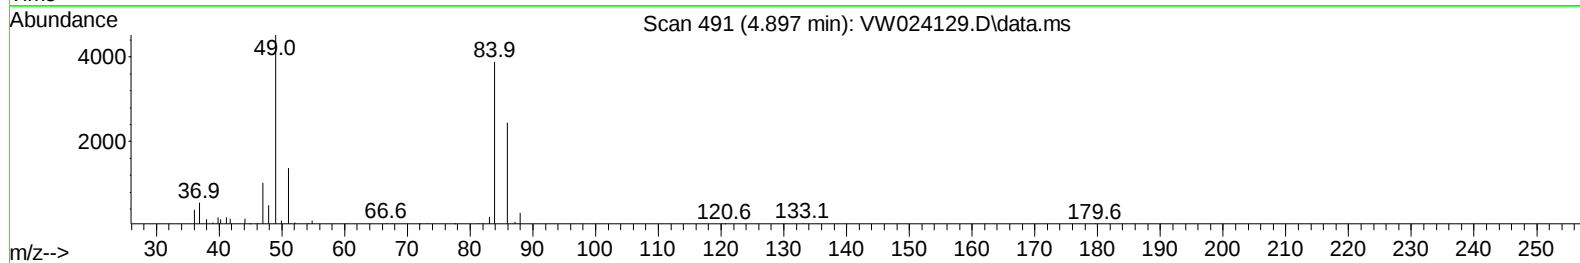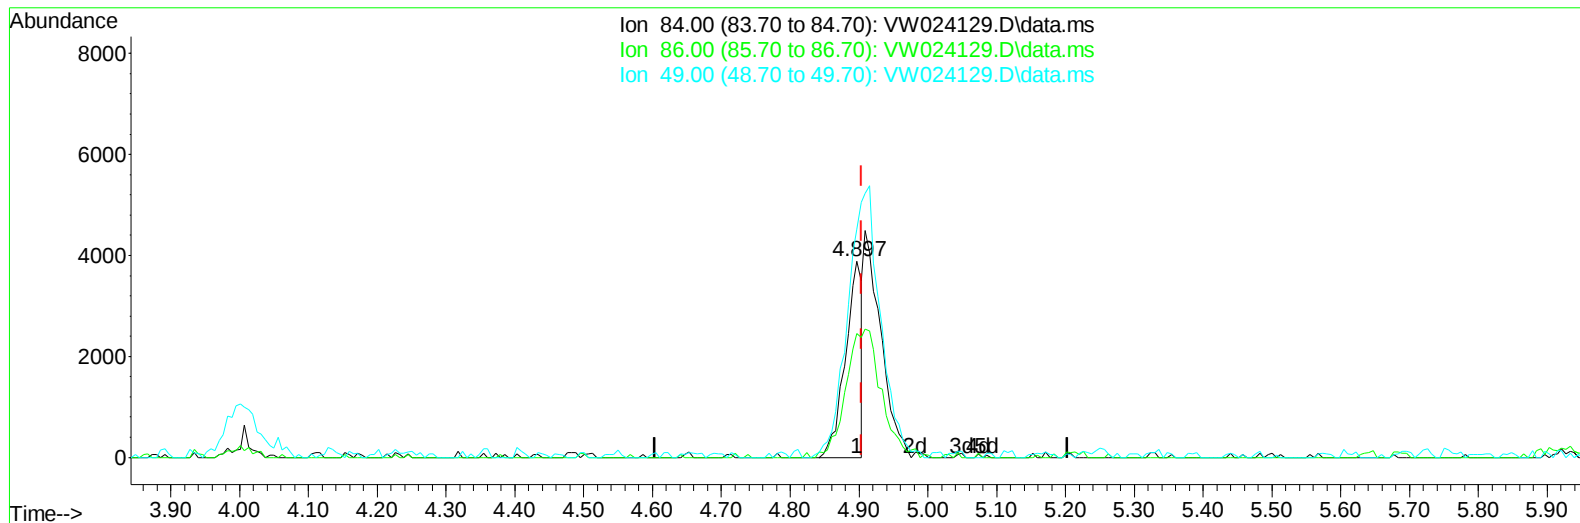

TIC: VW024129.D\data.ms

(16) Methylene chloride (T)

4.897min (-0.006) 2.03 ug/L

response 6478

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	62.97
49.00	119.50	116.20
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
 Data File : VW024129.D
 Acq On : 29 Jul 2022 15:28
 Operator : SY/VA
 Sample : VW0729SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK567

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 30 00:12:08 2022
 Response via : Initial Calibration

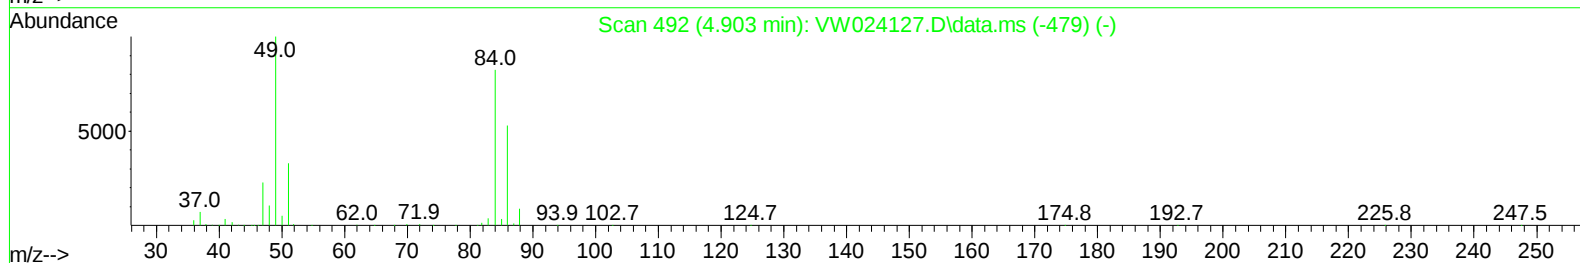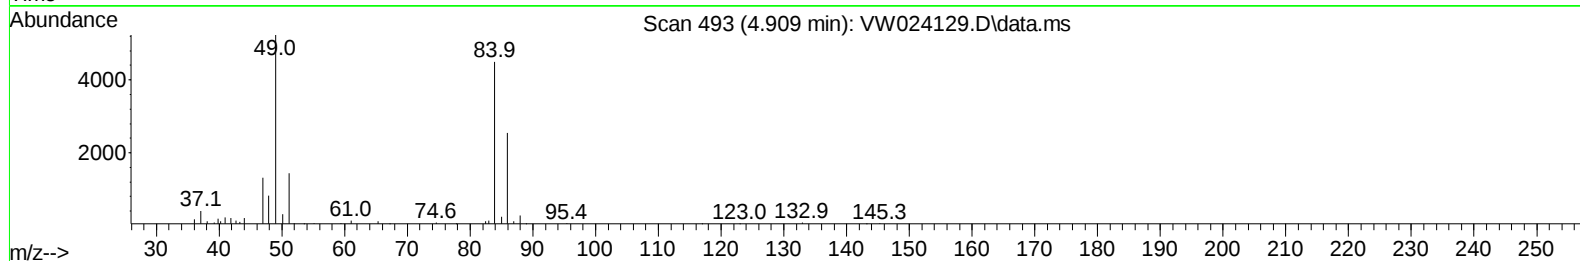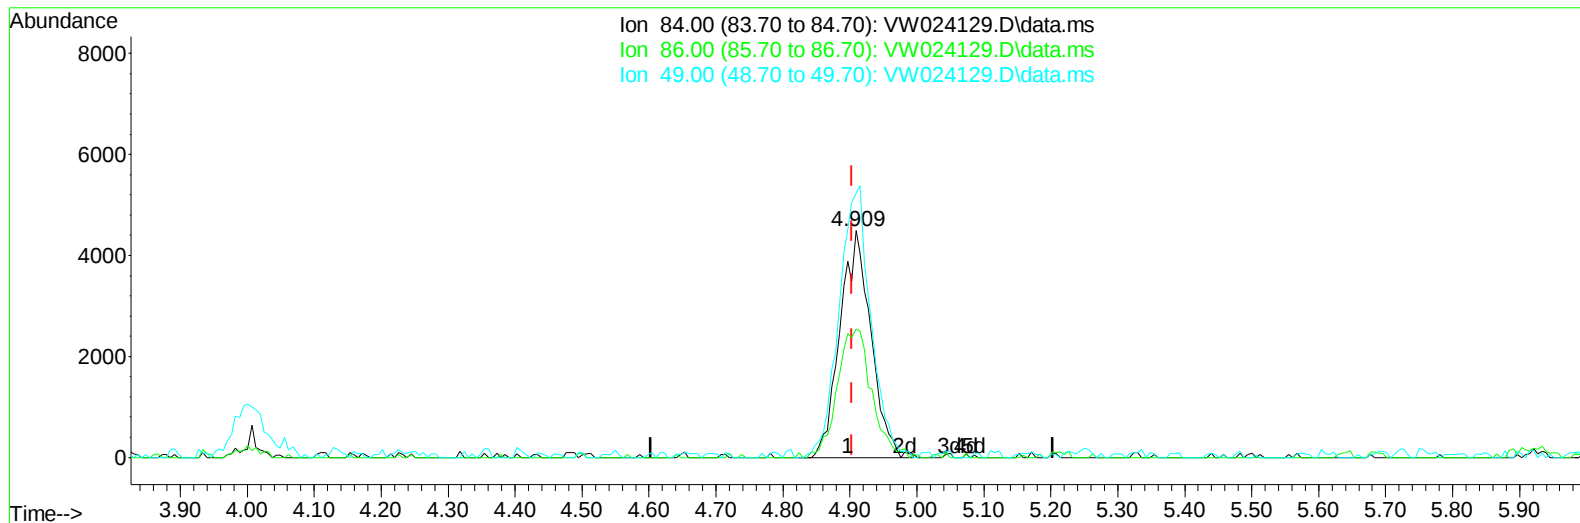

TIC: VW024129.D\data.ms

(16) Methylene chloride (T)

4.909min (+ 0.006) 4.50 ug/L m

response 14356

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	56.54
49.00	119.50	116.57
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
 Data File : VW024129.D
 Acq On : 29 Jul 2022 15:28
 Operator : SY/VA
 Sample : VW0729SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK567

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 30 00:12:08 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		209664	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117		213157	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		98413	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		111443	24.797	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	99.200%	
7) Chloroethane-d5	2.879	69		72728	23.951	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	95.800%	
11) 1,1-Dichloroethene-d2	4.001	63		64731	16.358	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	65.440%	
21) 2-Butanone-d5	7.079	46		36245	45.379	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	90.760%	
24) Chloroform-d	7.640	84		127163	22.061	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	88.240%	
26) 1,2-Dichloroethane-d4	8.305	65		74166	22.396	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	89.600%	
32) Benzene-d6	8.268	84		225940	22.818	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	91.280%	
36) 1,2-Dichloropropane-d6	9.268	67		71248	22.813	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	91.240%	
41) Toluene-d8	10.323	98		216319	21.845	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	87.360%	
43) trans-1,3-Dichloroprop...	10.579	79		29456	21.271	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	85.080%	
47) 2-Hexanone-d5	10.926	63		28377	43.461	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	86.920%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		75176	20.861	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	83.440%	
66) 1,2-Dichlorobenzene-d4	13.853	152		74948	23.515	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	94.080%	
Target Compounds							
16) Methylene chloride	4.909	84		14356m	4.499	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
Data File : VW024129.D
Acq On : 29 Jul 2022 15:28
Operator : SY/VA
Sample : VW0729SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK567

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 30 00:12:08 2022
Response via : Initial Calibration

