




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
Data File : VW024130.D
Acq On : 29 Jul 2022 15:53
Operator : SY/VA
Sample : N3790-25
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 30 00:12:08 2022
Response via : Initial Calibration

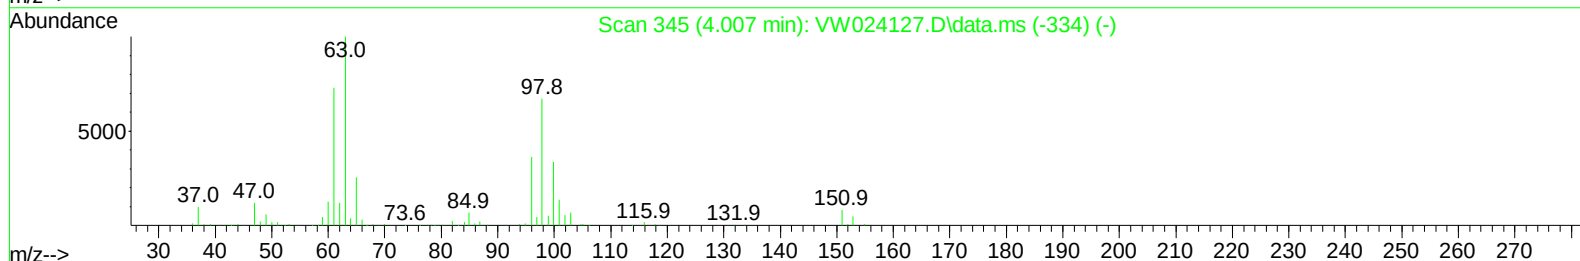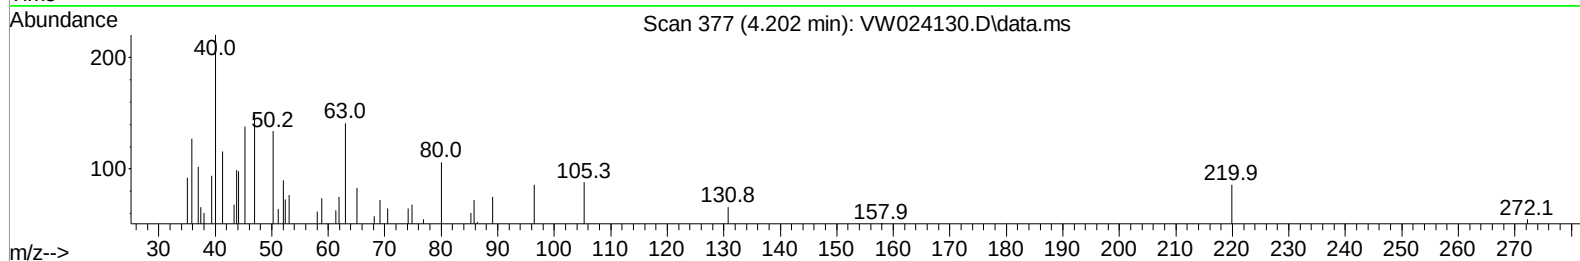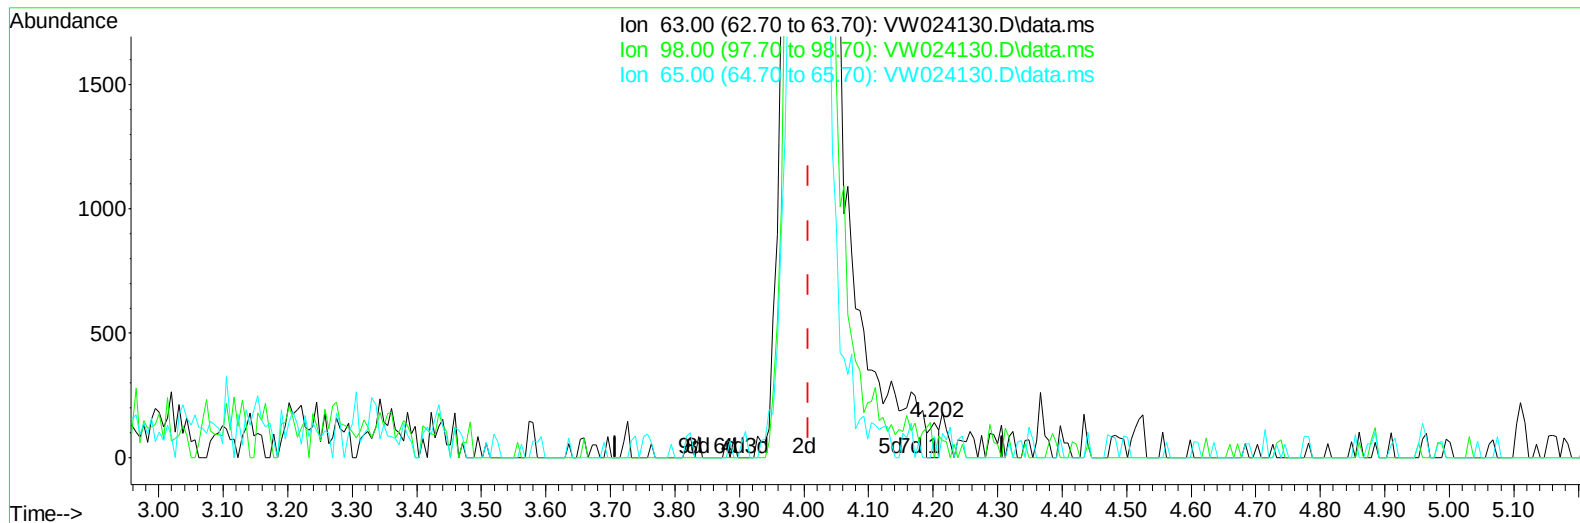

TIC: VW024130.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.202min (+ 0.195) 0.03 ug/L

response 133

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.10	60.15
65.00	23.20	22.56
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
Data File : VW024130.D
Acq On : 29 Jul 2022 15:53
Operator : SY/VA
Sample : N3790-25
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 30 00:12:08 2022
Response via : Initial Calibration

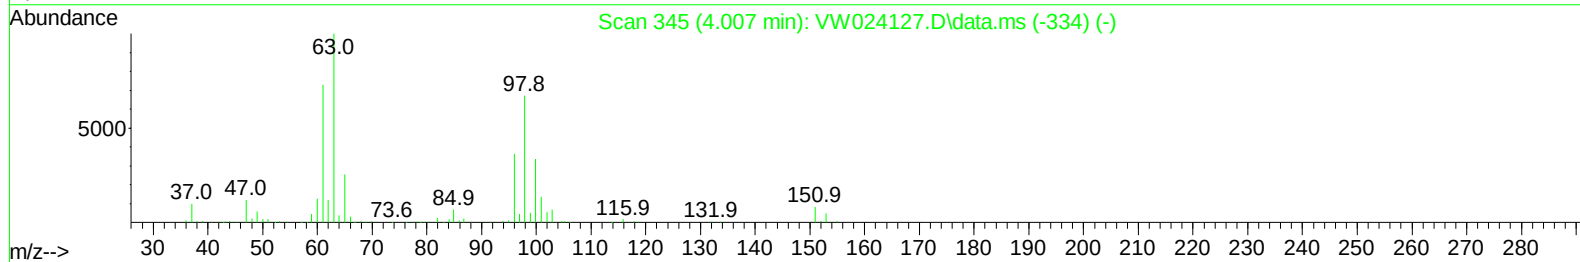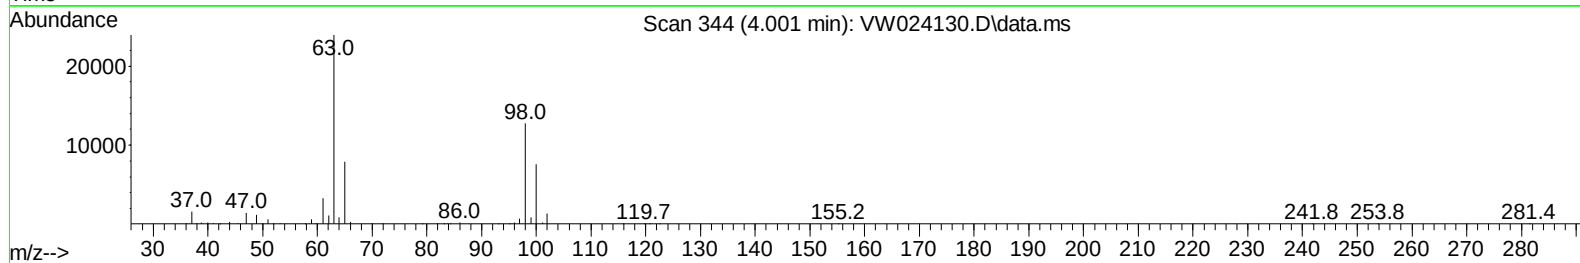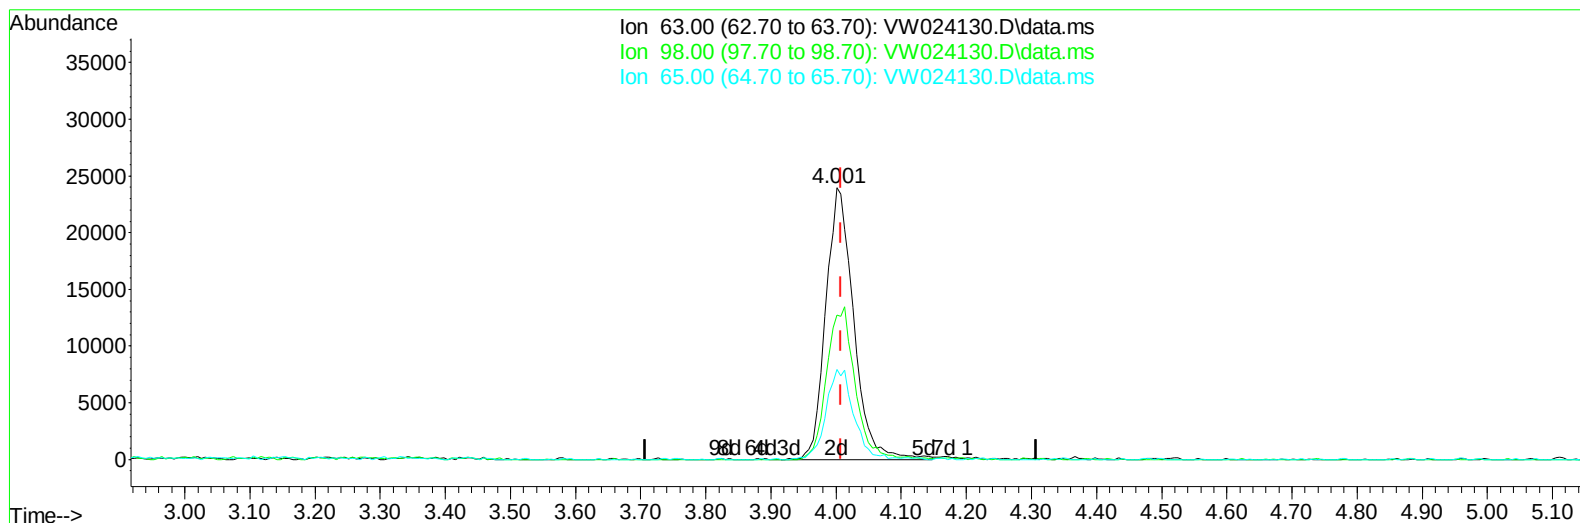

TIC: VW024130.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.001min (-0.006) 18.58 ug/L m

response 71290

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.10	0.11#
65.00	23.20	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
 Data File : VW024130.D
 Acq On : 29 Jul 2022 15:53
 Operator : SY/VA
 Sample : N3790-25
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 30 00:12:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	203238	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	208028	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	91225	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	120176	27.586	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	110.360%	
7) Chloroethane-d5	2.873	69	77363	26.283	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	105.120%	
11) 1,1-Dichloroethene-d2	4.001	63	71290m	18.585	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	74.320%	
21) 2-Butanone-d5	7.080	46	36695	47.395	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	94.800%	
24) Chloroform-d	7.647	84	140175	25.088	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	100.360%	
26) 1,2-Dichloroethane-d4	8.305	65	81632	25.430	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	101.720%	
32) Benzene-d6	8.269	84	251391	26.014	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	104.040%	
36) 1,2-Dichloropropane-d6	9.274	67	78891	25.882	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	103.520%	
41) Toluene-d8	10.323	98	234177	24.231	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	96.920%	
43) trans-1,3-Dichloroprop...	10.573	79	32449	24.011	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	96.040%	
47) 2-Hexanone-d5	10.921	63	30224	47.431	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	94.860%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	78804	22.407	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	89.640%	
66) 1,2-Dichlorobenzene-d4	13.853	152	81072	27.441	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	109.760%	
Target Compounds						
16) Methylene chloride	4.909	84	14465	4.676	ug/L	Qvalue 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
Data File : VW024130.D
Acq On : 29 Jul 2022 15:53
Operator : SY/VA
Sample : N3790-25
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 30 00:12:08 2022
Response via : Initial Calibration

