




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
Data File : VW024132.D
Acq On : 29 Jul 2022 16:42
Operator : SY/VA
Sample : VIBLK522
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK522

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 30 00:12:08 2022
Response via : Initial Calibration

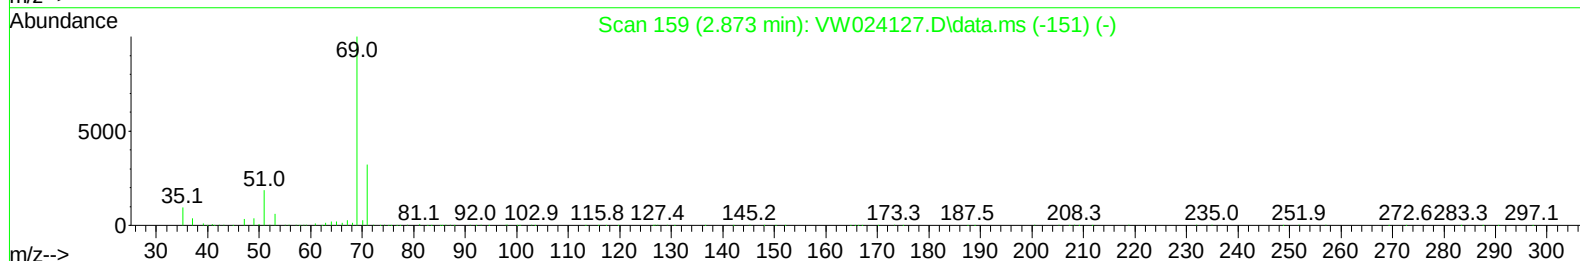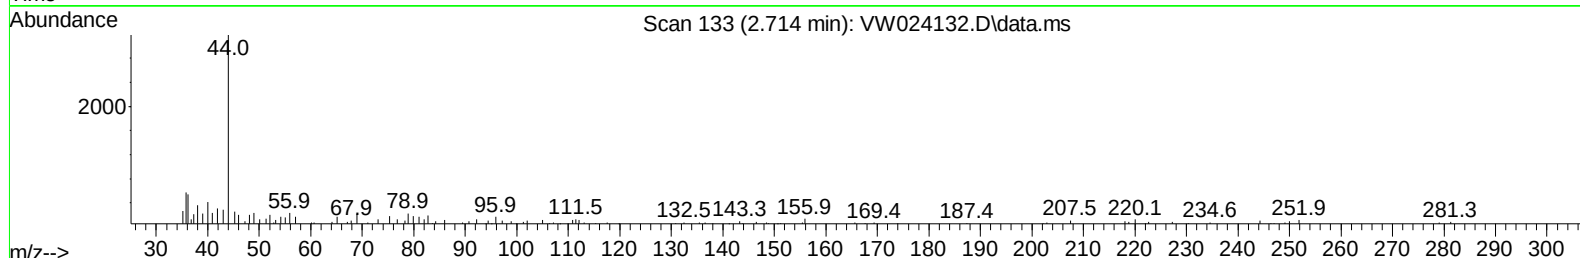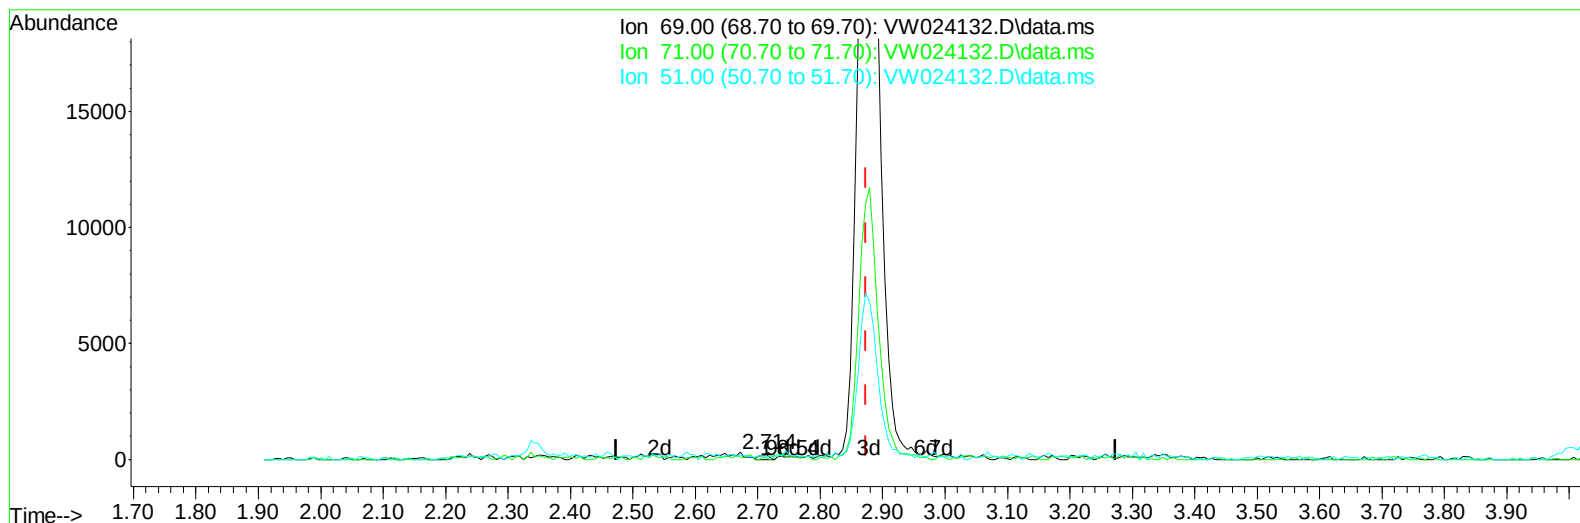

TIC: VW024132.D\data.ms

(7) Chloroethane-d5 (S)

2.714min (-0.159) 0.07 ug/L

response 212

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.80	23.11
51.00	27.90	34.91
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
 Data File : VW024132.D
 Acq On : 29 Jul 2022 16:42
 Operator : SY/VA
 Sample : VIBLK522
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK522

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 30 00:12:08 2022
 Response via : Initial Calibration

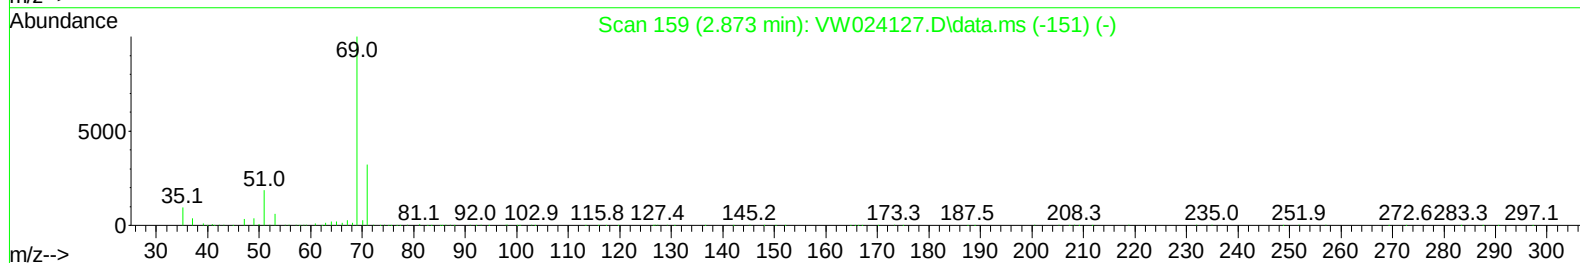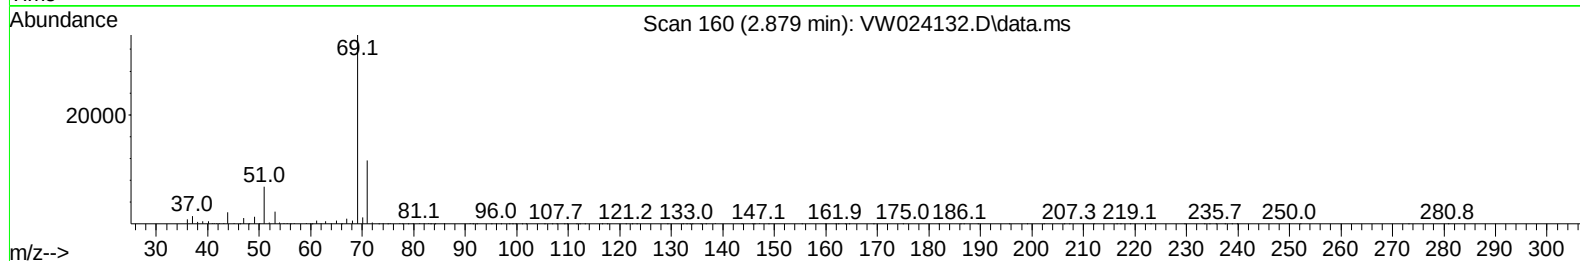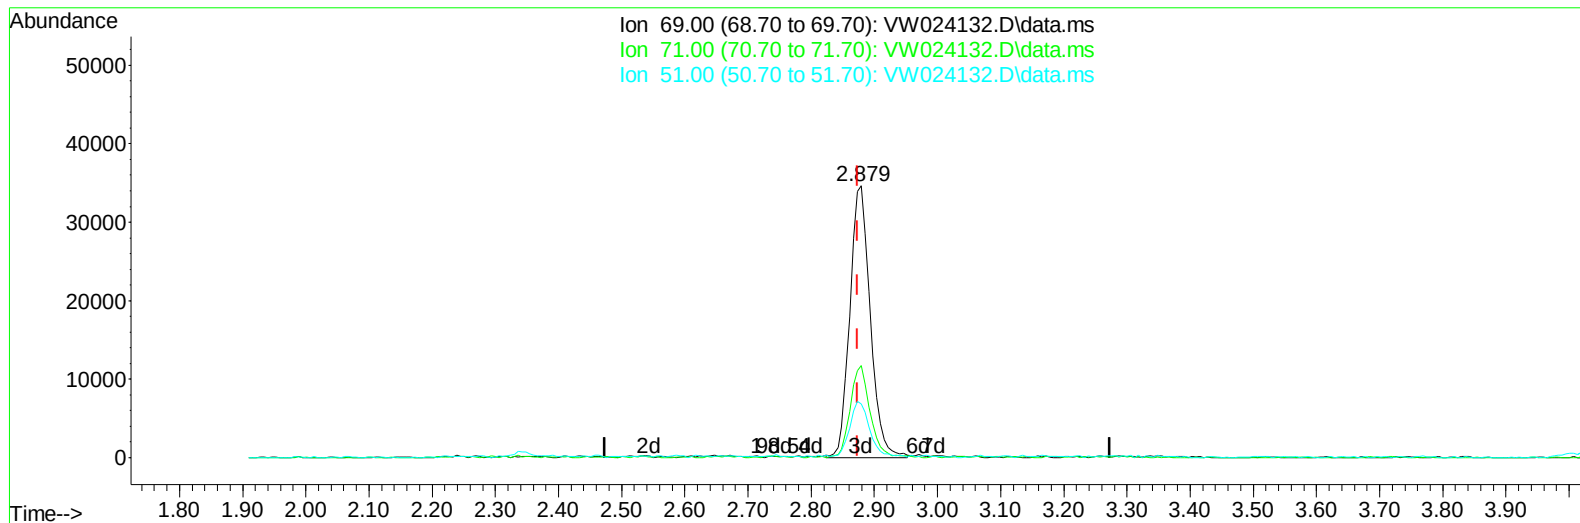

TIC: VW024132.D\data.ms

(7) Chloroethane-d5 (S)

2.879min (+ 0.006) 26.99 ug/L m

response 77259

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.80	0.06#
51.00	27.90	0.10#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
 Data File : VW024132.D
 Acq On : 29 Jul 2022 16:42
 Operator : SY/VA
 Sample : VIBLK522
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK522

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 30 00:12:08 2022
 Response via : Initial Calibration

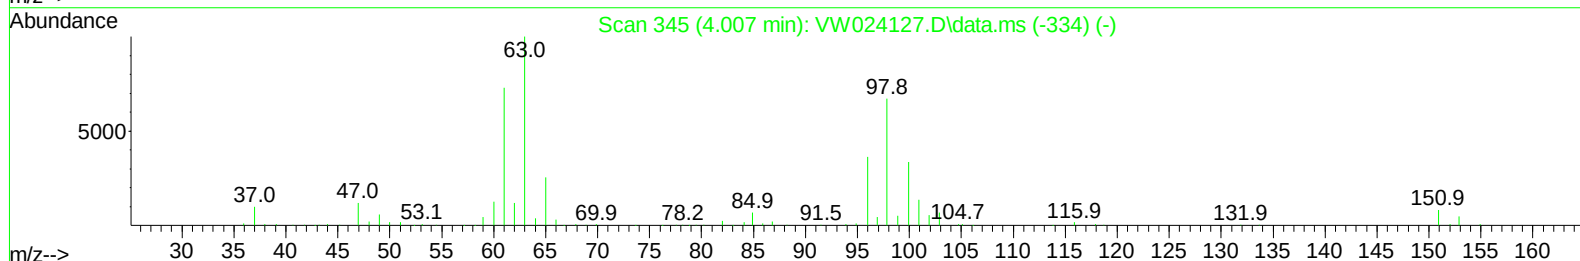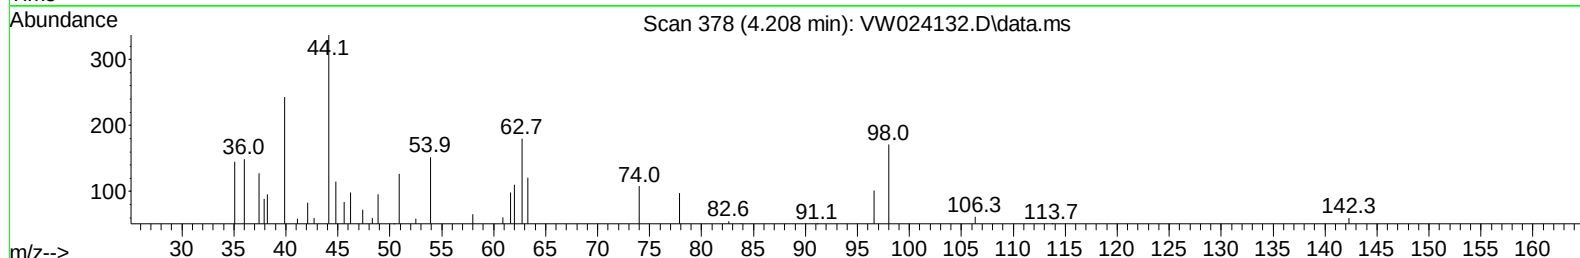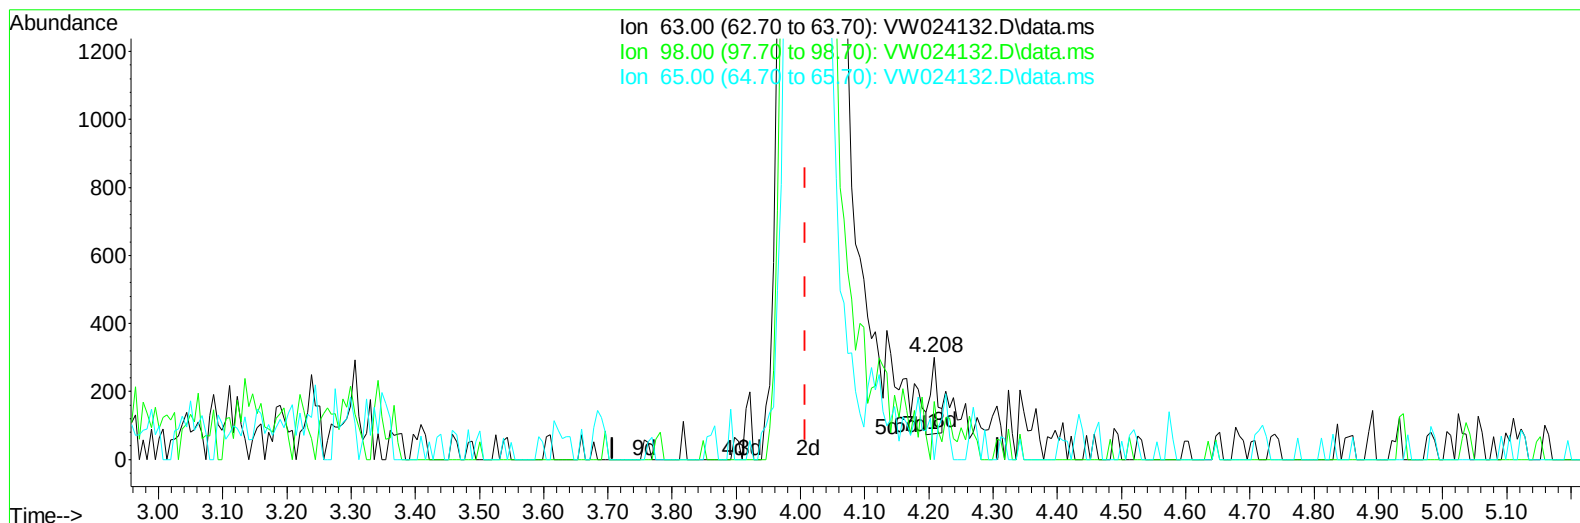

TIC: VW024132.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.208min (+ 0.201) 0.05 ug/L

response 180

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.10	62.22
65.00	23.20	24.44
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
Data File : VW024132.D
Acq On : 29 Jul 2022 16:42
Operator : SY/VA
Sample : VIBLK522
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK522

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 30 00:12:08 2022
Response via : Initial Calibration

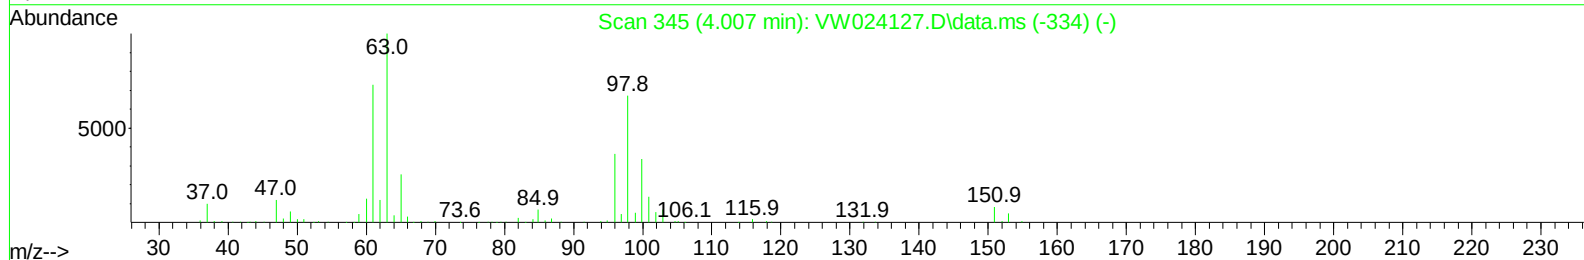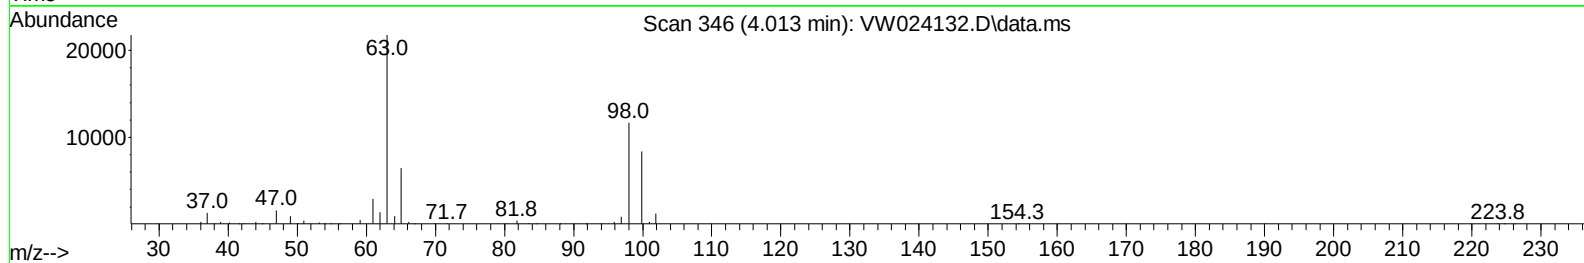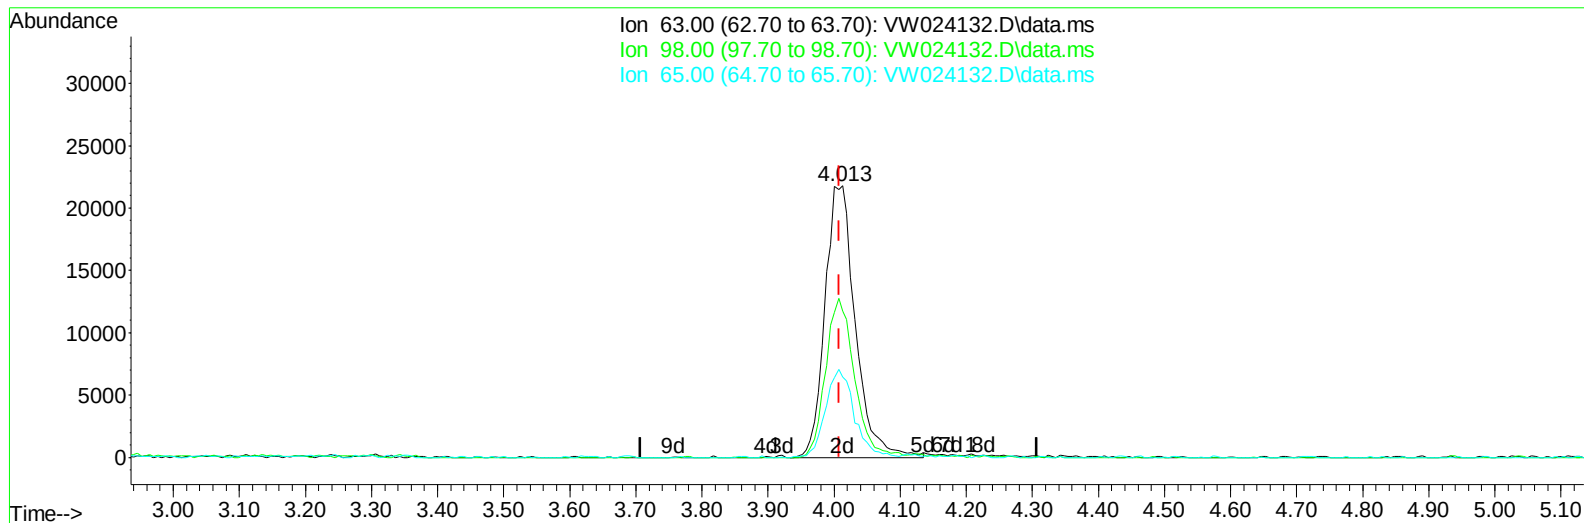

TIC: VW024132.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (+ 0.006) 18.65 ug/L m

response 69572

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.10	0.16#
65.00	23.20	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
 Data File : VW024132.D
 Acq On : 29 Jul 2022 16:42
 Operator : SY/VA
 Sample : VIBLK522
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK522

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
 Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 30 00:12:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	197643	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	194743	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	87046	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.342	65	118715	28.022	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	112.080%	
7) Chloroethane-d5	2.879	69	77259m	26.990	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	107.960%	
11) 1,1-Dichloroethene-d2	4.013	63	69572m	18.650	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	74.600%	
21) 2-Butanone-d5	7.079	46	38899	51.664	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	103.320%	
24) Chloroform-d	7.646	84	134079	24.676	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	98.720%	
26) 1,2-Dichloroethane-d4	8.305	65	80565	25.808	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.240%	
32) Benzene-d6	8.274	84	241289	26.672	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	106.680%	
36) 1,2-Dichloropropane-d6	9.274	67	78354	27.460	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	109.840%	
41) Toluene-d8	10.323	98	223932	24.752	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	99.000%	
43) trans-1,3-Dichloroprop...	10.573	79	31488	24.889	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	99.560%	
47) 2-Hexanone-d5	10.926	63	30965	51.909	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	103.820%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	80056	24.316	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	97.280%	
66) 1,2-Dichlorobenzene-d4	13.852	152	80700	28.627	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	114.520%	
Target Compounds						
16) Methylene chloride	4.909	84	14839	4.933	ug/L	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072922\
Data File : VW024132.D
Acq On : 29 Jul 2022 16:42
Operator : SY/VA
Sample : VIBLK522
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK522

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/01/2022
Supervised By :Mahesh Dadoda 08/01/2022

Quant Time: Jul 30 00:13:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 30 00:12:08 2022
Response via : Initial Calibration

