


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW073018\
Data File : VW004306.D
Acq On : 29 Jul 2018 10:47
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W073018S.M
Title : SW846 8260
Last Update : Mon Jul 30 02:37:04 2018

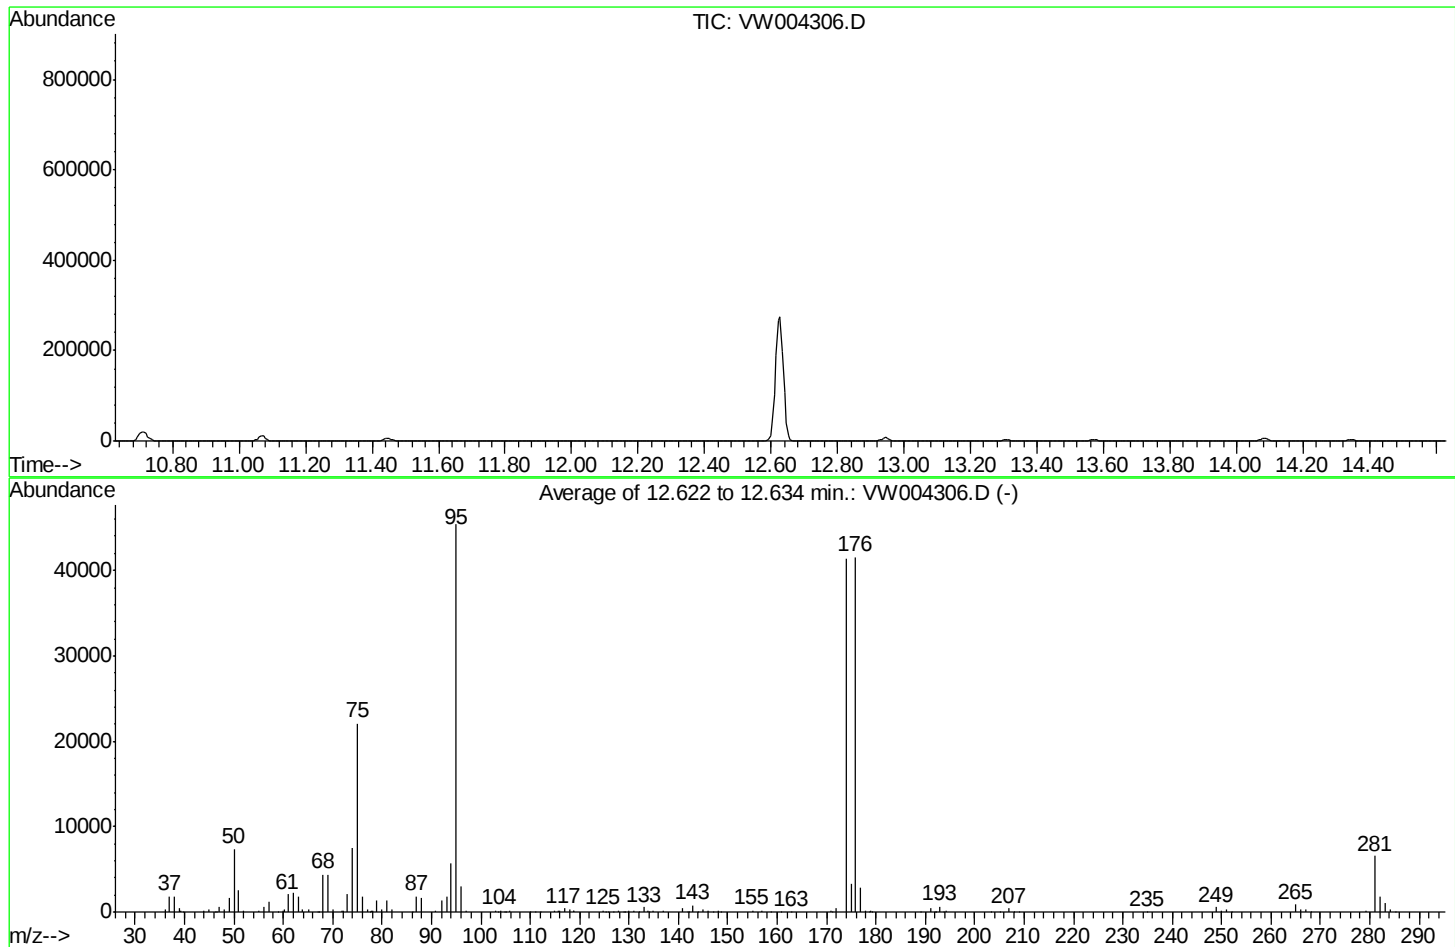

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	7417	PASS
75	95	30	60	48.6	22045	PASS
95	95	100	100	100.0	45397	PASS
96	95	5	9	6.6	2990	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.2	41384	PASS
175	174	5	9	7.9	3290	PASS
176	174	95	101	100.4	41549	PASS
177	176	5	9	7.0	2903	PASS