


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW073018\
 Data File : VW004331.D
 Acq On : 29 Jul 2018 23:51
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W073018S.M
 Title : SW846 8260
 Last Update : Mon Jul 30 02:37:04 2018

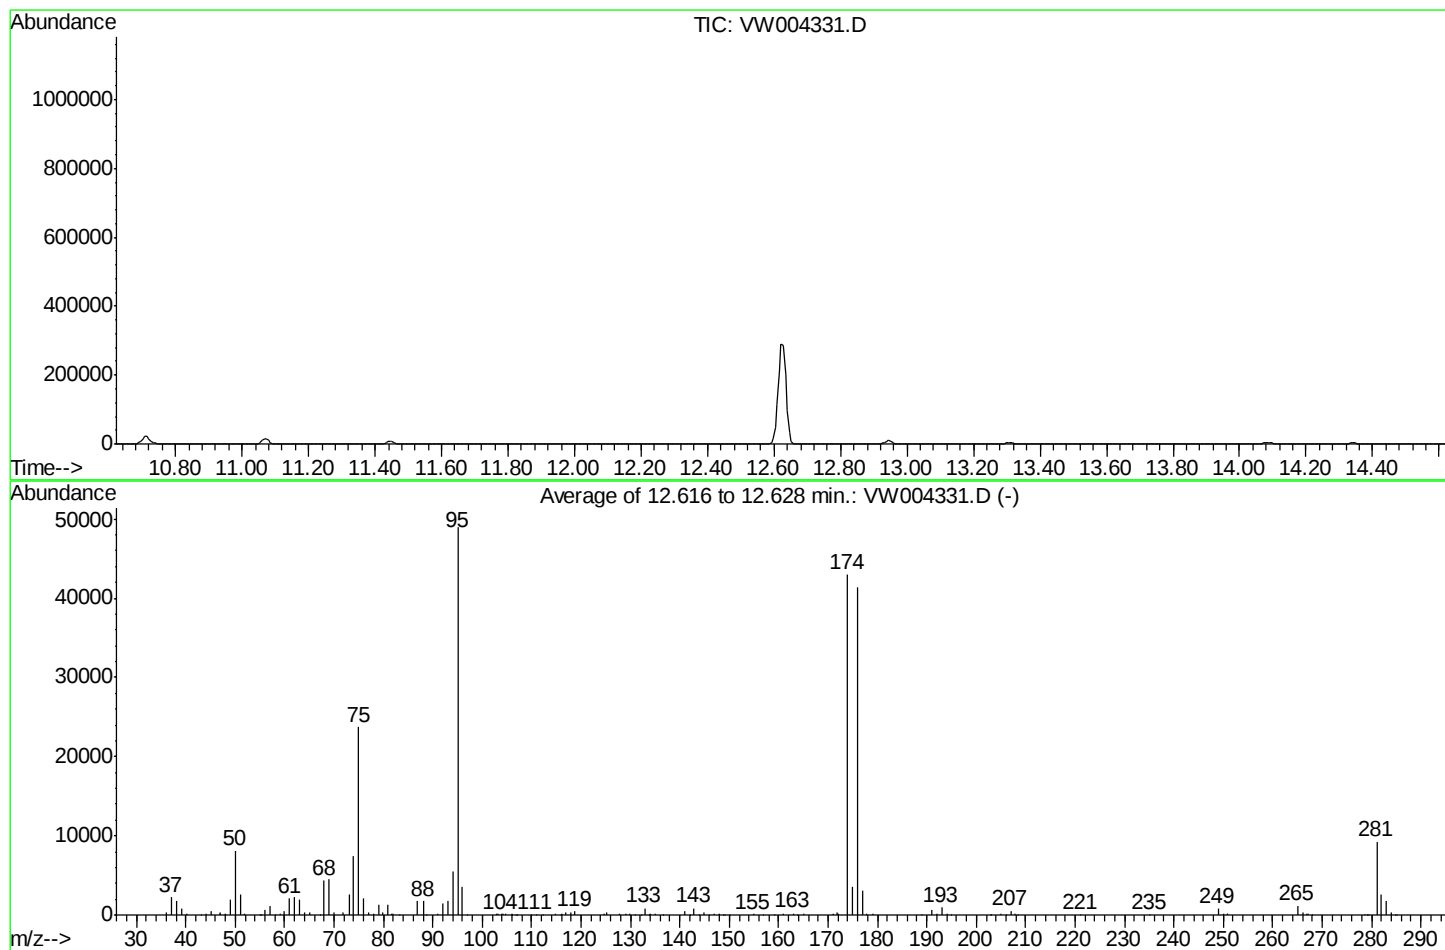

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	8163	PASS
75	95	30	60	48.5	23744	PASS
95	95	100	100	100.0	48946	PASS
96	95	5	9	7.2	3514	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.7	42917	PASS
175	174	5	9	8.3	3551	PASS
176	174	95	101	96.6	41456	PASS
177	176	5	9	7.3	3020	PASS