

Data File : VW011586.D
Acq On : 31 Jul 2019 14:45
Operator : SY/VA
Sample : K4070-18
Misc : 4.99G/10ML/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB9E9

Quant Time: Aug 01 05:23:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 01 05:20:41 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	354469	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	315527	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	136014	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	123580	24.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.04%
7) Chloroethane-d5	2.89	69	91702	25.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.04%
10) 1,1-Dichloroethene-d2	4.02	63	211103	18.45	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.80%
20) 2-Butanone-d5	7.07	46	110572	49.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.40%
24) Chloroform-d	7.65	84	245768	25.25	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.00%
26) 1,2-Dichloroethane-d4	8.31	65	156336	27.14	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	108.56%
29) Benzene-d6	8.27	84	512646	25.84	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.36%
33) 1,2-Dichloropropane-d6	9.27	67	170127	26.56	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.24%
37) Toluene-d8	10.32	98	439452	24.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.80%
38) trans-1,3-Dichloropropene-	10.58	79	68911	24.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.20%
39) 2-Hexanone-d5	10.93	63	73359	49.03	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.06%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	136006	25.57	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.28%
61) 1,2-Dichlorobenzene-d4	13.85	152	136254	26.00	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.00%


Target Compounds					Qvalue
22) cis-1,2-Dichloroethene	7.17	96	24450	4.443 ug/L	99
35) Trichloroethene	9.09	95	15955	2.842 ug/L	99
66) 1,2-Dibromo-3-chloropropan	14.32	75	1161	1.342 ug/L #	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011586.D
Acq On : 31 Jul 2019 14:45
Operator : SY/VA
Sample : K4070-18
Misc : 4.99G/10ML/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB9E9

Quant Time: Aug 01 05:23:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 01 05:20:41 2019
Response via : Initial Calibration

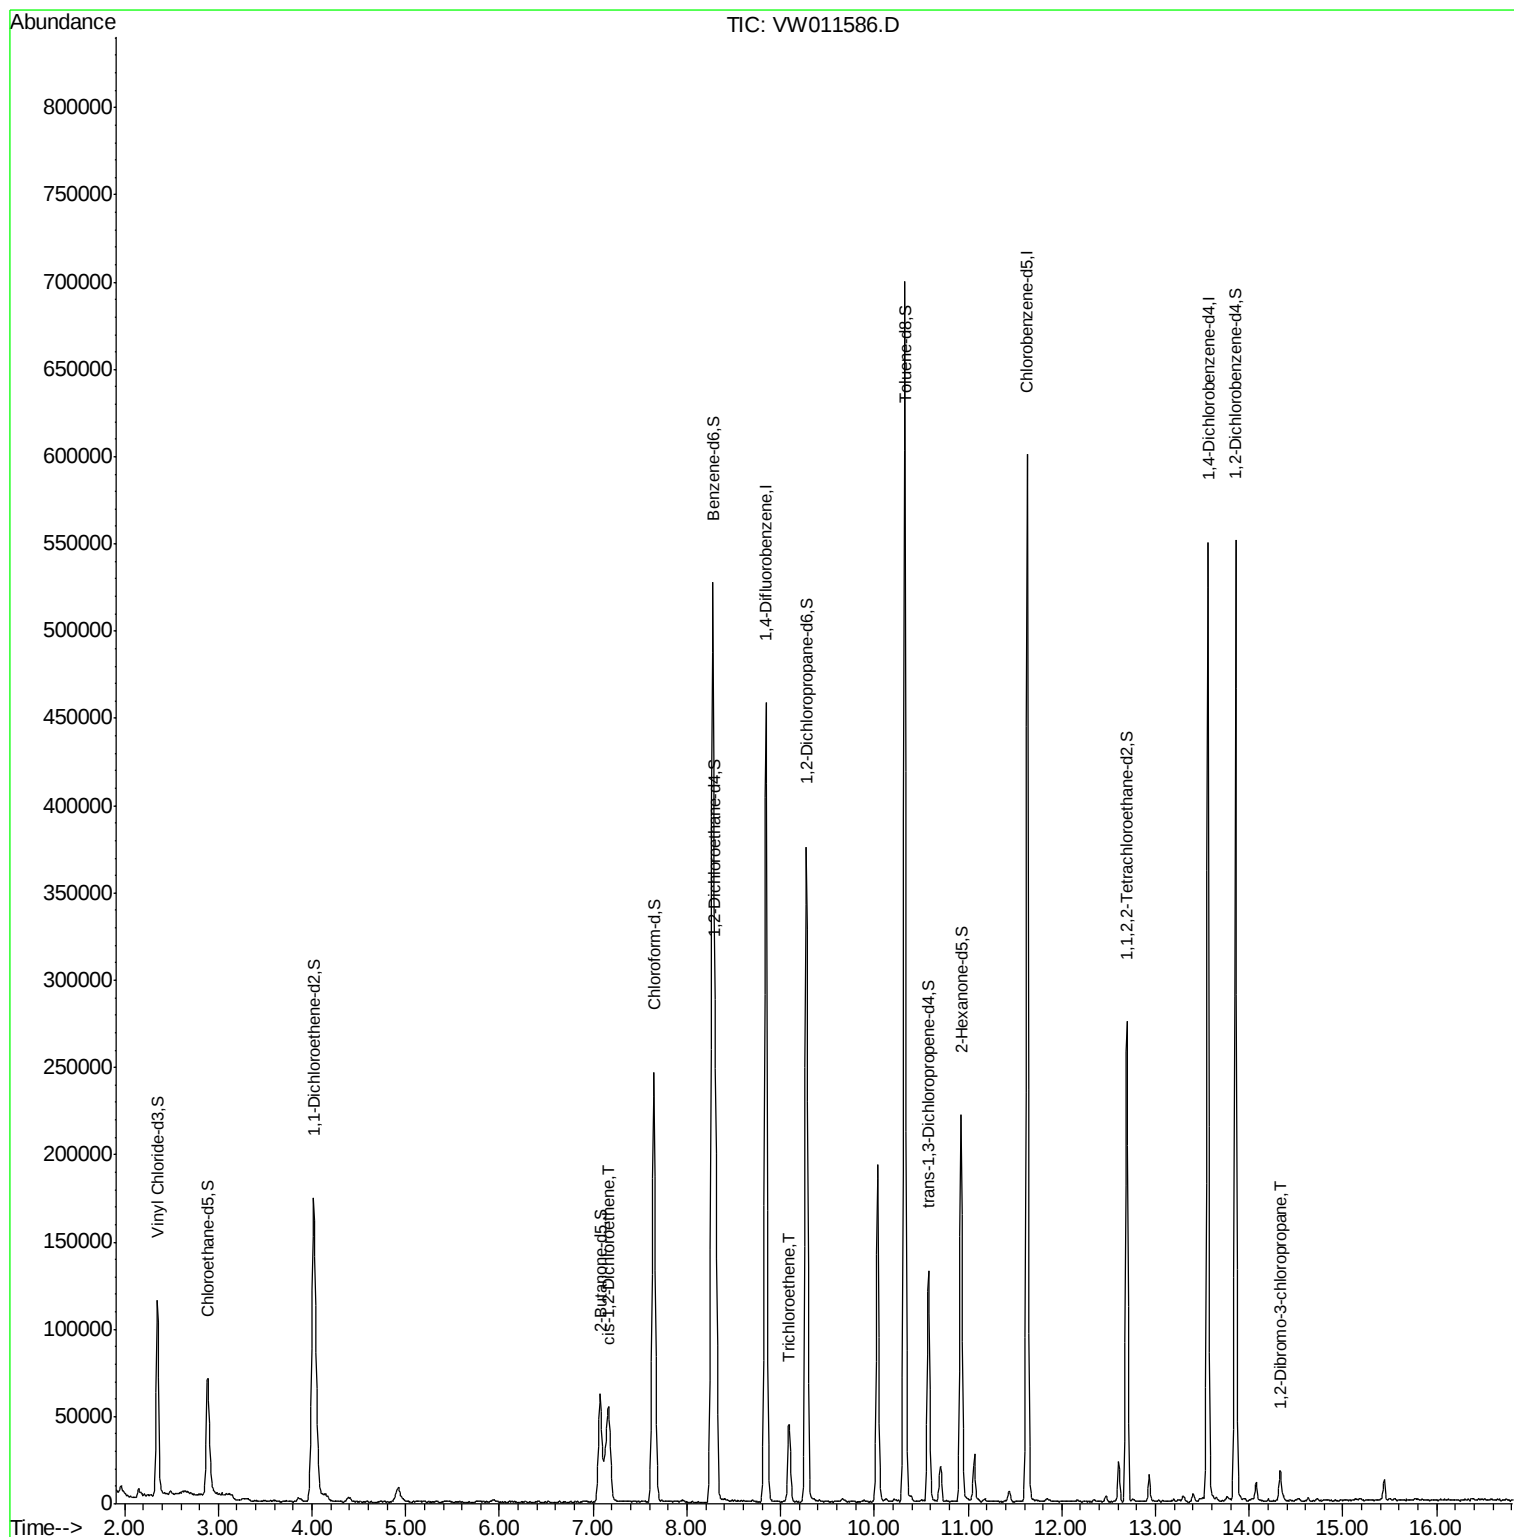




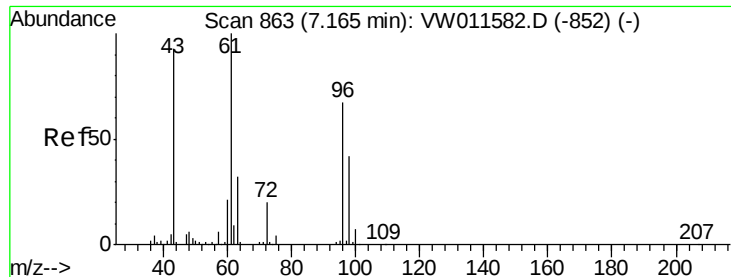


#22

cis-1,2-Dichloroethene
Concen: 4.443 ug/L
RT: 7.17 min Scan# 863
Delta R.T. 0.00 min
Lab File: VW011586.D
Acq: 31 Jul 2019 14:45

Instrument :
MSVOA_W
ClientSampled :
DB9E9




Tgt Ion: 96 Resp: 24450
Ion Ratio Lower Upper
96 100
61 150.4 103.9 192.9
98 63.1 43.5 80.9

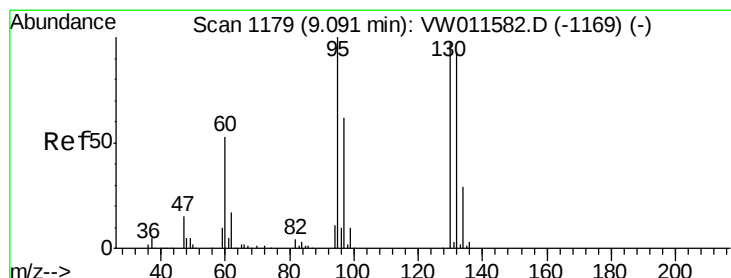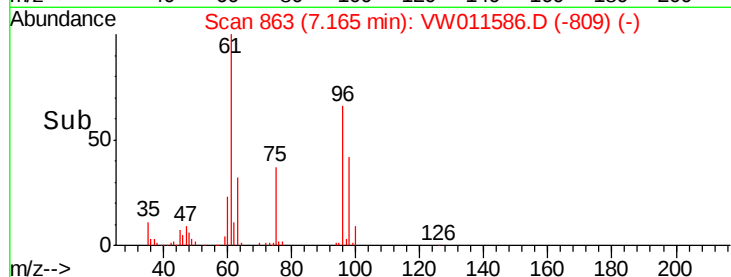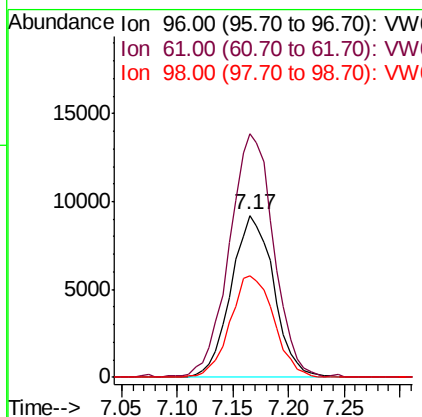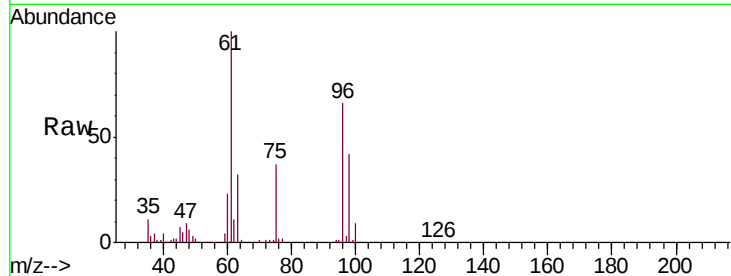


#35

Trichloroethene
Concen: 2.842 ug/L
RT: 9.09 min Scan# 1179
Delta R.T. 0.00 min
Lab File: VW011586.D
Acq: 31 Jul 2019 14:45

Tgt Ion: 95 Resp: 15955
Ion Ratio Lower Upper
95 100
97 64.4 44.8 83.2
132 93.1 65.0 120.6
130 94.4 68.0 126.4

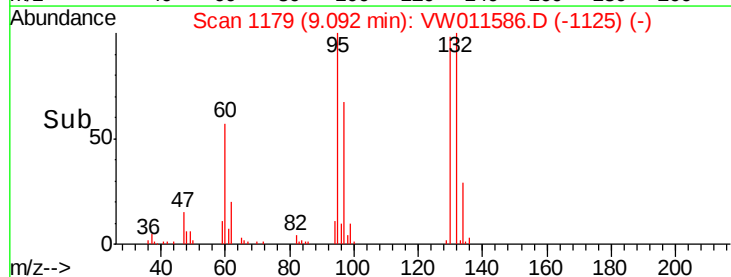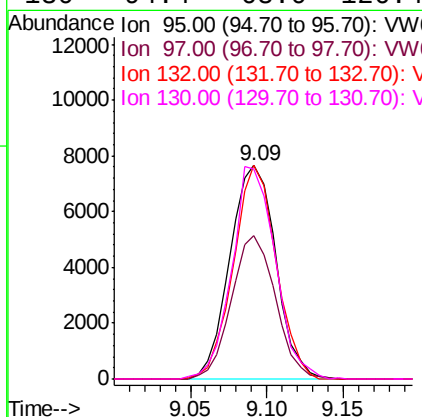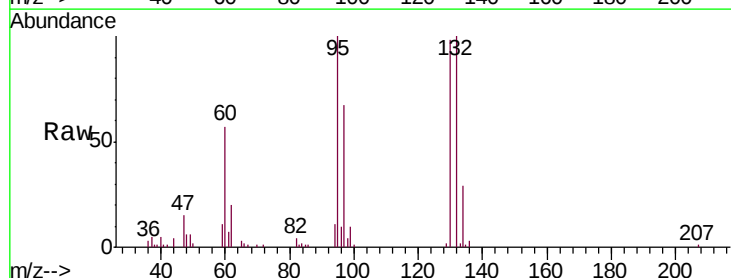

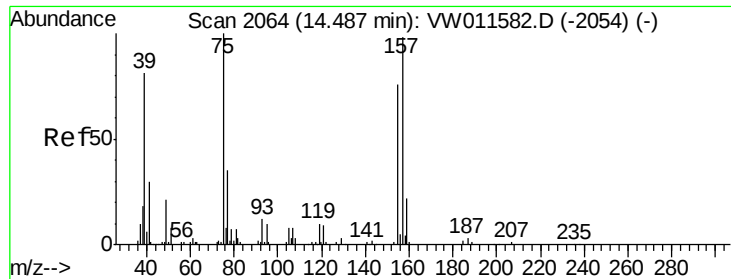

#66

1,2-Dibromo-3-chloropropane

Concen: 1.342 ug/L

RT: 14.32 min Scan# 2037

Delta R.T. -0.16 min

Lab File: VW011586.D

Acq: 31 Jul 2019 14:45

Instrument :

MSVOA_W

ClientSampleId :

DB9E9


Tgt Ion: 75 Resp: 1161

Ion Ratio Lower Upper

75 100

157 0.0 79.3 118.9#

155 0.0 59.9 89.9#

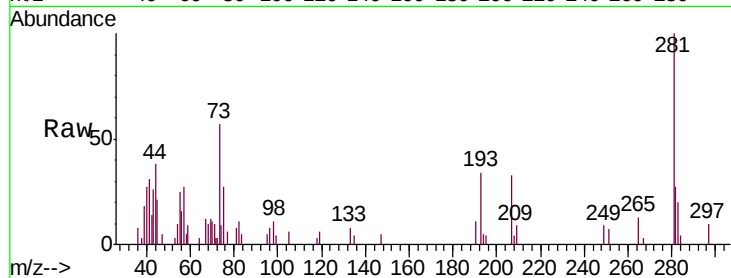

Abundance Ion 75.00 (74.70 to 75.70): VW

Ion 157.00 (156.70 to 157.70): V

Ion 155.00 (154.70 to 155.70): V

