




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW073124\
Data File : VW029812.D
Acq On : 31 Jul 2024 13:56
Operator : SY/MD
Sample : P3397-01
Misc : 3.99g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BHCL0

Manual IntegrationsAPPROVED

Quant Time: Aug 01 04:45:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 01 04:42:41 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/01/2024
Supervised By :Mahesh Dadoda 08/02/2024

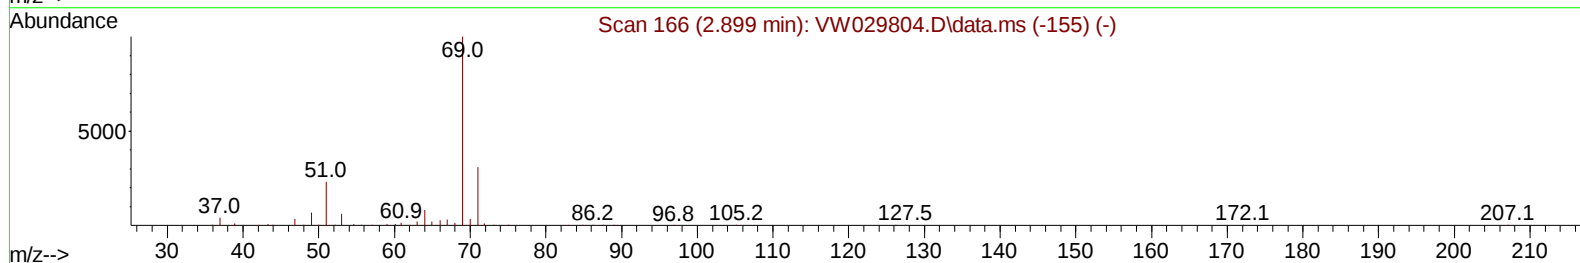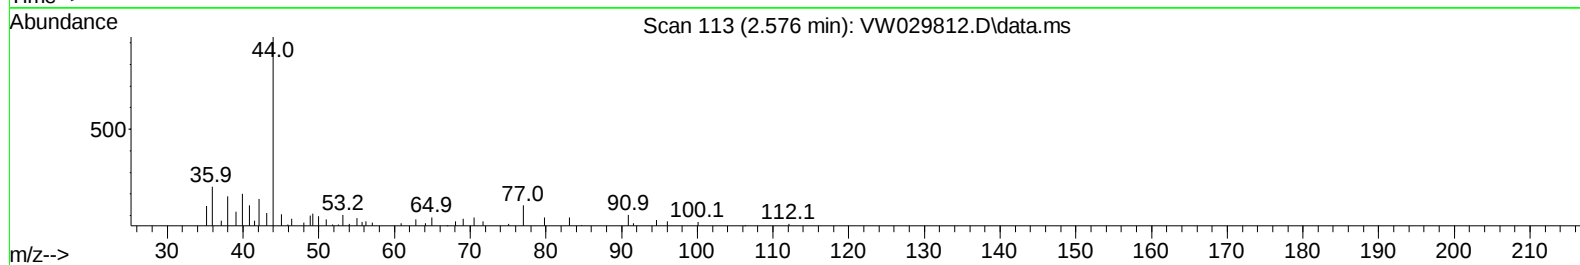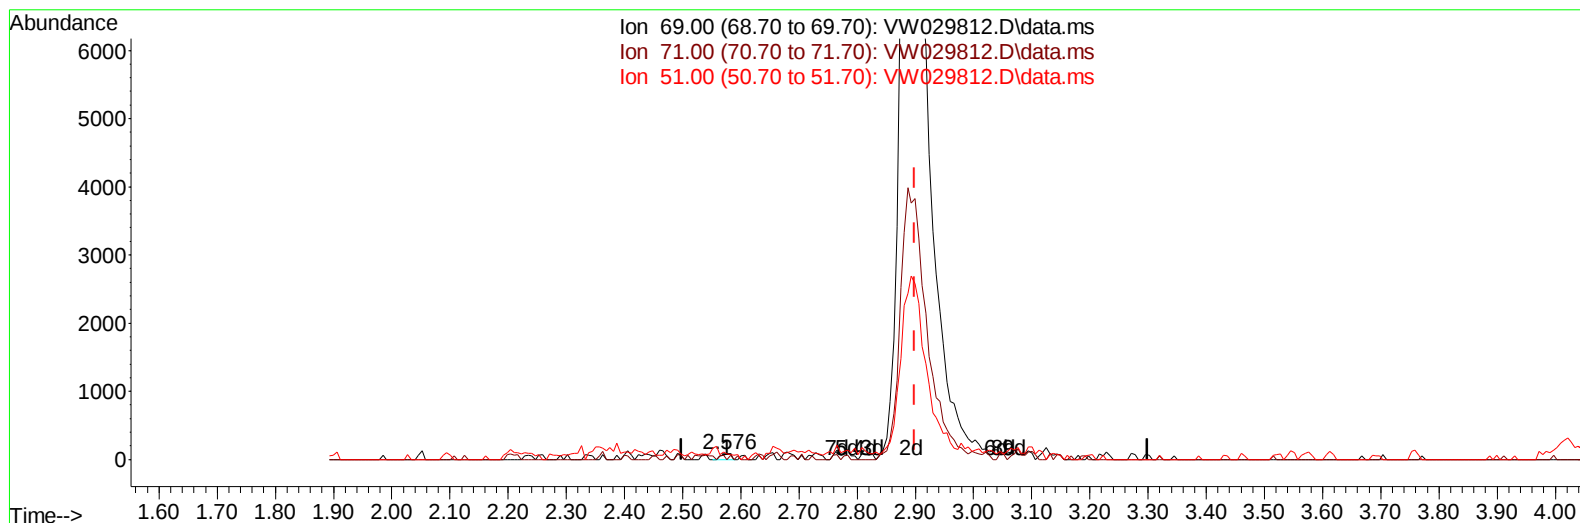

TIC: VW029812.D\data.ms

(7) Chloroethane-d5 (S)

2.576min (-0.323) 0.03 ug/L

response 104

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.70	39.42
51.00	31.60	25.96
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW073124\
 Data File : VW029812.D
 Acq On : 31 Jul 2024 13:56
 Operator : SY/MD
 Sample : P3397-01
 Misc : 3.99g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BHCL0

Manual IntegrationsAPPROVED

Quant Time: Aug 01 04:45:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 01 04:42:41 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/01/2024
 Supervised By :Mahesh Dadoda 08/02/2024

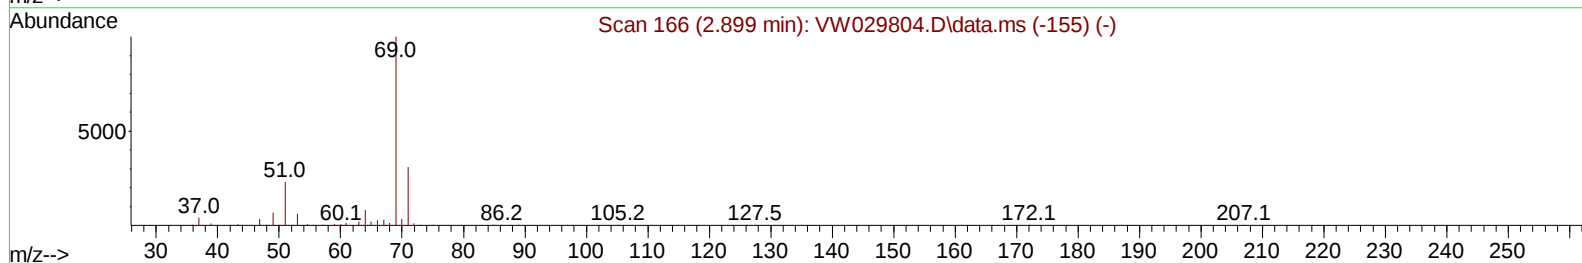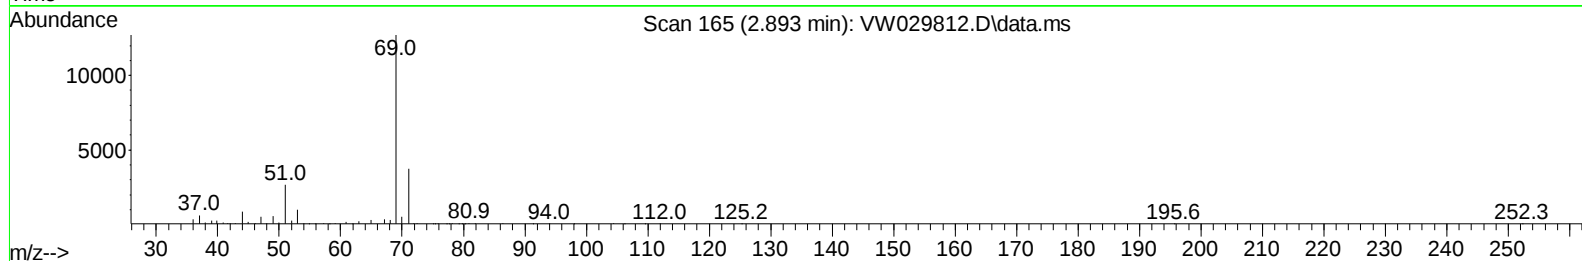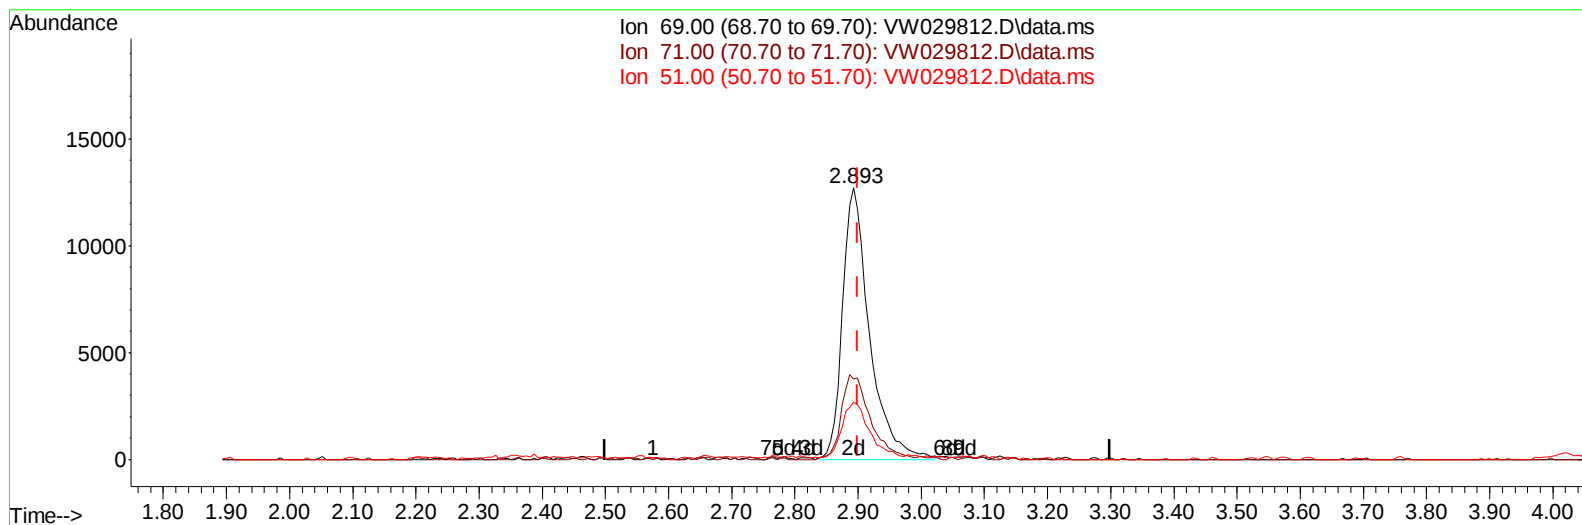

TIC: VW029812.D\data.ms

(7) Chloroethane-d5 (S)

2.893min (-0.006) 11.92 ug/L m

response 37782

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.70	0.11#
51.00	31.60	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW073124\
 Data File : VW029812.D
 Acq On : 31 Jul 2024 13:56
 Operator : SY/MD
 Sample : P3397-01
 Misc : 3.99g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BHCL0

Manual IntegrationsAPPROVED

Quant Time: Aug 01 04:45:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 01 04:42:41 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/01/2024
 Supervised By :Mahesh Dadoda 08/02/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	312711	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	290450	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	127529	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	36019	8.113	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	32.440%	
7) Chloroethane-d5	2.893	69	37782m	11.921	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	47.680%	
11) 1,1-Dichloroethene-d2	4.015	65	19126	9.438	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	37.760%#	
21) 2-Butanone-d5	7.075	46	74969	61.612	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	123.220%	
24) Chloroform-d	7.648	84	150212	18.556	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	74.240%	
26) 1,2-Dichloroethane-d4	8.307	65	95358	20.682	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	82.720%	
32) Benzene-d6	8.270	84	232205	14.796	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	59.200%	
36) 1,2-Dichloropropane-d6	9.270	67	96282	19.214	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	76.840%	
41) Toluene-d8	10.319	98	184598	13.229	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	52.920%	
43) trans-1,3-Dichloroprop...	10.575	79	33917	16.727	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	66.920%	
47) 2-Hexanone-d5	10.922	63	49747	60.206	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.420%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	105678	28.402	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	113.600%	
66) 1,2-Dichlorobenzene-d4	13.849	152	84808	21.417	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	85.680%	
Target Compounds						
16) Methylene chloride	4.917	84	27839	4.258	ug/L	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW073124\
Data File : VW029812.D
Acq On : 31 Jul 2024 13:56
Operator : SY/MD
Sample : P3397-01
Misc : 3.99g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BHCL0

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/01/2024
Supervised By :Mahesh Dadoda 08/02/2024

Quant Time: Aug 01 04:45:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 01 04:42:41 2024
Response via : Initial Calibration

