


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW080118\
 Data File : VW004367.D
 Acq On : 01 Aug 2018 09:34
 Operator : SY/AP
 Sample : BFB90
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB90

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073118S.M
 Title : VOC Analysis
 Last Update : Thu Aug 02 05:11:26 2018

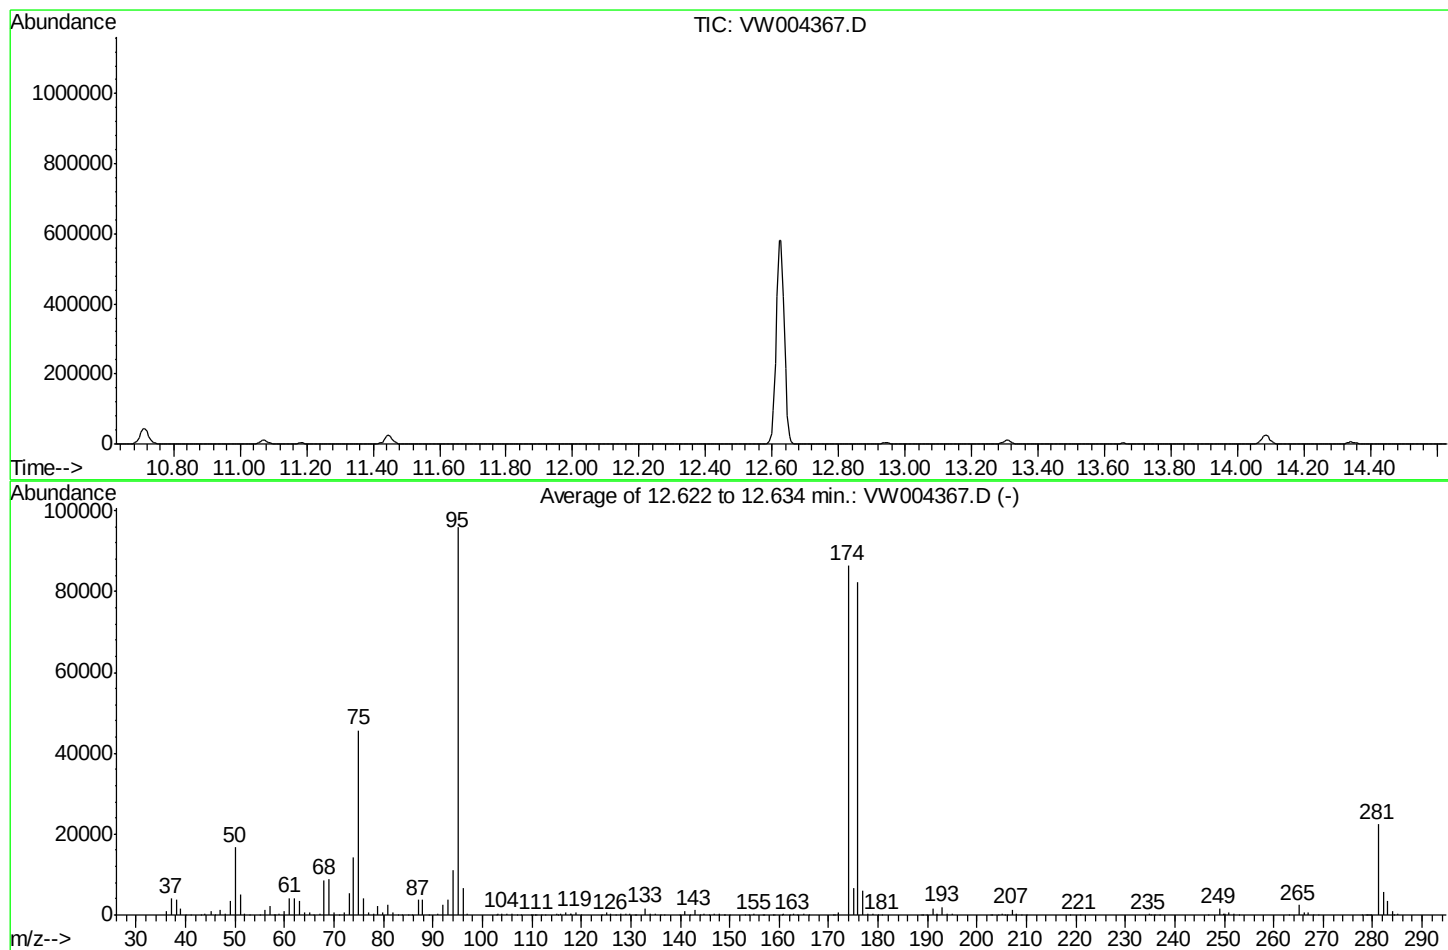

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	16732	PASS
75	95	30	80	47.7	45728	PASS
95	95	100	100	100.0	95890	PASS
96	95	5	9	6.8	6527	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.1	86434	PASS
175	174	5	9	7.7	6623	PASS
176	174	95	101	95.4	82426	PASS
177	176	5	9	7.5	6155	PASS

Scan 1802 (12.573 min): VW004367.D
BFB90

m/z	Abundance
39.00	74.0
39.90	111.0
41.00	62.0
43.90	181.0
55.10	113.0
207.00	104.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

m/z	Abundance
36.00	912.0
37.00	4807.0
38.10	4326.0
39.00	2035.0
40.00	239.0
41.00	63.0
42.90	203.0
43.90	688.0
45.00	1184.0
46.00	176.0
47.00	1197.0
48.00	538.0
49.00	3885.0
50.00	19480.0
51.00	5614.0
52.00	247.0
53.00	94.0
55.00	299.0
56.00	1329.0
57.00	2679.0
58.20	86.0
59.00	327.0
60.00	997.0
61.00	5040.0
62.00	4778.0
63.00	4048.0
64.00	717.0
65.00	780.0
65.80	102.0
67.10	343.0
68.00	9448.0
69.00	10214.0
70.00	950.0
72.00	765.0
73.00	6487.0
74.00	15732.0
75.00	50208.0
76.00	4757.0
76.90	802.0
77.90	411.0
78.90	2550.0
80.00	781.0
80.90	2890.0
81.90	721.0
83.00	90.0
83.80	58.0
85.10	74.0
85.90	168.0
86.90	4326.0
87.90	4028.0
90.90	390.0
92.00	2716.0
92.90	3977.0
94.00	11806.0
95.00	102912.0
96.00	7265.0
96.90	283.0
102.90	474.0
103.90	510.0
104.90	279.0
105.80	466.0
106.90	103.0
107.90	51.0
109.70	175.0
110.10	194.0
111.10	267.0
111.90	286.0
112.70	102.0
114.90	312.0
115.90	374.0
116.90	772.0
117.80	684.0
119.00	871.0
120.00	71.0
124.10	91.0
125.10	1184.0
126.10	199.0
126.80	79.0
128.00	334.0
128.90	302.0
129.90	321.0
130.80	308.0
133.00	2656.0
134.80	377.0
135.90	55.0
136.80	146.0
140.90	969.0
142.10	94.0
142.80	1160.0
144.00	110.0
144.90	505.0
145.80	175.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

146.90	372.0
147.90	325.0
148.80	345.0
153.90	88.0
154.90	247.0
156.60	72.0
158.80	250.0
160.70	255.0
162.10	90.0
162.90	407.0
163.80	132.0
164.80	217.0
165.90	78.0
170.90	316.0
171.90	726.0
173.90	87824.0
174.90	6540.0
175.90	82864.0
177.00	6590.0
177.90	378.0
179.00	631.0
179.90	202.0
180.80	71.0
188.80	262.0
189.90	122.0
191.00	2234.0
191.80	466.0
193.00	2927.0
194.00	494.0
195.00	294.0
203.00	219.0
204.20	89.0
205.00	654.0
206.10	206.0
207.10	1975.0
208.00	425.0
209.00	157.0
218.80	99.0
220.90	128.0
234.80	232.0
236.00	57.0
236.80	83.0
246.80	85.0
249.00	2099.0
250.10	545.0
251.00	1045.0
252.00	206.0
252.90	183.0
263.10	55.0
265.00	3522.0
266.10	1035.0
267.00	1070.0
268.00	253.0
268.90	77.0
277.70	62.0
279.20	296.0
281.10	29808.0
282.10	7571.0
283.10	4855.0
284.00	1144.0
285.00	415.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

m/z	Abundance
36.00	831.0
37.00	4106.0
38.00	4180.0
39.10	1719.0
40.10	193.0
41.00	87.0
42.90	92.0
44.00	608.0
45.10	936.0
46.80	1227.0
47.90	556.0
49.00	3896.0
50.00	18600.0
51.00	5738.0
51.90	258.0
52.90	101.0
54.90	181.0
56.00	1351.0
57.00	2564.0
57.90	148.0
58.90	219.0
60.00	932.0
61.00	4536.0
62.00	4431.0
63.00	3902.0
64.00	518.0
65.00	545.0
65.80	78.0
67.00	394.0
68.00	9285.0
69.00	9903.0
70.00	744.0
71.90	600.0
73.00	5683.0
74.00	16157.0
75.00	51264.0
76.00	4611.0
76.90	643.0
77.90	516.0
78.90	2492.0
79.90	681.0
80.90	2419.0
81.90	605.0
82.90	138.0
85.90	75.0
87.00	4013.0
87.90	4096.0
90.90	319.0
92.00	3040.0
93.00	4493.0
94.00	12272.0
95.00	106840.0
96.00	7444.0
96.90	222.0
103.10	494.0
104.00	422.0
104.90	152.0
105.90	379.0
106.80	73.0
109.90	195.0
110.90	184.0
112.00	81.0
112.70	99.0
115.00	200.0
115.80	458.0
116.90	773.0
118.00	695.0
118.90	874.0
125.00	668.0
125.90	193.0
127.90	363.0
129.00	182.0
129.90	465.0
131.00	167.0
133.00	1534.0
133.90	376.0
134.90	271.0
135.90	78.0
136.90	191.0
139.80	91.0
140.90	1023.0
141.90	185.0
142.90	1553.0
144.00	99.0
144.90	490.0
145.80	117.0
146.80	333.0
147.80	318.0
149.00	204.0
149.80	192.0
153.10	71.0
154.90	228.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

156.70	126.0
159.00	123.0
160.90	300.0
161.90	61.0
162.90	303.0
164.90	276.0
171.10	252.0
172.10	831.0
173.90	96232.0
175.00	7553.0
175.90	91680.0
176.90	6833.0
178.00	365.0
179.00	501.0
179.80	64.0
180.80	64.0
189.00	228.0
189.90	77.0
191.00	1666.0
192.00	313.0
193.00	1985.0
193.90	441.0
195.00	330.0
203.10	121.0
205.10	400.0
206.00	111.0
207.10	1527.0
208.00	411.0
209.00	233.0
210.00	57.0
220.80	124.0
234.80	290.0
249.00	1671.0
249.80	450.0
251.00	707.0
252.00	168.0
252.80	86.0
265.10	2577.0
266.00	699.0
267.10	632.0
268.10	166.0
278.50	113.0
279.40	199.0
281.10	23856.0
282.10	6097.0
283.10	3777.0
284.00	920.0
284.90	292.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

m/z	Abundance
36.00	682.0
37.00	3189.0
38.00	2926.0
39.00	1267.0
39.90	169.0
41.10	77.0
43.00	106.0
44.00	638.0
45.00	570.0
45.90	51.0
47.00	995.0
48.00	362.0
49.00	2476.0
50.00	12116.0
51.00	3586.0
52.10	145.0
52.90	70.0
55.00	185.0
55.90	800.0
57.00	1763.0
57.90	63.0
58.20	91.0
59.00	108.0
60.10	565.0
61.00	3189.0
62.00	3064.0
63.00	2552.0
64.00	346.0
64.90	297.0
67.20	287.0
68.00	6946.0
69.00	6767.0
70.10	518.0
70.90	71.0
72.00	349.0
73.00	3702.0
74.00	10922.0
75.00	35712.0
76.00	3169.0
76.90	306.0
77.80	275.0
78.90	1814.0
79.90	562.0
80.90	1909.0
81.90	524.0
82.90	78.0
85.90	65.0
87.00	3027.0
87.90	2853.0
89.10	62.0
90.80	255.0
92.00	2259.0
93.00	3334.0
94.00	8752.0
95.00	77920.0
96.00	4872.0
97.00	141.0
103.20	151.0
103.90	373.0
105.00	144.0
105.90	313.0
107.00	93.0
109.80	112.0
110.70	68.0
111.90	85.0
114.80	141.0
115.20	101.0
116.00	317.0
116.80	670.0
117.90	392.0
118.80	537.0
125.00	233.0
125.80	128.0
127.80	264.0
128.90	159.0
129.90	302.0
130.80	202.0
132.90	1047.0
134.00	197.0
135.00	160.0
136.90	133.0
139.80	98.0
140.90	817.0
141.90	101.0
142.90	988.0
145.00	298.0
145.80	97.0
146.90	133.0
147.80	253.0
149.00	82.0
149.90	113.0
152.90	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

153.90	60.0
154.90	165.0
156.90	173.0
158.90	123.0
160.90	240.0
162.80	142.0
165.00	75.0
170.90	193.0
172.00	741.0
173.90	75248.0
175.00	5776.0
175.90	72736.0
177.00	5043.0
178.00	299.0
178.90	233.0
188.80	97.0
191.00	813.0
191.90	209.0
192.00	209.0
192.90	1074.0
193.90	256.0
194.90	135.0
202.70	137.0
205.10	292.0
205.70	100.0
207.00	743.0
208.00	234.0
209.00	86.0
220.90	74.0
235.10	96.0
249.00	821.0
249.90	215.0
251.00	498.0
252.00	162.0
265.00	1395.0
266.10	572.0
267.00	311.0
278.80	99.0
279.70	191.0
281.10	13699.0
282.00	3002.0
283.00	2008.0
283.90	411.0
284.20	378.0
285.10	119.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90