

Data File : VW011605.D
Acq On : 01 Aug 2019 17:35
Operator : SY/VA
Sample : K4116-03
Misc : 4.85G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JLLD2

Quant Time: Aug 02 04:34:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 02 04:30:25 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	243164	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	192999	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	71345	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	90219	26.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.40%
7) Chloroethane-d5	2.88	69	66773	27.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.28%
10) 1,1-Dichloroethene-d2	4.02	63	150112	19.12	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.48%
20) 2-Butanone-d5	7.07	46	87770	56.93	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.86%
24) Chloroform-d	7.65	84	176524	26.43	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	105.72%
26) 1,2-Dichloroethane-d4	8.30	65	116645	29.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	118.04%
29) Benzene-d6	8.27	84	351779	28.98	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	115.92%
33) 1,2-Dichloropropane-d6	9.27	67	120800	30.83	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	123.32%#
37) Toluene-d8	10.32	98	281404	26.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.48%
38) trans-1,3-Dichloropropene-	10.58	79	44759	26.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	104.28%
39) 2-Hexanone-d5	10.93	63	57778	63.14	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.28%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	93663	28.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	115.16%
61) 1,2-Dichlorobenzene-d4	13.85	152	71383	25.96	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.84%


Target Compounds					Qvalue
13) Acetone	4.12	43	5617	3.402 ug/L	94
40) 1,2-Dichloropropane	9.27	63	13442	3.723 ug/L #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011605.D
Acq On : 01 Aug 2019 17:35
Operator : SY/VA
Sample : K4116-03
Misc : 4.85G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JLLD2

Quant Time: Aug 02 04:34:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 02 04:30:25 2019
Response via : Initial Calibration

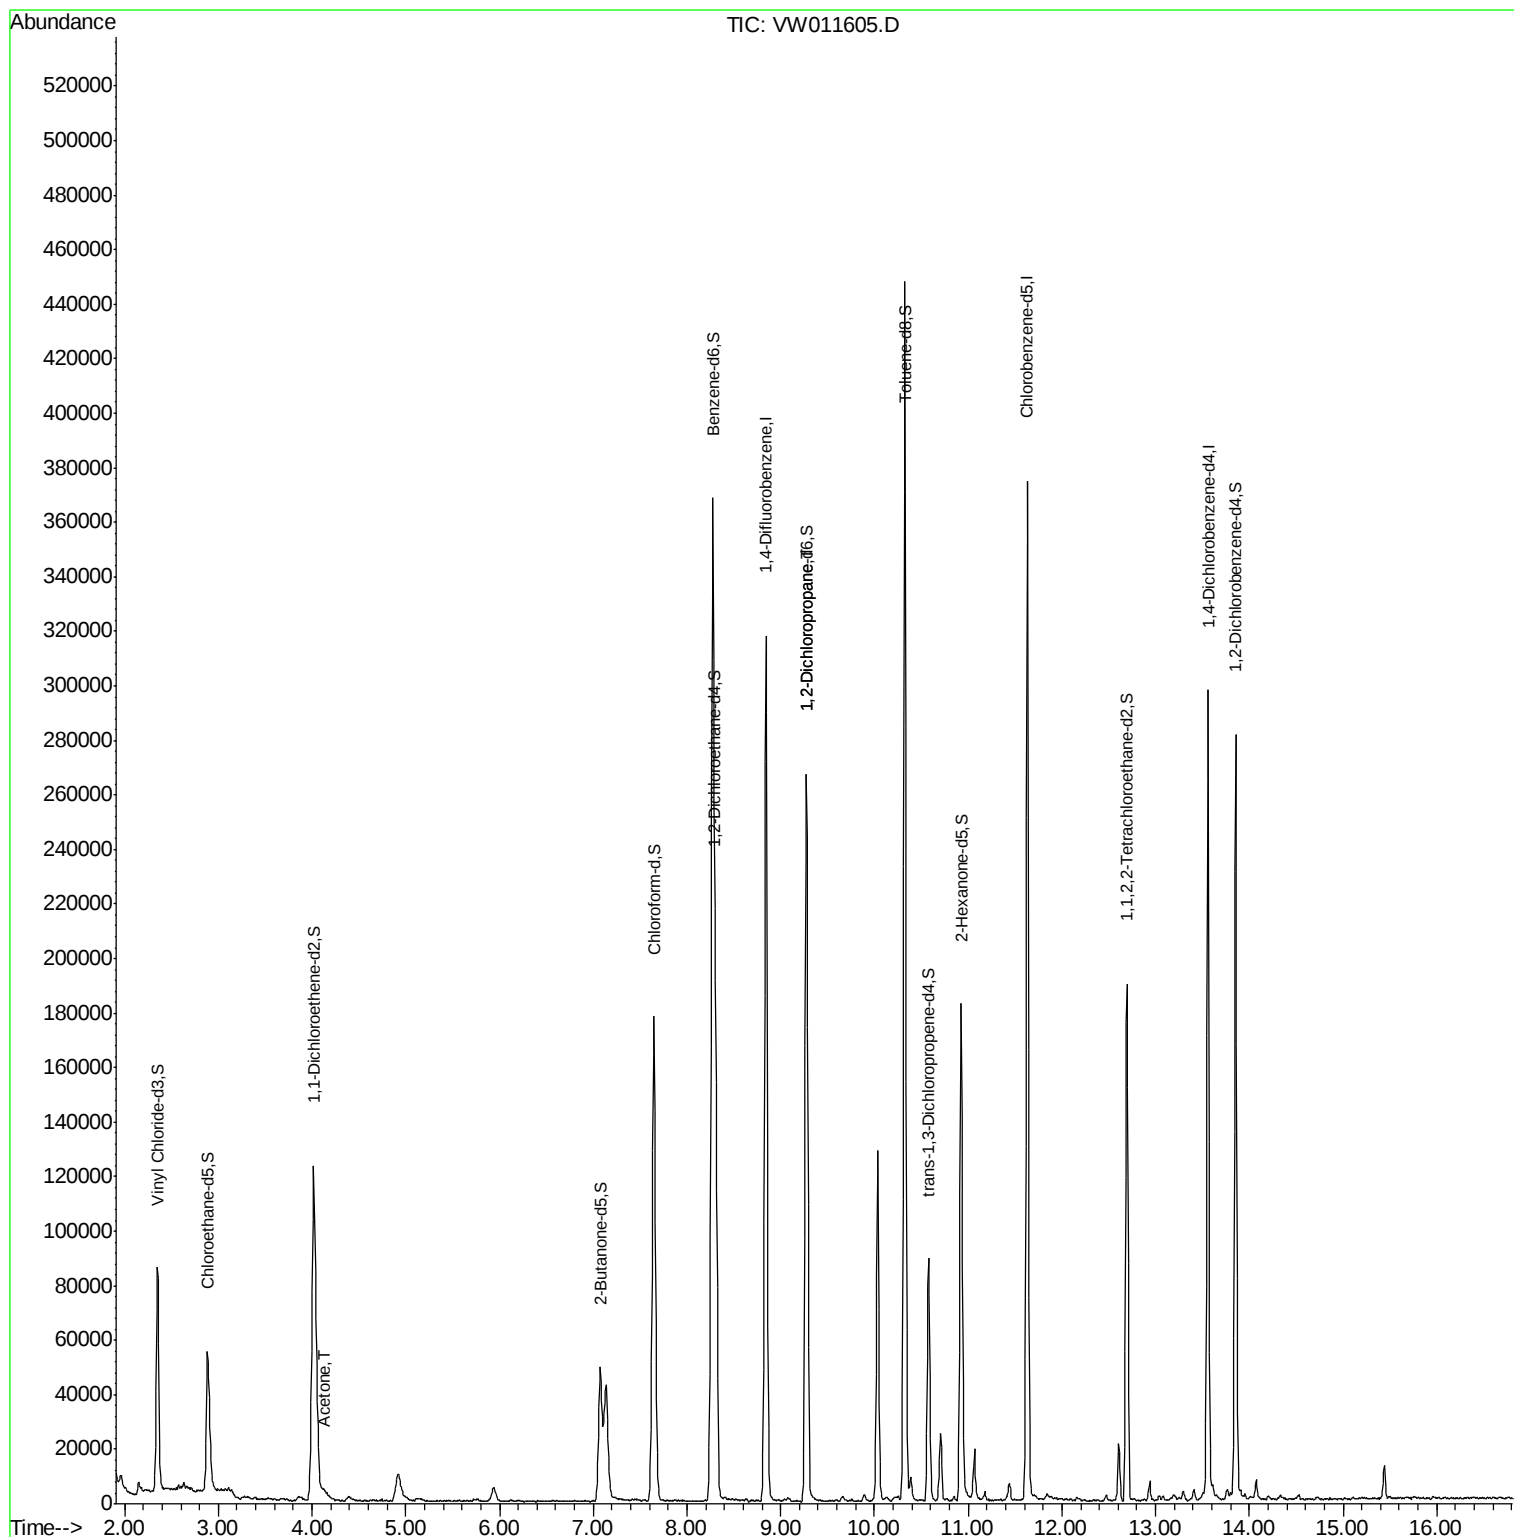

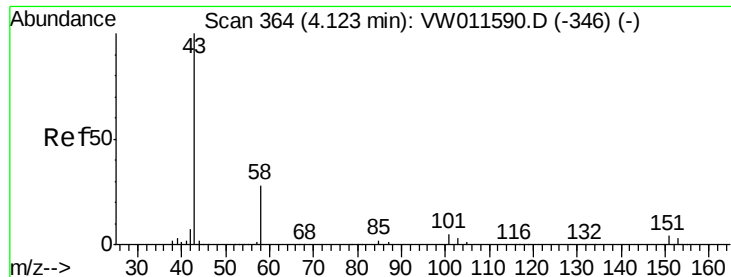

#13

Acetone

Concen: 3.402 ug/L

RT: 4.12 min Scan# 364

Delta R.T. -0.00 min

Lab File: VW011605.D

Acq: 01 Aug 2019 17:35

Instrument :

MSVOA_W

ClientSampleId :





JLLD2

Tgt Ion: 43 Resp: 5617

Ion Ratio Lower Upper

43 100

58 29.8 0.0 53.4

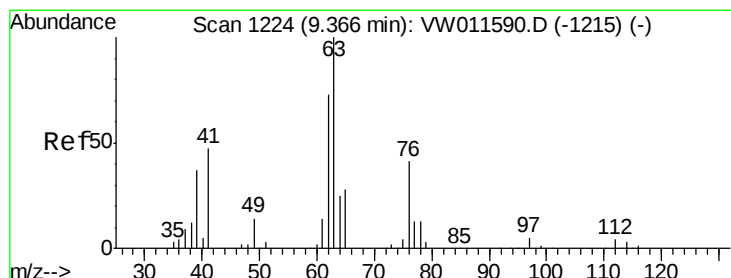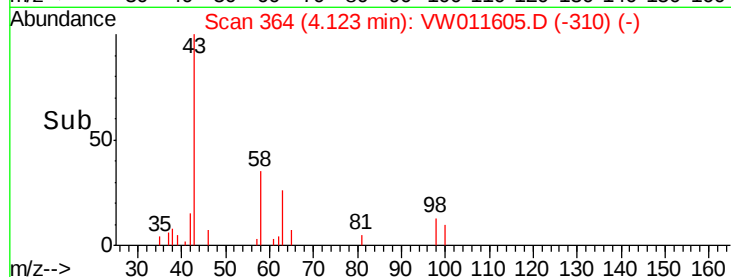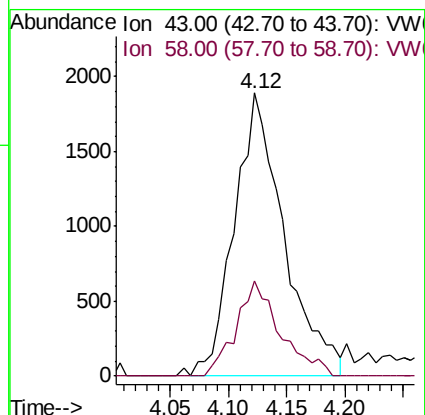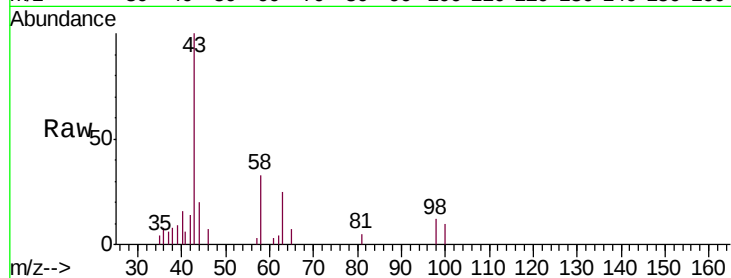

#40

1,2-Dichloropropane

Concen: 3.723 ug/L

RT: 9.27 min Scan# 1209

Delta R.T. -0.09 min

Lab File: VW011605.D

Acq: 01 Aug 2019 17:35

Tgt Ion: 63 Resp: 13442

Ion Ratio Lower Upper

63 100

112 0.0 3.1 4.7#

