

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
 Data File : VW029824.D
 Acq On : 01 Aug 2024 11:25
 Operator : SY/MD
 Sample : P3382-04
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Aug 02 01:46:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 02 01:45:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	242148	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	230572	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	103337	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	53758	15.638	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.560%
7) Chloroethane-d5	2.893	69	45265	18.443	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.760%
11) 1,1-Dichloroethene-d2	4.021	65	26177	16.681	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.720%
21) 2-Butanone-d5	7.081	46	40318	42.790	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.580%
24) Chloroform-d	7.648	84	139628	22.275	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.080%
26) 1,2-Dichloroethane-d4	8.306	65	83639	23.426	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.720%
32) Benzene-d6	8.276	84	259073	20.795	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.200%
36) 1,2-Dichloropropane-d6	9.276	67	87100	21.895	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.600%
41) Toluene-d8	10.324	98	226965	20.489	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.960%
43) trans-1,3-Dichloroprop...	10.574	79	32280	20.054	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.200%
47) 2-Hexanone-d5	10.922	63	26841	40.920	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.840%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	68602	23.226	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.920%
66) 1,2-Dichlorobenzene-d4	13.848	152	75503	23.531	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.120%
Target Compounds						
39) cis-1,3-Dichloropropene	10.026	75	2544	0.403	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
Data File : VW029824.D
Acq On : 01 Aug 2024 11:25
Operator : SY/MD
Sample : P3382-04
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Aug 02 01:46:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 02 01:45:39 2024
Response via : Initial Calibration

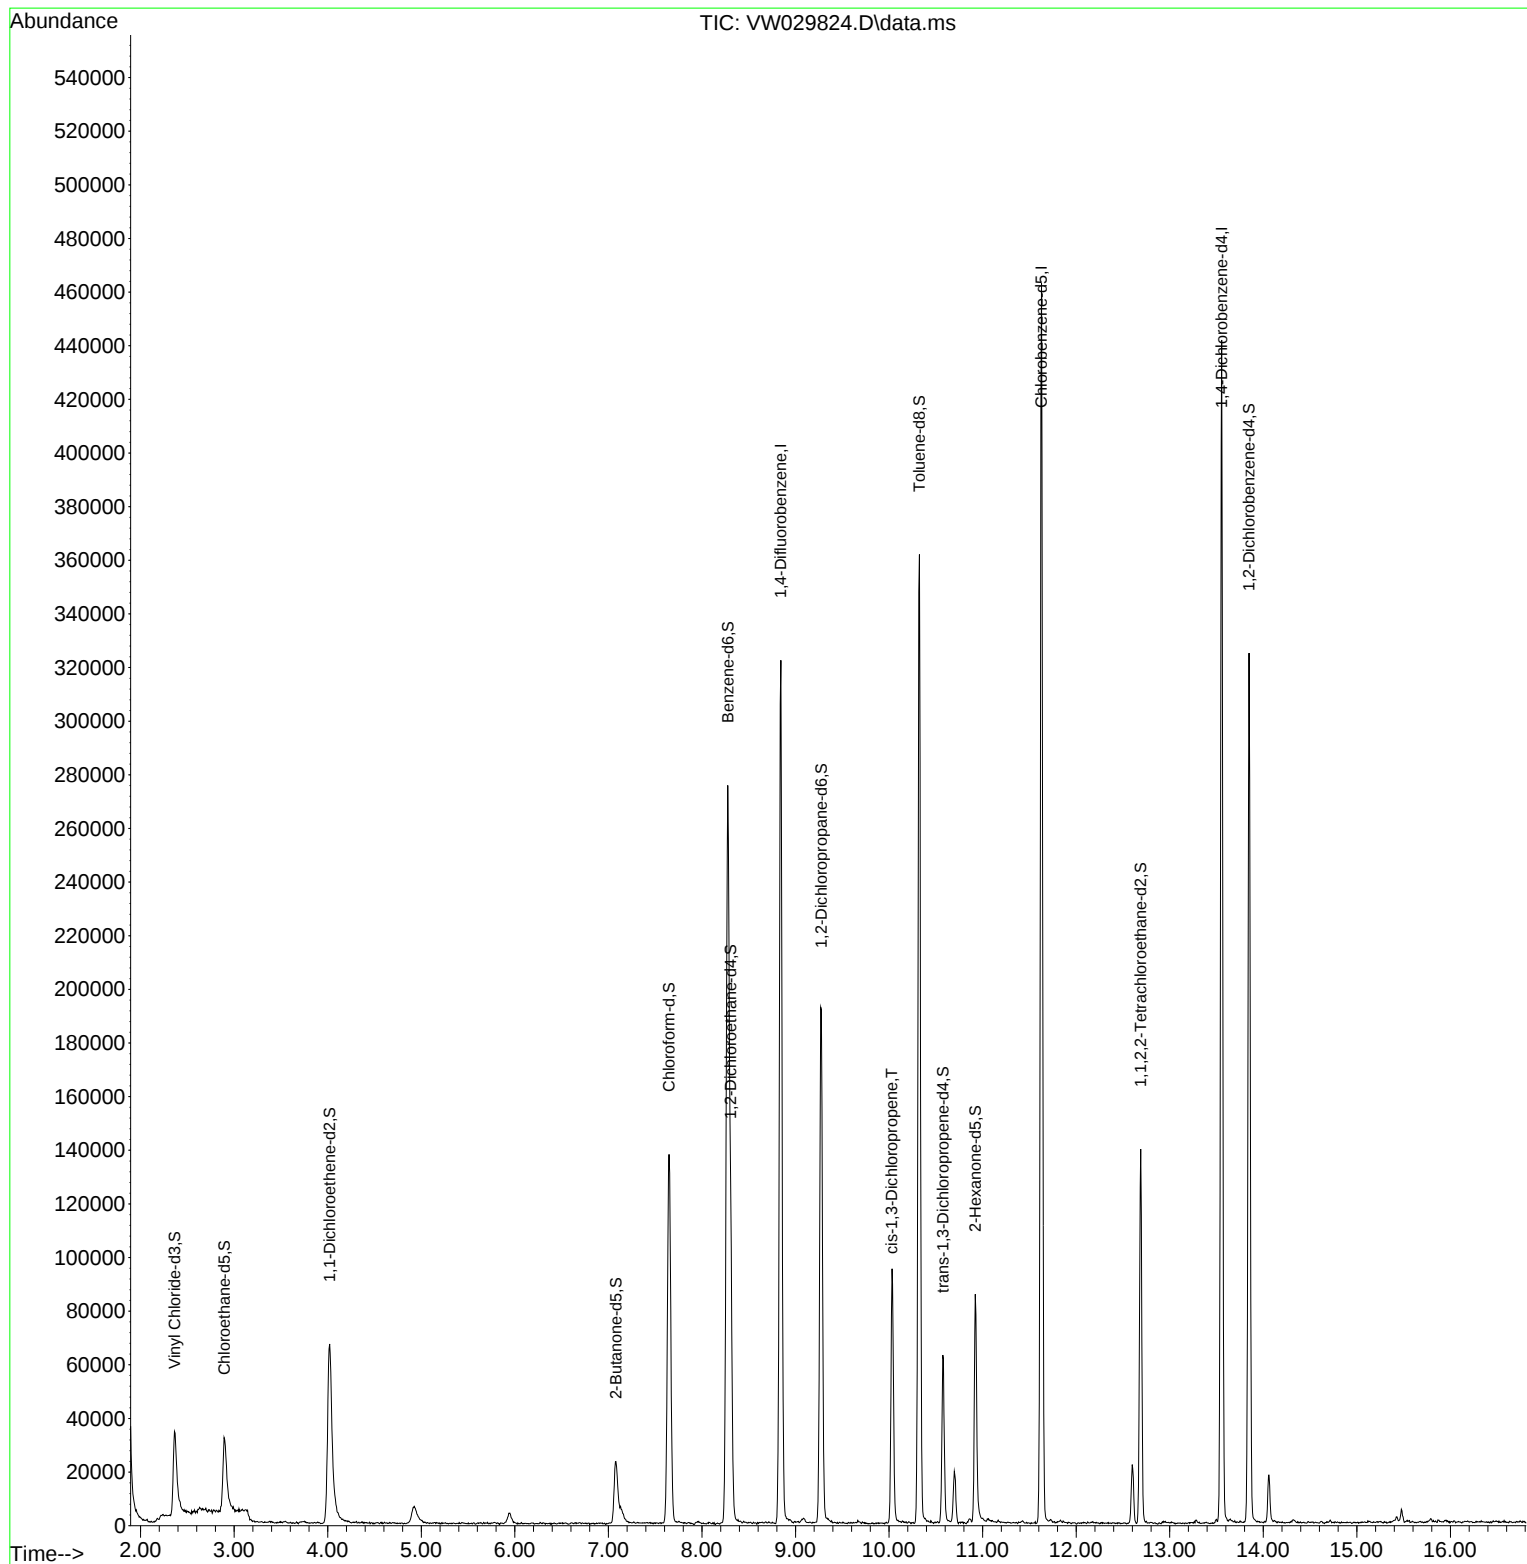

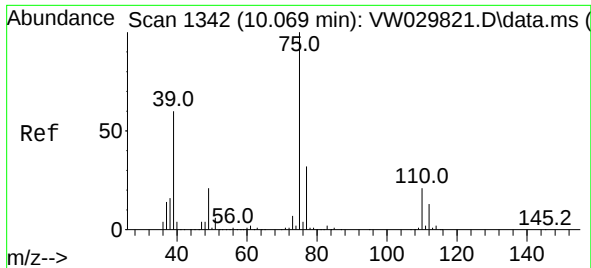

#39
 cis-1,3-Dichloropropene
 Concen: 0.403 ug/L
 RT: 10.026 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW029824.D
 Acq: 01 Aug 2024 11:25

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 2544
 Ion Ratio Lower Upper
 75 100
 77 37.7 20.8 38.6

