

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
 Data File : VW029825.D
 Acq On : 01 Aug 2024 11:50
 Operator : SY/MD
 Sample : P3328-20
 Misc : 11.53g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E20N1

Quant Time: Aug 02 01:46:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 02 01:45:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	231246	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	221374	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	101450	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	58446	17.803	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.200%		
7) Chloroethane-d5	2.893	69	47276	20.171	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.680%		
11) 1,1-Dichloroethene-d2	4.021	65	29194	19.481	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	77.920%		
21) 2-Butanone-d5	7.075	46	43618	48.475	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	96.960%		
24) Chloroform-d	7.648	84	148545	24.815	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	99.240%		
26) 1,2-Dichloroethane-d4	8.307	65	91602	26.866	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	107.480%		
32) Benzene-d6	8.270	84	280440	23.446	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	93.800%		
36) 1,2-Dichloropropane-d6	9.270	67	96748	25.331	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.320%		
41) Toluene-d8	10.325	98	246604	23.187	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	92.760%		
43) trans-1,3-Dichloroprop...	10.581	79	35284	22.831	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.320%		
47) 2-Hexanone-d5	10.922	63	29609	47.016	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.040%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	73444	25.898	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.600%		
66) 1,2-Dichlorobenzene-d4	13.848	152	80515	25.560	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	102.240%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	2869	0.474	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
Data File : VW029825.D
Acq On : 01 Aug 2024 11:50
Operator : SY/MD
Sample : P3328-20
Misc : 11.53g/10mL/MSVOA_W/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E20N1

Quant Time: Aug 02 01:46:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 02 01:45:39 2024
Response via : Initial Calibration

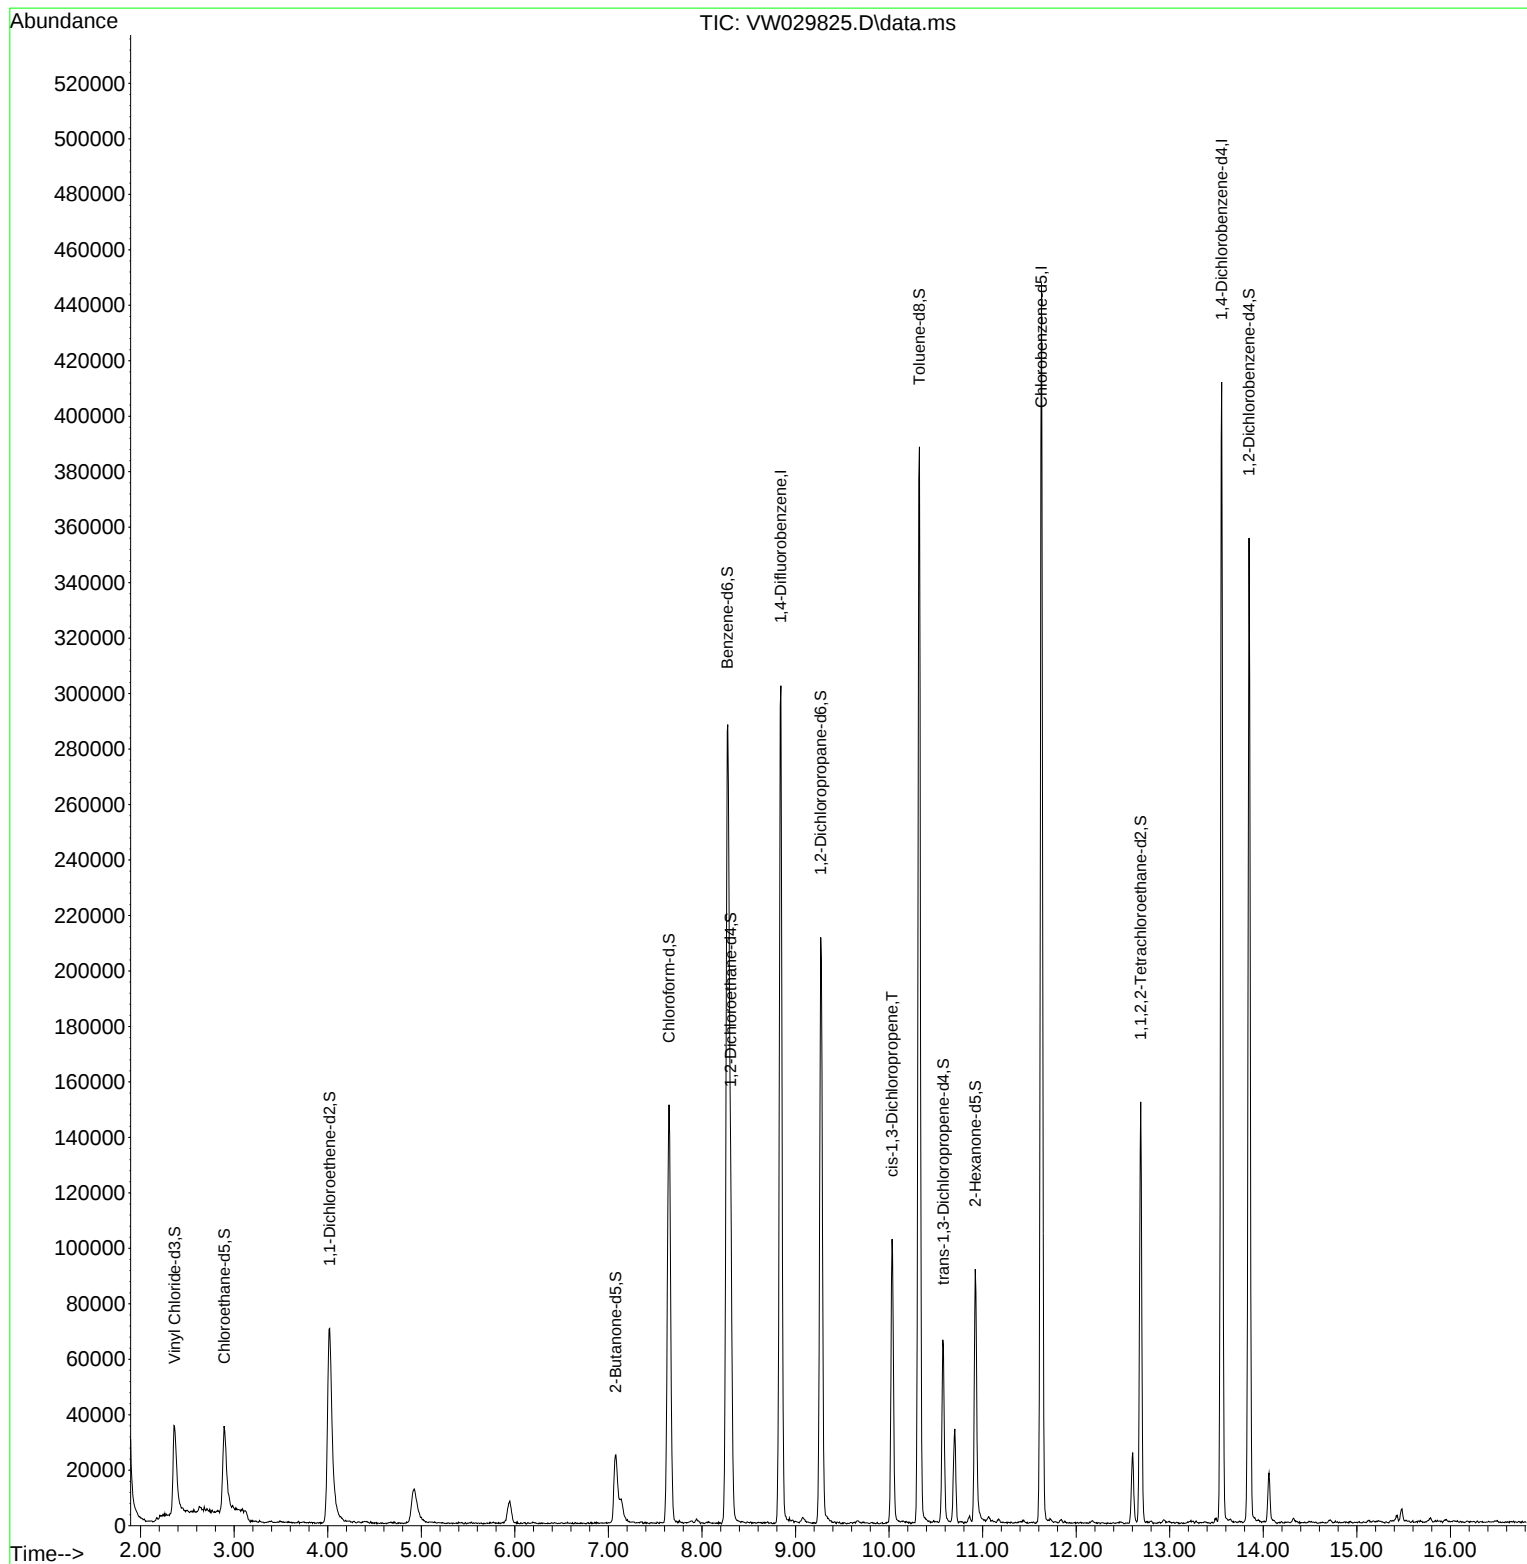

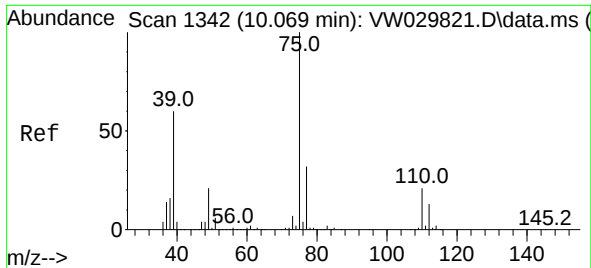

#39
 cis-1,3-Dichloropropene
 Concen: 0.474 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029825.D
 Acq: 01 Aug 2024 11:50

Instrument :
 MSVOA_W
 ClientSampleId :
 E20N1

Tgt Ion: 75 Resp: 2869
 Ion Ratio Lower Upper
 75 100
 77 46.7 20.8 38.6#

