

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
 Data File : VW029828.D
 Acq On : 01 Aug 2024 13:02
 Operator : SY/MD
 Sample : P3328-10
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Aug 02 01:47:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 02 01:45:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	230506	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	222412	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	99437	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	59391	18.149	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.600%		
7) Chloroethane-d5	2.893	69	50152	21.466	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.880%		
11) 1,1-Dichloroethene-d2	4.021	65	29116	19.491	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	77.960%		
21) 2-Butanone-d5	7.075	46	45508	50.738	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.480%		
24) Chloroform-d	7.648	84	153444	25.715	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	102.880%		
26) 1,2-Dichloroethane-d4	8.471	65	102	0.030	ug/L	0.17
Spiked Amount 25.000	Range 70 - 130		Recovery =	0.120%#		
32) Benzene-d6	8.276	84	282328	23.493	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	93.960%		
36) 1,2-Dichloropropane-d6	9.270	67	97020	25.284	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.120%		
41) Toluene-d8	10.325	98	249845	23.382	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.520%		
43) trans-1,3-Dichloroprop...	10.575	79	36803	23.702	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	94.800%		
47) 2-Hexanone-d5	10.922	63	30733	48.573	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	97.140%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	75456	26.483	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	105.920%		
66) 1,2-Dichlorobenzene-d4	13.848	152	81687	26.457	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	105.840%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	2806	0.461	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
Data File : VW029828.D
Acq On : 01 Aug 2024 13:02
Operator : SY/MD
Sample : P3328-10
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Aug 02 01:47:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 02 01:45:39 2024
Response via : Initial Calibration

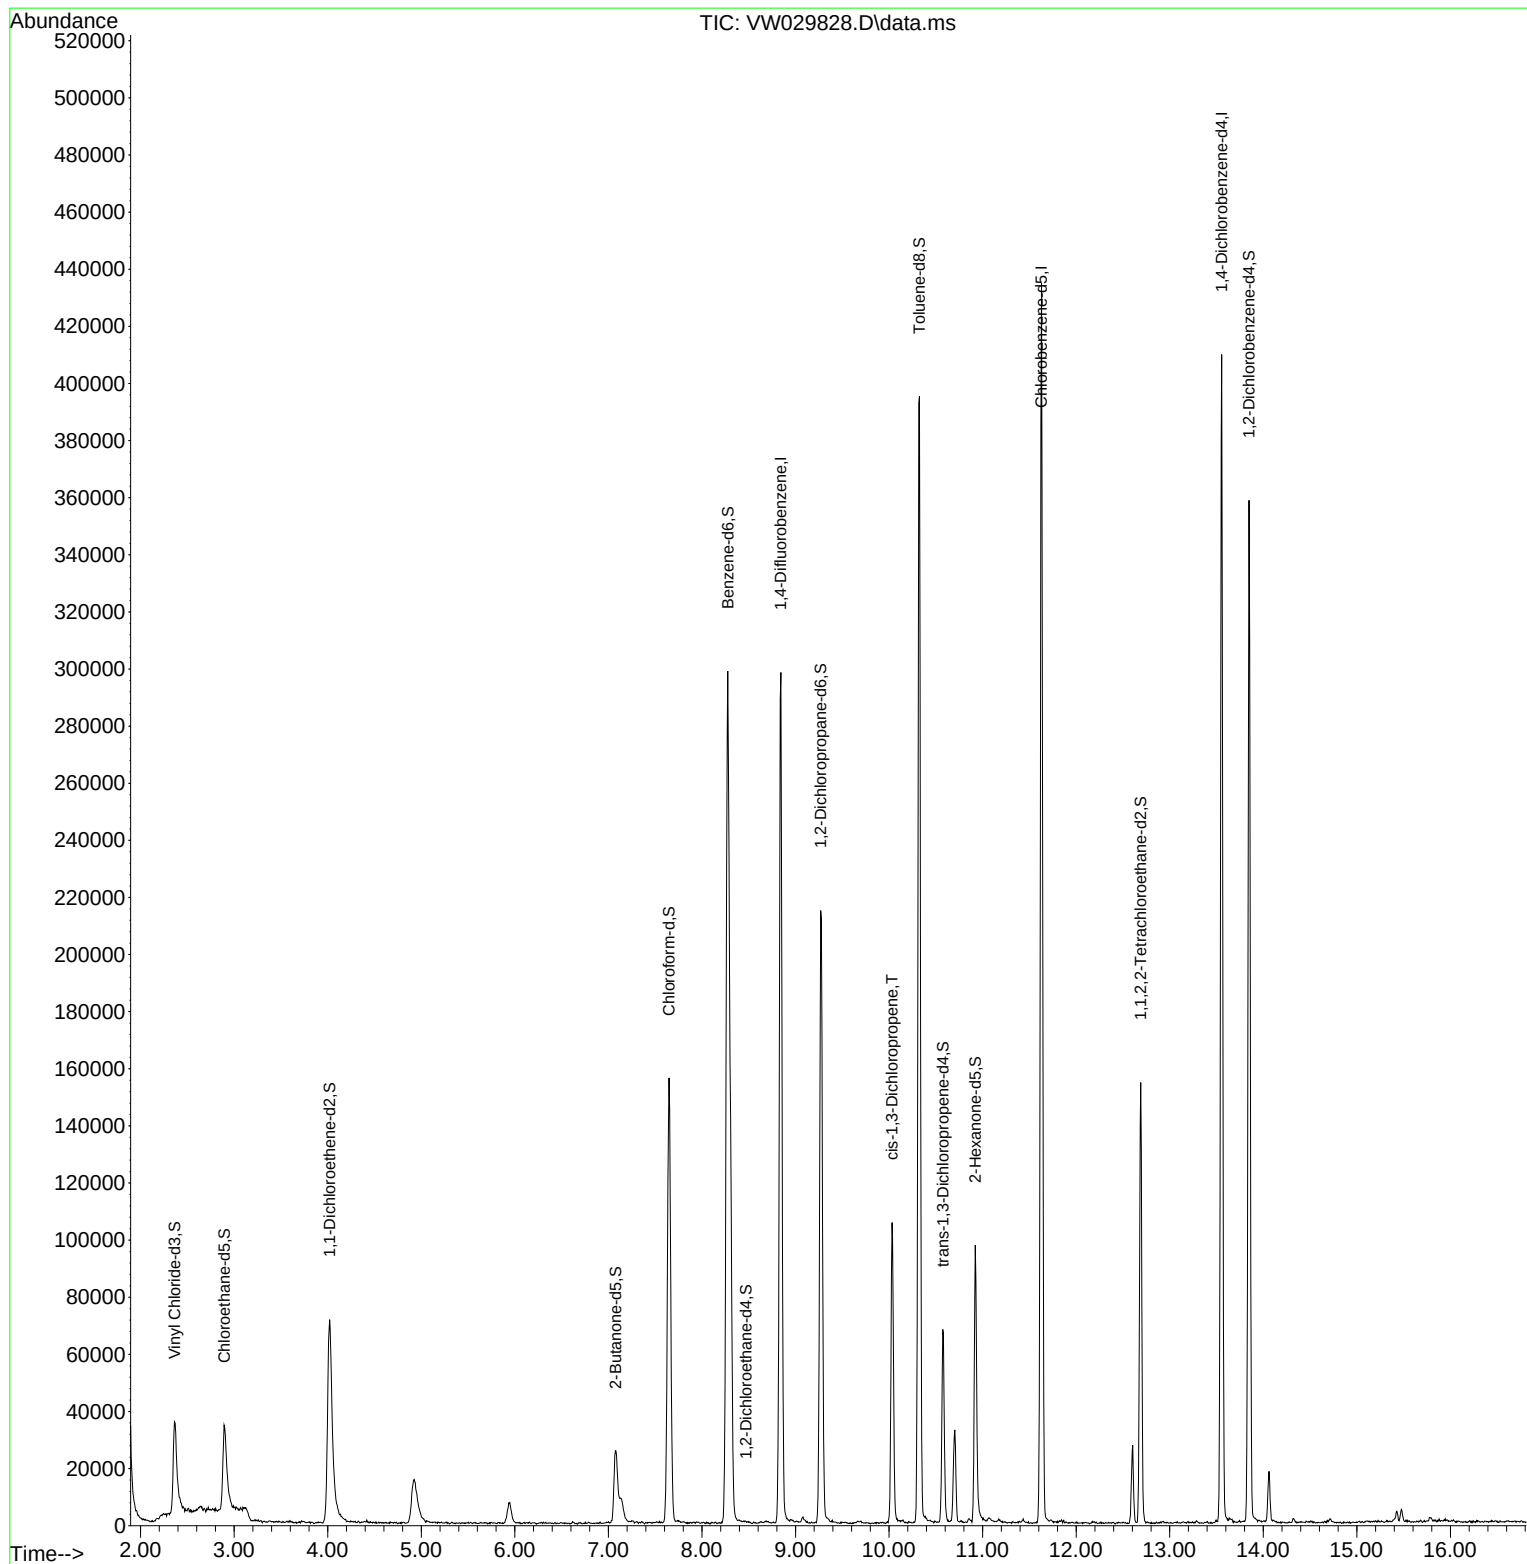

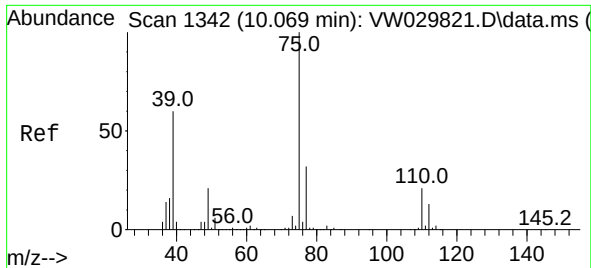

#39
 cis-1,3-Dichloropropene
 Concen: 0.461 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029828.D
 Acq: 01 Aug 2024 13:02

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 2806
 Ion Ratio Lower Upper
 75 100
 77 47.1 20.8 38.6#

