




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
Data File : VW029827.D
Acq On : 01 Aug 2024 12:38
Operator : SY/MD
Sample : P3397-09
Misc : 5.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/02/2024
Supervised By :Mahesh Dadoda 08/02/2024

Quant Time: Aug 02 01:47:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 02 01:45:39 2024
Response via : Initial Calibration

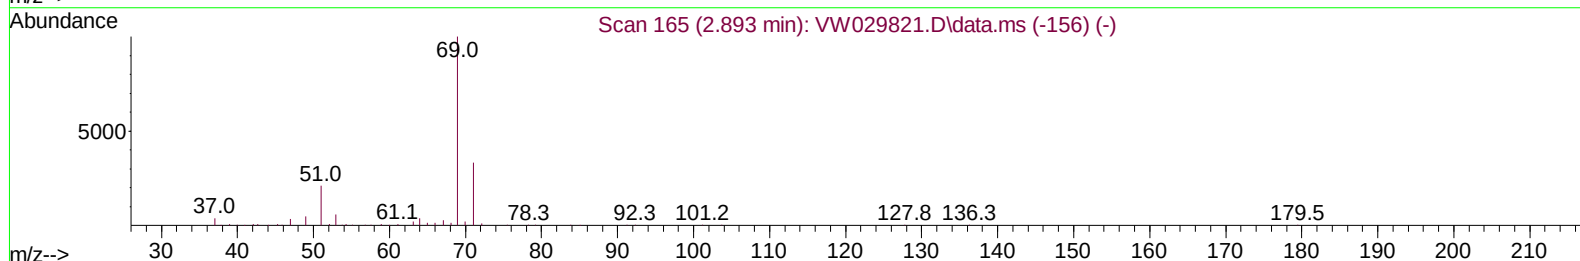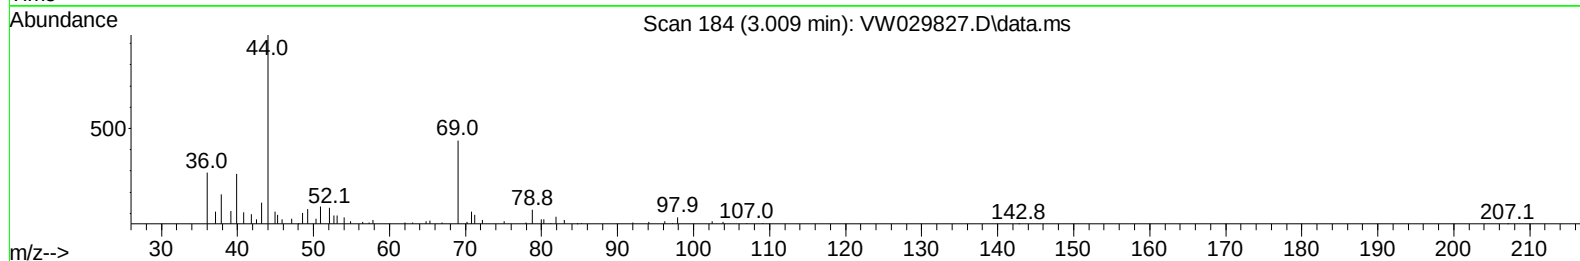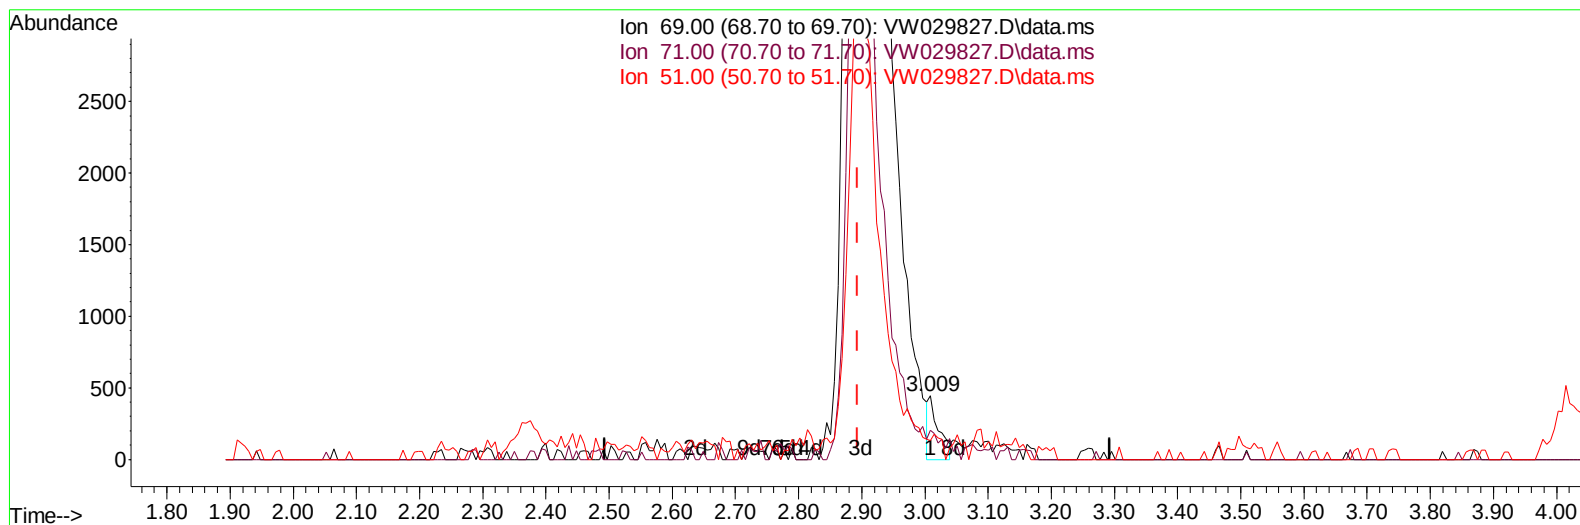

TIC: VW029827.D\data.ms

(7) Chloroethane-d5 (S)

3.009min (+ 0.116) 0.20 ug/L

response 495

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.70	35.56
51.00	31.60	34.75
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
 Data File : VW029827.D
 Acq On : 01 Aug 2024 12:38
 Operator : SY/MD
 Sample : P3397-09
 Misc : 5.04g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 02 01:47:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 02 01:45:39 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/02/2024
 Supervised By :Mahesh Dadoda 08/02/2024

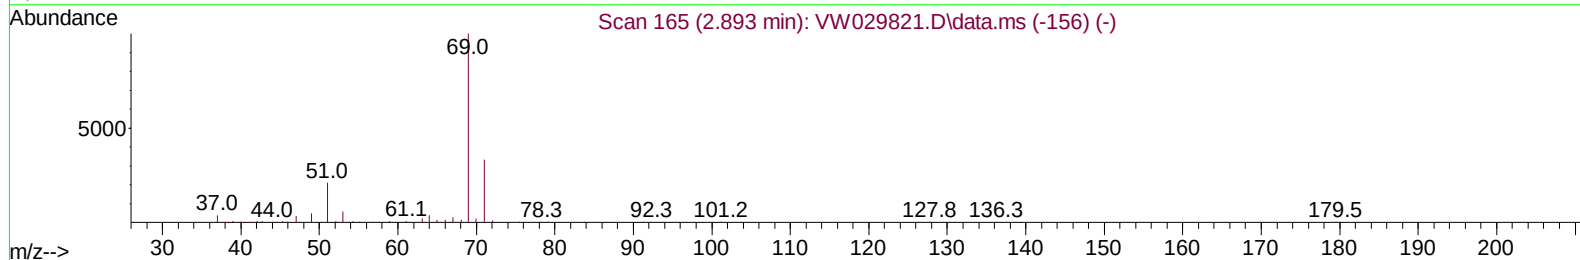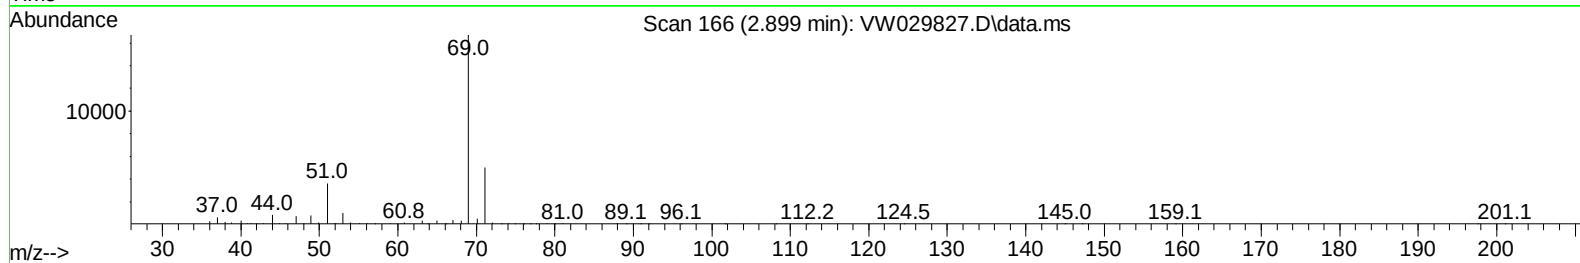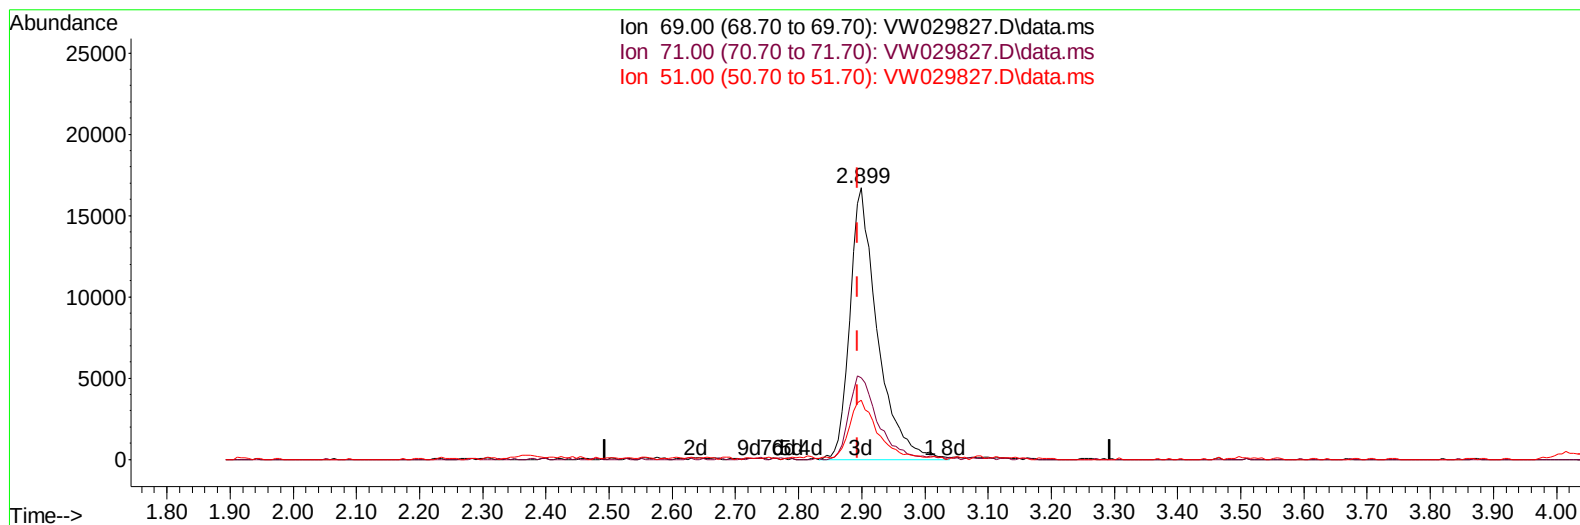

TIC: VW029827.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (+ 0.006) 20.79 ug/L m

response 50856

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.70	0.35#
51.00	31.60	0.34#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
 Data File : VW029827.D
 Acq On : 01 Aug 2024 12:38
 Operator : SY/MD
 Sample : P3397-09
 Misc : 5.04g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/02/2024
 Supervised By :Mahesh Dadoda 08/02/2024

Quant Time: Aug 02 01:47:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 02 01:45:39 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		241344	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		230456	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		100698	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		59588	17.391	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	69.560%		
7) Chloroethane-d5	2.899	69		50856m	20.790	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	83.160%		
11) 1,1-Dichloroethene-d2	4.021	65		29758	19.026	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	76.120%		
21) 2-Butanone-d5	7.075	46		46119	49.110	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	98.220%		
24) Chloroform-d	7.648	84		151591	24.264	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	97.040%		
26) 1,2-Dichloroethane-d4	8.307	65		92706	26.052	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	104.200%		
32) Benzene-d6	8.270	84		285092	22.895	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	91.600%		
36) 1,2-Dichloropropane-d6	9.270	67		96916	24.375	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	97.520%		
41) Toluene-d8	10.325	98		246023	22.221	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	88.880%		
43) trans-1,3-Dichloroprop...	10.575	79		36210	22.507	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	90.040%		
47) 2-Hexanone-d5	10.922	63		30454	46.452	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	92.900%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		75478	25.566	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	102.280%		
66) 1,2-Dichlorobenzene-d4	13.848	152		85778	27.434	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	109.720%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
Data File : VW029827.D
Acq On : 01 Aug 2024 12:38
Operator : SY/MD
Sample : P3397-09
Misc : 5.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/02/2024
Supervised By :Mahesh Dadoda 08/02/2024

Quant Time: Aug 02 01:47:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 02 01:45:39 2024
Response via : Initial Calibration

