




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
 Data File : VW029828.D
 Acq On : 01 Aug 2024 13:02
 Operator : SY/MD
 Sample : P3328-10
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 02 02:21:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 02 01:45:39 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/02/2024
 Supervised By :Mahesh Dadoda 08/02/2024

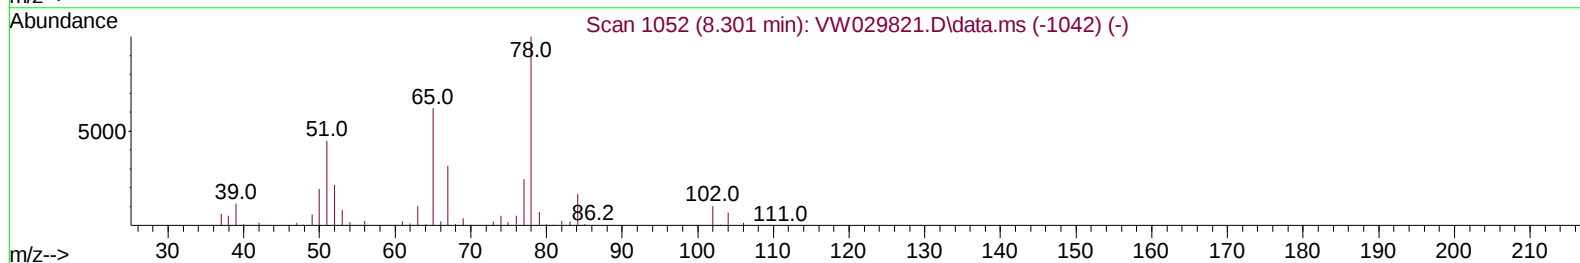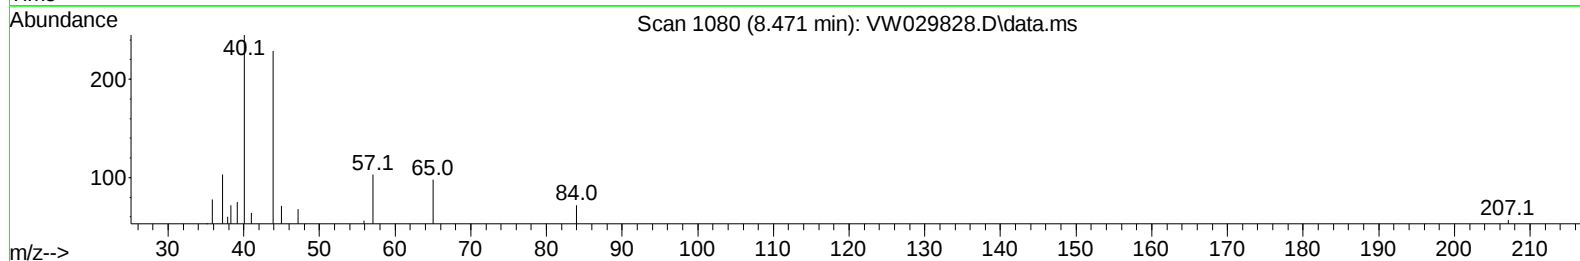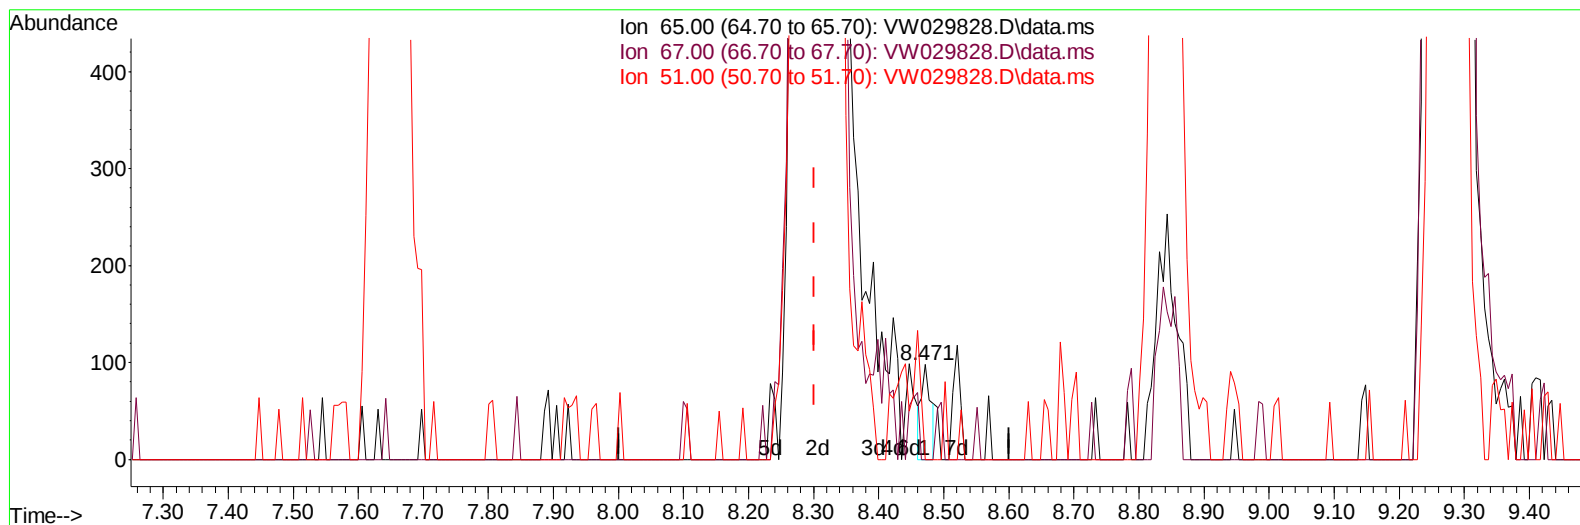

TIC: VW029828.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.471min (+ 0.171) 0.03 ug/L

response 102

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	66.67
51.00	120.50	94.12
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
 Data File : VW029828.D
 Acq On : 01 Aug 2024 13:02
 Operator : SY/MD
 Sample : P3328-10
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 02 01:47:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 02 01:45:39 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/02/2024
 Supervised By :Mahesh Dadoda 08/02/2024

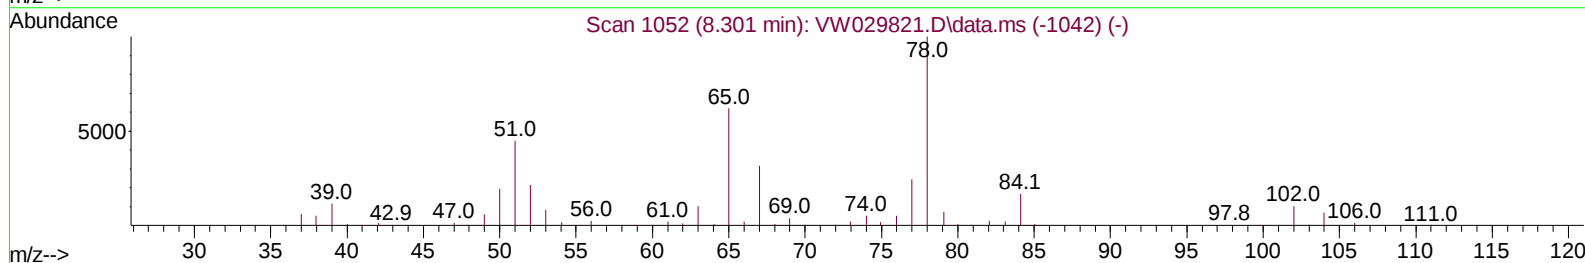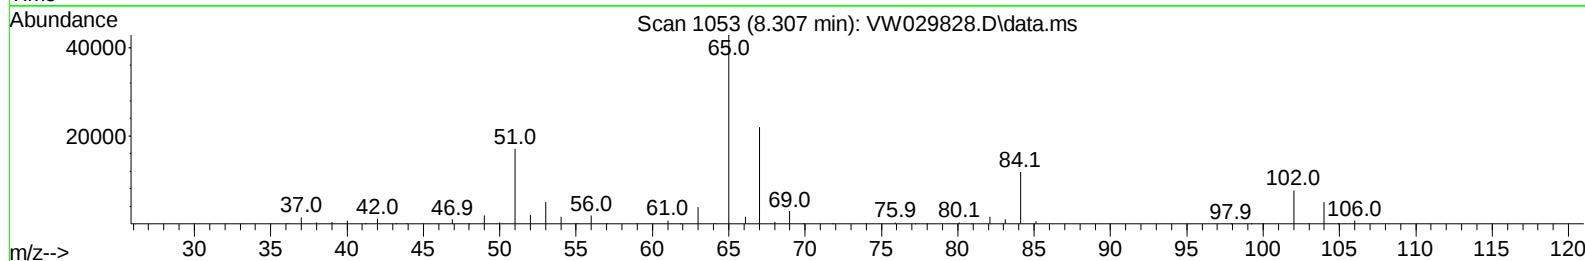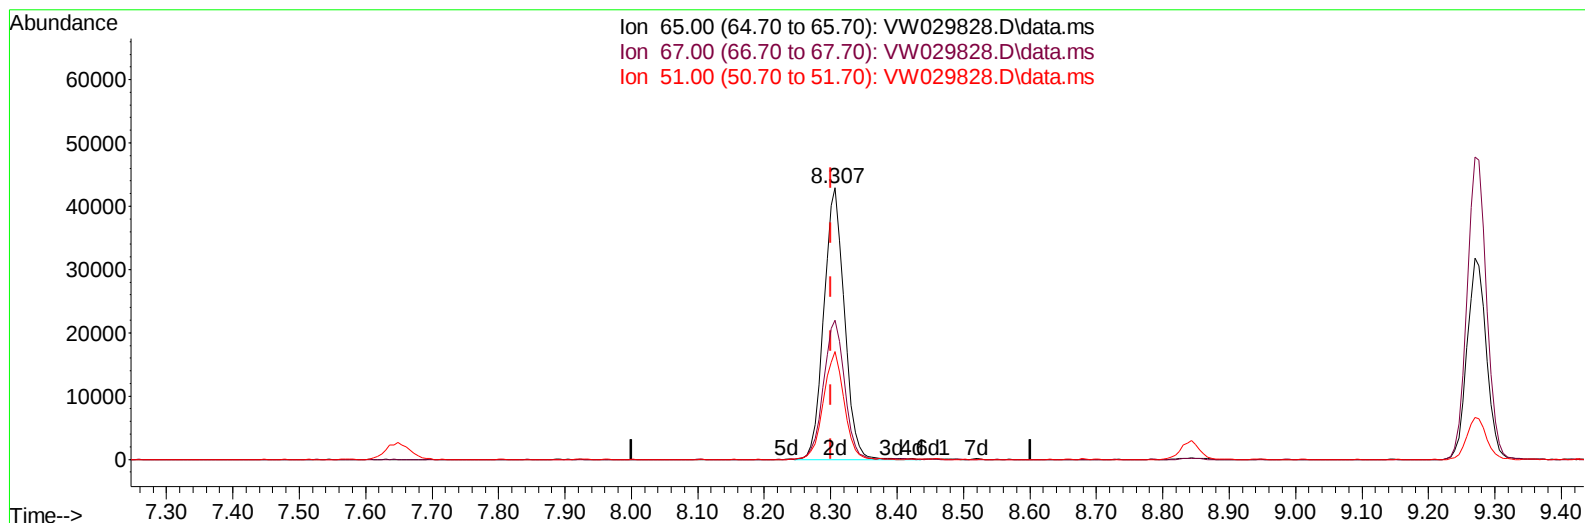

TIC: VW029828.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 27.17 ug/L m

response 92352

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.07#
51.00	120.50	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
 Data File : VW029828.D
 Acq On : 01 Aug 2024 13:02
 Operator : SY/MD
 Sample : P3328-10
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/02/2024
 Supervised By :Mahesh Dadoda 08/02/2024

Quant Time: Aug 02 01:47:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 02 01:45:39 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		230506	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		222412	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		99437	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		59391	18.149	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	72.600%		
7) Chloroethane-d5	2.893	69		50152	21.466	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	85.880%		
11) 1,1-Dichloroethene-d2	4.021	65		29116	19.491	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	77.960%		
21) 2-Butanone-d5	7.075	46		45508	50.738	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	101.480%		
24) Chloroform-d	7.648	84		153444	25.715	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	102.880%		
26) 1,2-Dichloroethane-d4	8.307	65		92352m	27.173	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	108.680%		
32) Benzene-d6	8.276	84		282328	23.493	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	93.960%		
36) 1,2-Dichloropropane-d6	9.270	67		97020	25.284	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	101.120%		
41) Toluene-d8	10.325	98		249845	23.382	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	93.520%		
43) trans-1,3-Dichloroprop...	10.575	79		36803	23.702	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	94.800%		
47) 2-Hexanone-d5	10.922	63		30733	48.573	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	97.140%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		75456	26.483	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	105.920%		
66) 1,2-Dichlorobenzene-d4	13.848	152		81687	26.457	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	105.840%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080124\
Data File : VW029828.D
Acq On : 01 Aug 2024 13:02
Operator : SY/MD
Sample : P3328-10
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 02 01:47:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 02 01:45:39 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 08/02/2024
Supervised By :Mahesh Dadoda 08/02/2024

