

Data File : VW011613.D
Acq On : 02 Aug 2019 10:56
Operator : SY/VA
Sample : K4116-03RE
Misc : 4.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JLLD2

Quant Time: Aug 03 02:25:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 03 02:22:50 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	334883	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	271351	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	96758	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.34	65	103948	22.04	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.16%
7) Chloroethane-d5	2.88	69	79170	23.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.24%
10) 1,1-Dichloroethene-d2	4.01	63	187021	17.30	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.20%
20) 2-Butanone-d5	7.09	46	71200	33.53	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	67.06%
24) Chloroform-d	7.65	84	218149	23.72	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.88%
26) 1,2-Dichloroethane-d4	8.30	65	125777	23.11	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.44%
29) Benzene-d6	8.27	84	447688	26.24	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.96%
33) 1,2-Dichloropropane-d6	9.27	67	145808	26.47	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.88%
37) Toluene-d8	10.32	98	374371	24.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.88%
38) trans-1,3-Dichloropropene-	10.58	79	52840	21.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.56%
39) 2-Hexanone-d5	10.93	63	48010	37.31	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.62%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	90510	19.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.16%
61) 1,2-Dichlorobenzene-d4	13.85	152	86402	23.17	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.68%


Target Compounds						Qvalue
59) 1,2,3-Trichloropropane	13.55	75	13288	3.746	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW011613.D
Acq On : 02 Aug 2019 10:56
Operator : SY/VA
Sample : K4116-03RE
Misc : 4.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JLLD2

Quant Time: Aug 03 02:25:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM073019S.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 03 02:22:50 2019
Response via : Initial Calibration

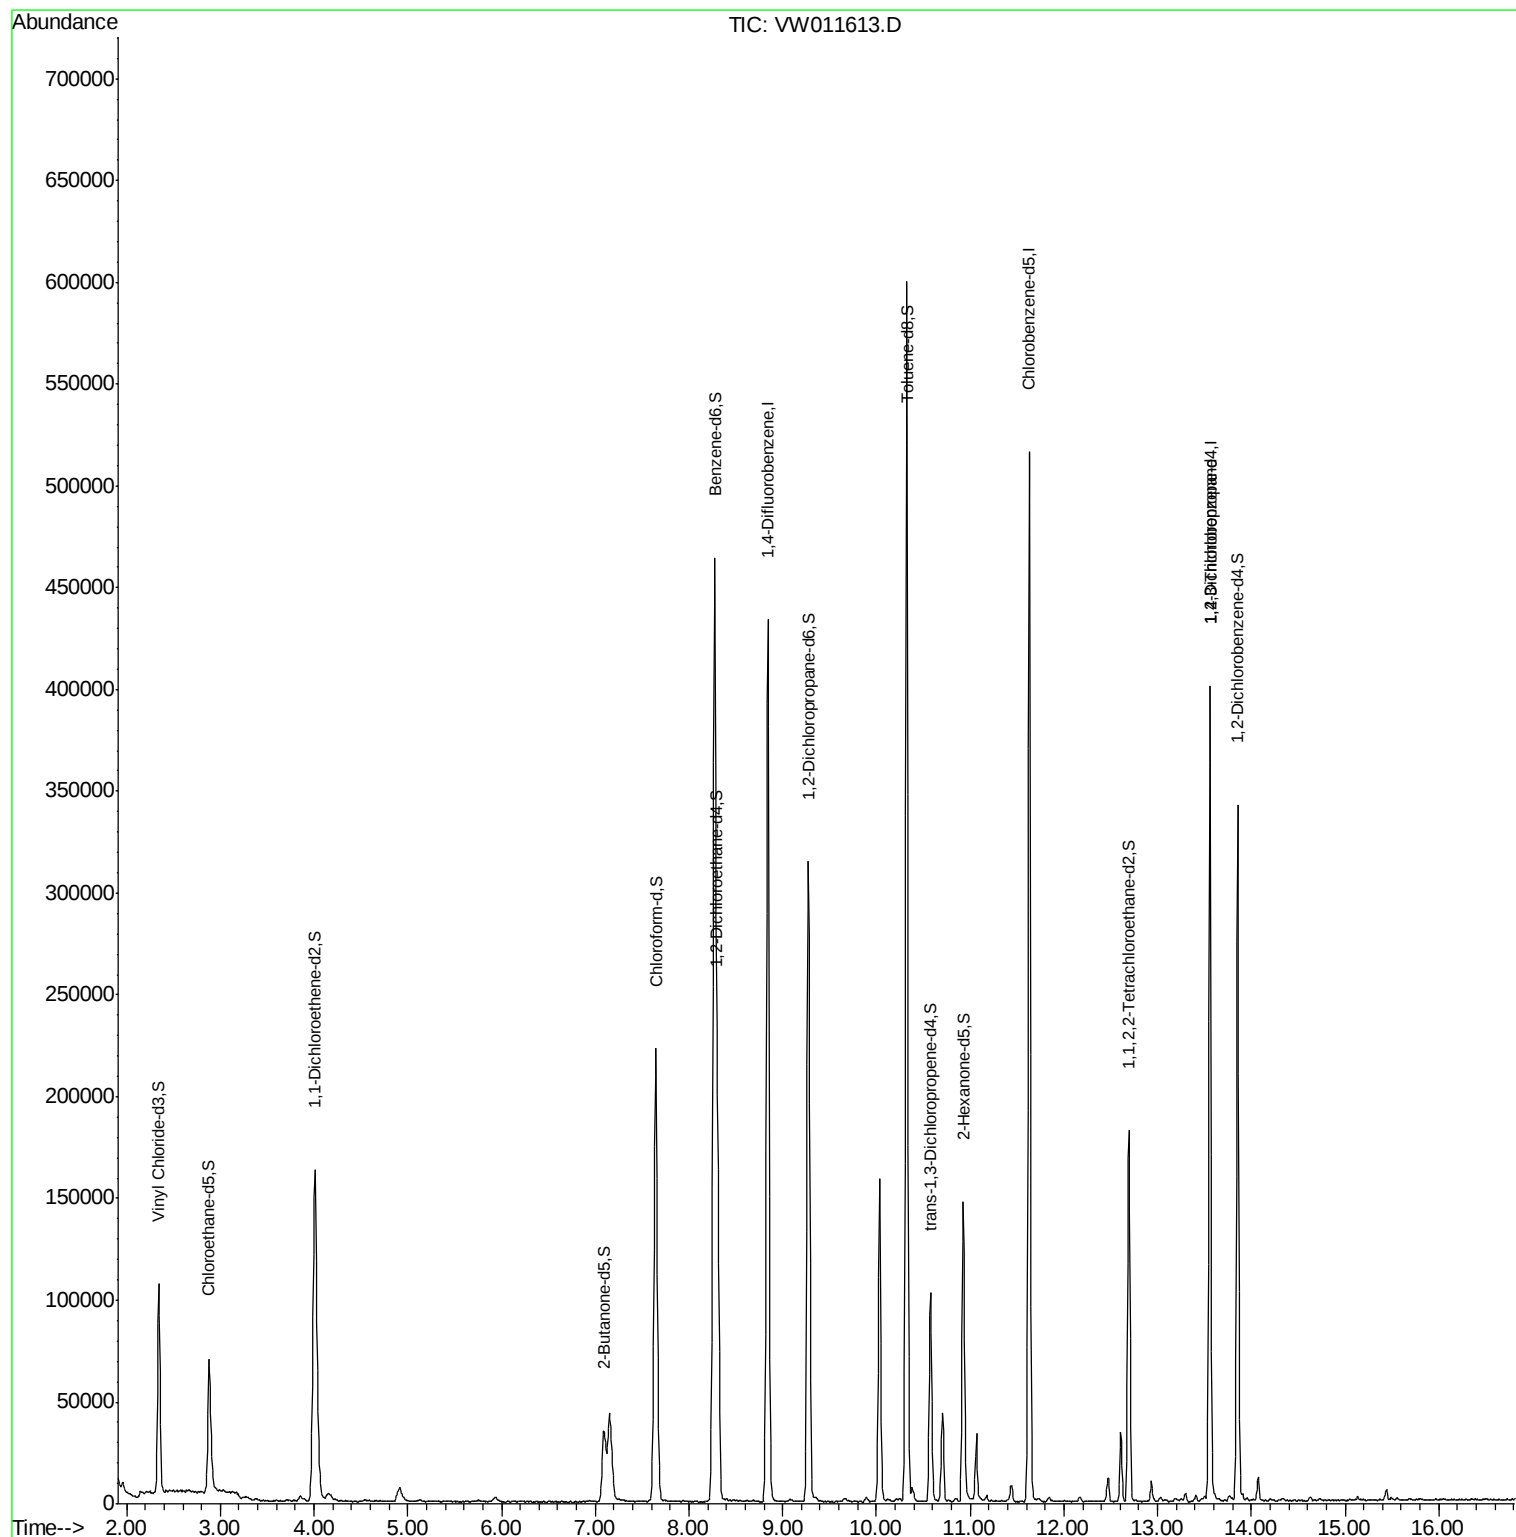

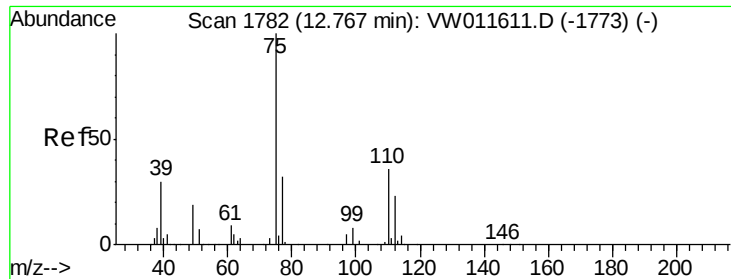

#59

1,2,3-Trichloropropane

Concen: 3.746 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW011613.D

Acq: 02 Aug 2019 10:56

Instrument :

MSVOA_W

ClientSampleId :

JLLD2

Tgt Ion: 75 Resp: 13288

Ion Ratio Lower Upper

75 100

77 35.9 25.1 37.7

